

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
 Data File : BF127388.D
 Acq On : 17 Mar 2022 21:08
 Operator : CG\JU
 Sample : N1981-01 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-3-031622

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.487	541	544	557	rBV	317213	322810	14.68%	1.231%
2	6.498	713	716	731	rBV	310646	337108	15.33%	1.286%
3	6.869	775	779	784	rBV	580891	500956	22.78%	1.911%
4	7.428	871	874	881	rBV	230501	223836	10.18%	0.854%
5	7.816	933	940	945	rVB4	52652	61974	2.82%	0.236%
6	7.886	948	952	957	rVV2	159704	223045	10.14%	0.851%
7	7.933	957	960	967	rVB	90165	138659	6.30%	0.529%
8	8.151	993	997	999	rVV	738662	651476	29.62%	2.485%
9	8.175	999	1001	1004	rVV	747586	592471	26.94%	2.260%
10	8.863	1115	1118	1122	rBV	436049	338880	15.41%	1.293%
11	8.963	1130	1135	1141	rVB	342094	266903	12.14%	1.018%
12	9.222	1176	1179	1183	rVB	406338	320212	14.56%	1.222%
13	9.328	1194	1197	1202	rBV	85027	71225	3.24%	0.272%
14	9.422	1211	1213	1218	rVB	56015	59951	2.73%	0.229%
15	9.486	1220	1224	1229	rBV	100893	142689	6.49%	0.544%
16	9.563	1234	1237	1240	rBV	170236	169401	7.70%	0.646%
17	9.592	1240	1242	1247	rVB	107895	94482	4.30%	0.360%
18	9.680	1253	1257	1262	rBV	81032	90849	4.13%	0.347%
19	9.769	1266	1272	1277	rBV2	88357	87959	4.00%	0.336%
20	9.886	1289	1292	1293	rBV	61210	47076	2.14%	0.180%
21	9.910	1293	1296	1298	rVV	690991	563081	25.60%	2.148%
22	9.939	1298	1301	1305	rVB	626231	512705	23.31%	1.956%
23	10.010	1310	1313	1317	rVB3	30247	43455	1.98%	0.166%
24	10.063	1317	1322	1324	rBV2	43186	51270	2.33%	0.196%
25	10.116	1327	1331	1334	rVV	296812	295884	13.45%	1.129%
26	10.145	1334	1336	1340	rVB	55481	51410	2.34%	0.196%
27	10.222	1345	1349	1352	rBV2	47072	53258	2.42%	0.203%
28	10.316	1360	1365	1366	rBV2	36098	48618	2.21%	0.185%
29	10.457	1385	1389	1395	rVB	658427	544945	24.78%	2.079%
30	10.522	1398	1400	1402	rVV	74292	73297	3.33%	0.280%
31	10.545	1402	1404	1406	rVV2	98993	85033	3.87%	0.324%
32	10.616	1413	1416	1419	rVV	94258	91282	4.15%	0.348%
33	10.698	1423	1430	1434	rVB3	267445	298756	13.58%	1.140%
34	10.816	1445	1450	1457	rVB5	37121	75557	3.44%	0.288%
35	11.004	1475	1482	1485	rBV2	114285	150326	6.84%	0.573%
36	11.033	1485	1487	1490	rVV2	71063	66153	3.01%	0.252%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
 Data File : BF127388.D
 Acq On : 17 Mar 2022 21:08
 Operator : CG\JU
 Sample : N1981-01 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-3-031622

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.086	1493	1496	1499	rVB3	52931	53847	2.45%	0.205%
38	11.133	1499	1504	1506	rBV3	40839	71021	3.23%	0.271%
39	11.157	1506	1508	1513	rVV	51732	60503	2.75%	0.231%
40	11.245	1520	1523	1527	rVV3	57924	75460	3.43%	0.288%
41	11.298	1529	1532	1537	rVB	178422	155463	7.07%	0.593%
42	11.404	1546	1550	1552	rBV	638246	668079	30.38%	2.549%
43	11.427	1552	1554	1558	rVV	2205031	1967946	89.48%	7.507%
44	11.480	1558	1563	1566	rVV	727843	666975	30.33%	2.544%
45	11.510	1566	1568	1574	rVV	80374	92560	4.21%	0.353%
46	11.633	1584	1589	1594	rVV	353941	364229	16.56%	1.389%
47	11.692	1597	1599	1604	rVV3	43895	58492	2.66%	0.223%
48	11.733	1604	1606	1611	rVB2	44506	51245	2.33%	0.195%
49	11.904	1631	1635	1637	rBV	283451	237933	10.82%	0.908%
50	11.933	1637	1640	1643	rVB	399541	335378	15.25%	1.279%
51	11.980	1643	1648	1651	rBV	158802	156820	7.13%	0.598%
52	12.016	1651	1654	1657	rVV	540236	580692	26.40%	2.215%
53	12.039	1657	1658	1663	rVB	184714	102724	4.67%	0.392%
54	12.086	1663	1666	1668	rBV	59373	57167	2.60%	0.218%
55	12.198	1682	1685	1688	rVV	193470	147703	6.72%	0.563%
56	12.227	1688	1690	1694	rVB	61869	54504	2.48%	0.208%
57	12.345	1705	1710	1713	rBV4	59273	62066	2.82%	0.237%
58	12.374	1713	1715	1718	rVV	55043	48348	2.20%	0.184%
59	12.451	1724	1728	1731	rBV	119863	141763	6.45%	0.541%
60	12.492	1732	1735	1737	rVV3	85556	98588	4.48%	0.376%
61	12.545	1740	1744	1748	rBV4	64136	97650	4.44%	0.373%
62	12.621	1753	1757	1761	rBV	2177718	2199232	100.00%	8.390%
63	12.680	1765	1767	1770	rVB	59998	49182	2.24%	0.188%
64	12.768	1779	1782	1785	rBV2	74288	73050	3.32%	0.279%
65	12.851	1789	1796	1801	rBV2	1650268	2176497	98.97%	8.303%
66	12.898	1801	1804	1808	rVB2	106373	109881	5.00%	0.419%
67	12.968	1812	1816	1817	rBV	139777	151463	6.89%	0.578%
68	12.980	1817	1818	1821	rVV	308411	254514	11.57%	0.971%
69	13.010	1821	1823	1826	rVB	106397	96343	4.38%	0.368%
70	13.057	1828	1831	1836	rBV3	127481	221159	10.06%	0.844%
71	13.104	1836	1839	1844	rBV	62855	66949	3.04%	0.255%
72	13.151	1844	1847	1848	rBV2	124530	119603	5.44%	0.456%
73	13.174	1848	1851	1854	rVB	406164	414701	18.86%	1.582%
74	13.245	1859	1863	1865	rBV	432907	394982	17.96%	1.507%
75	13.280	1865	1869	1871	rVV2	182852	227582	10.35%	0.868%
76	13.304	1871	1873	1876	rVV	101305	98510	4.48%	0.376%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
 Data File : BF127388.D
 Acq On : 17 Mar 2022 21:08
 Operator : CG\JU
 Sample : N1981-01 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-3-031622

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	13.333	1876	1878	1881	rVV2	55660	52912	2.41%	0.202%
78	13.374	1882	1885	1887	rVV	90768	82235	3.74%	0.314%
79	13.404	1887	1890	1898	rVB2	102519	140706	6.40%	0.537%
80	13.574	1917	1919	1921	rVV3	54749	52281	2.38%	0.199%
81	13.598	1921	1923	1926	rVV	69290	67702	3.08%	0.258%
82	13.657	1930	1933	1936	rBV	75976	93252	4.24%	0.356%
83	13.686	1936	1938	1942	rVB	69759	69873	3.18%	0.267%
84	13.798	1954	1957	1959	rBV	126343	108709	4.94%	0.415%
85	13.821	1959	1961	1964	rVV	134441	107449	4.89%	0.410%
86	13.851	1964	1966	1972	rVV3	87894	144668	6.58%	0.552%
87	14.045	1992	1999	2002	rBV2	908640	1384725	62.96%	5.282%
88	14.074	2002	2004	2011	rVB	640509	630522	28.67%	2.405%
89	14.157	2015	2018	2020	rVB	161738	123587	5.62%	0.471%
90	14.245	2031	2033	2035	rBV	59171	45901	2.09%	0.175%
91	14.280	2037	2039	2042	rVB	78099	62680	2.85%	0.239%
92	14.398	2057	2059	2061	rBV	67906	62711	2.85%	0.239%
93	14.433	2063	2065	2068	rVB	144069	140157	6.37%	0.535%
94	14.580	2089	2090	2093	rVB	97128	75469	3.43%	0.288%
95	15.104	2175	2179	2182	rBV	421426	639362	29.07%	2.439%
96	15.215	2195	2198	2201	rBV	104477	111164	5.05%	0.424%
97	15.415	2228	2232	2238	rVB	216150	293942	13.37%	1.121%
98	15.480	2239	2243	2248	rBV	371715	455848	20.73%	1.739%
99	15.539	2250	2253	2256	rBV	205397	237484	10.80%	0.906%
100	17.051	2507	2510	2521	rVB2	115502	222744	10.13%	0.850%


Sum of corrected areas: 26213879

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127388.D
Acq On : 17 Mar 2022 21:08
Operator : CG\JU
Sample : N1981-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-3-031622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

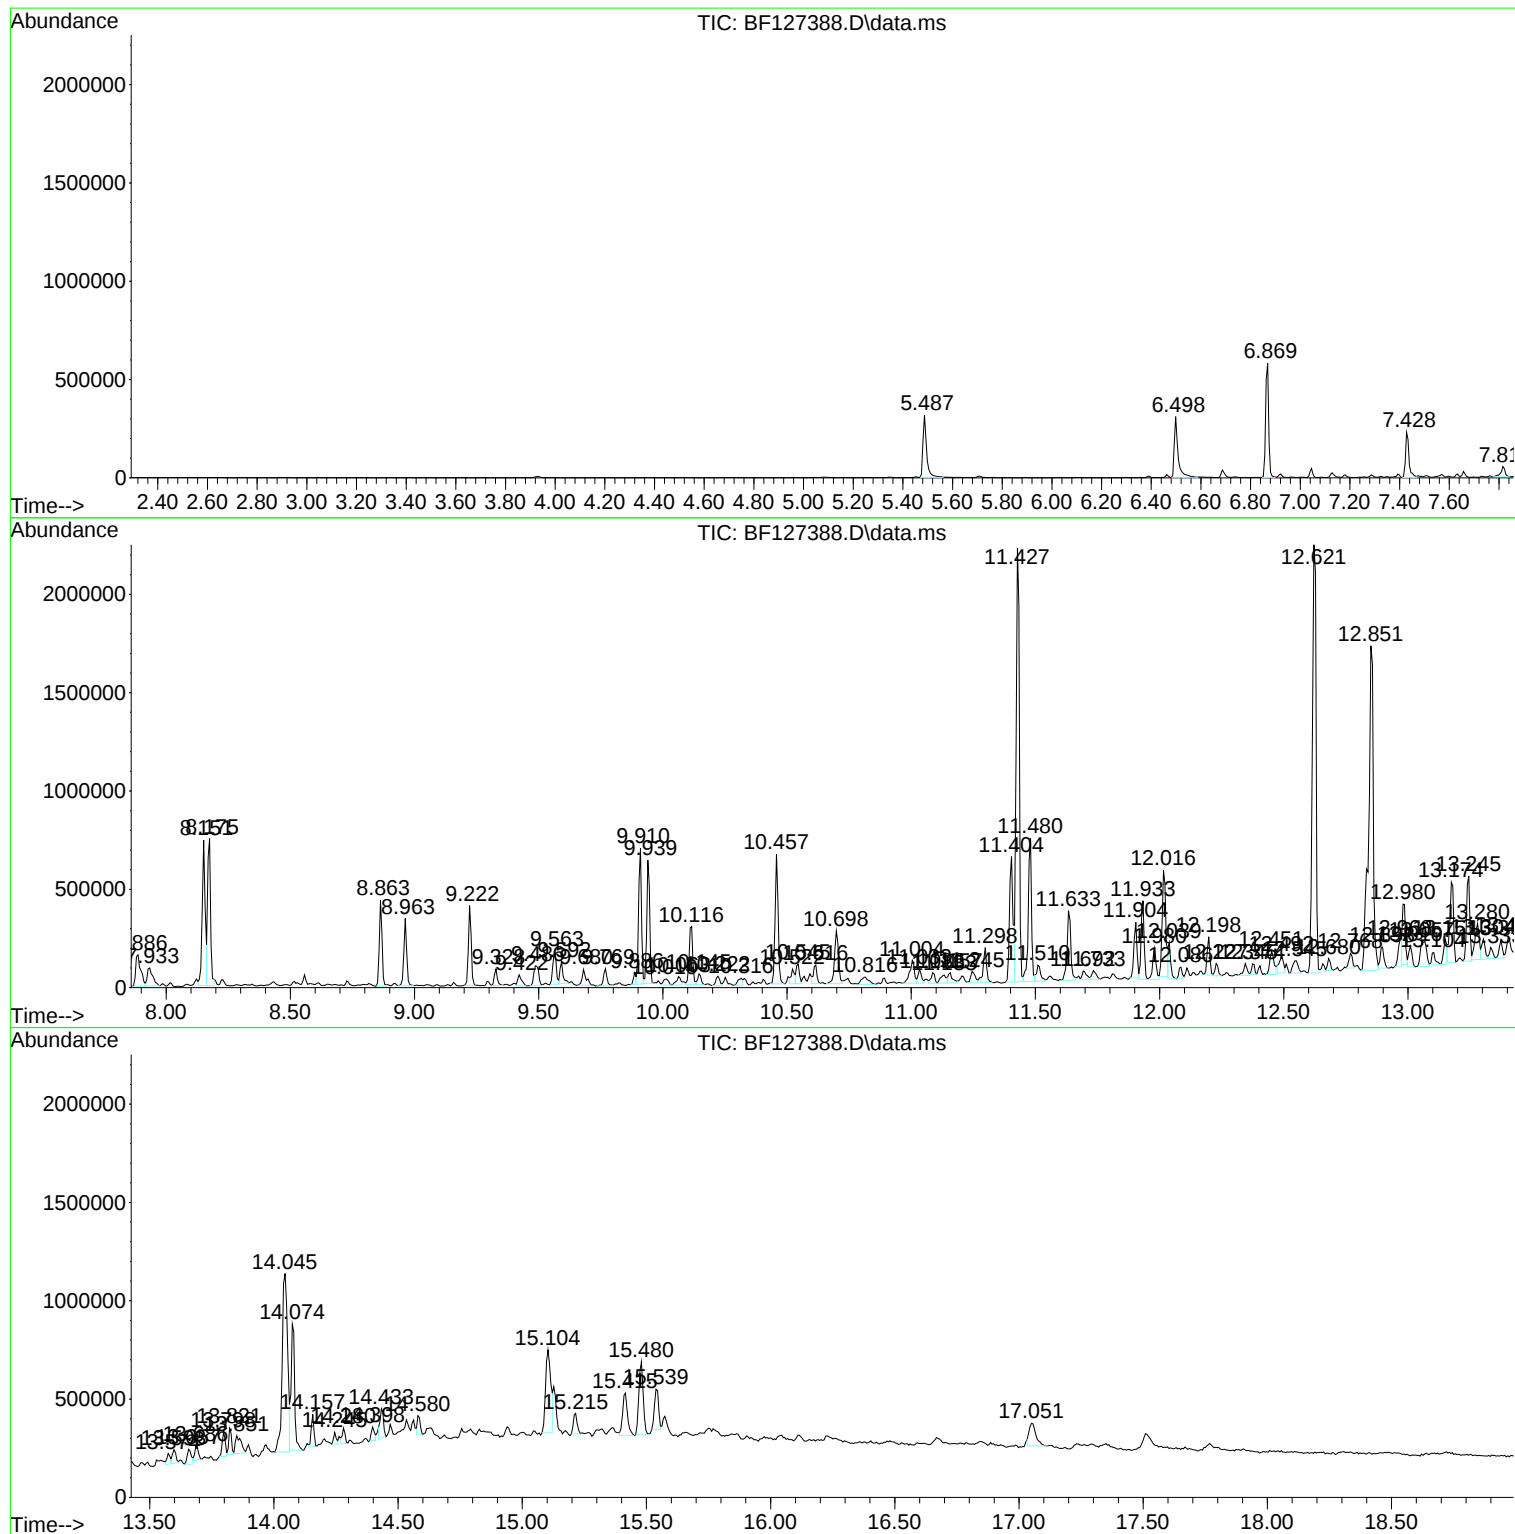

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127388.D
Acq On : 17 Mar 2022 21:08
Operator : CG\JU
Sample : N1981-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-3-031622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031722\
Data File : BF127388.D
Acq On : 17 Mar 2022 21:08
Operator : CG\JU
Sample : N1981-01 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-3-031622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------