
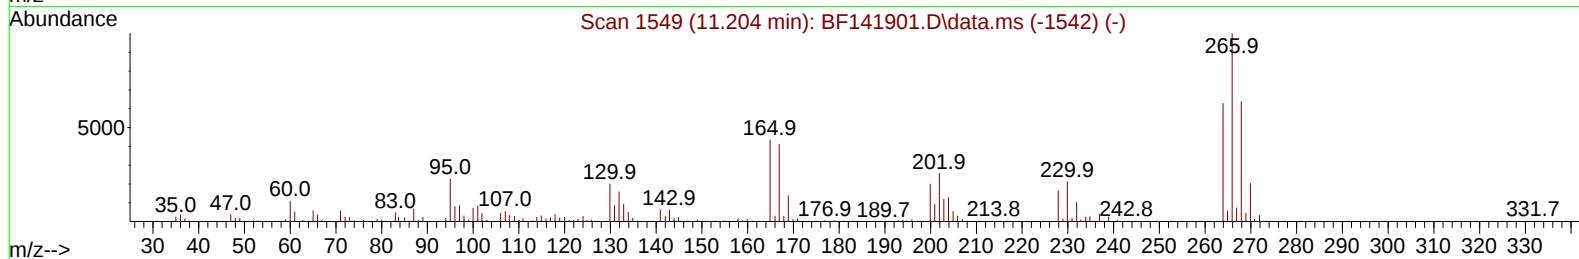
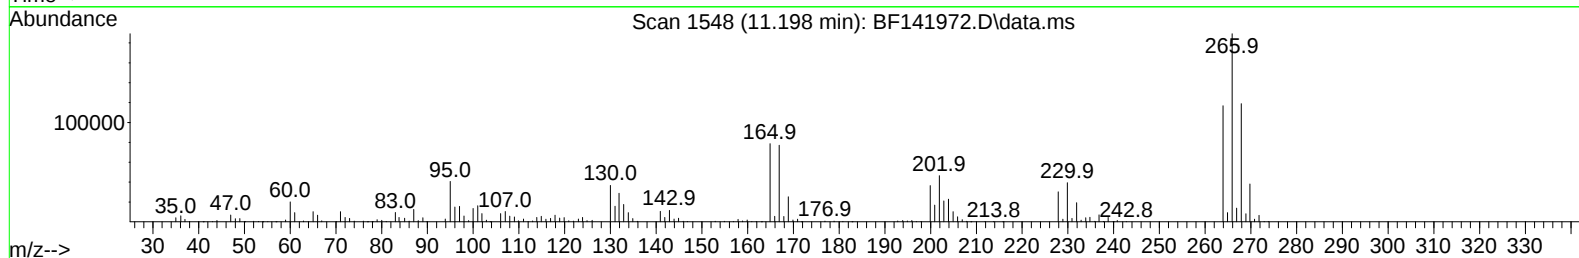


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031725\
Data File : BF141972.D
Acq On : 17 Mar 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 11:52:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

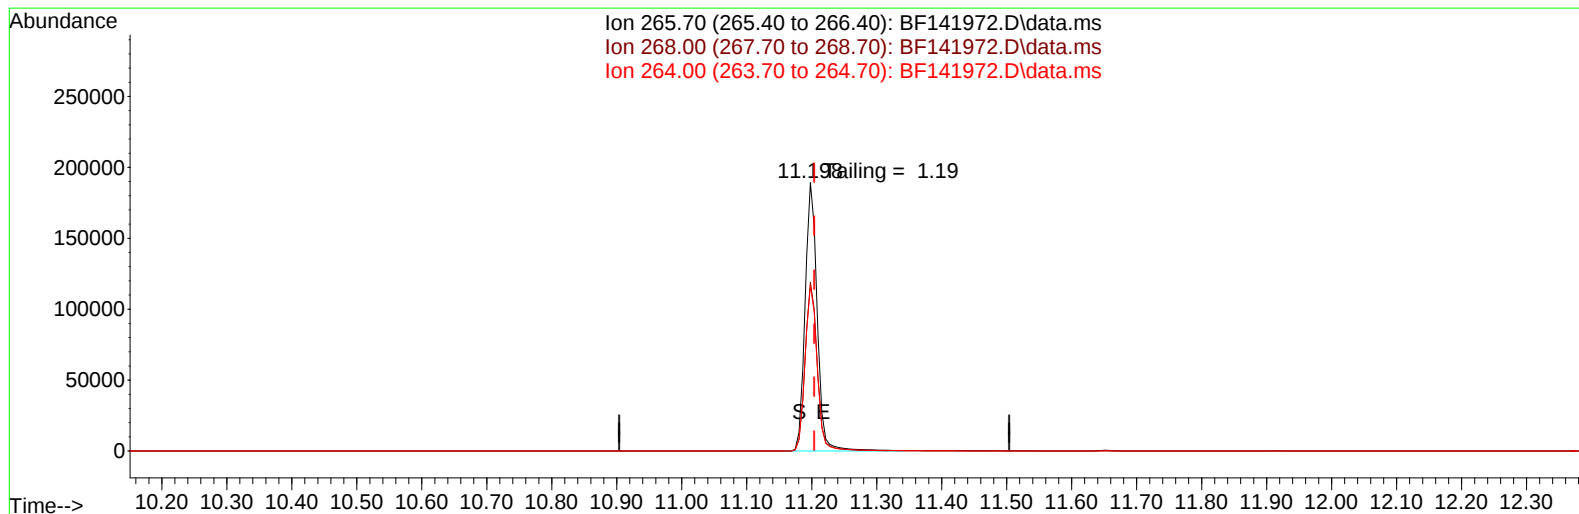

TIC: BF141972.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.006) 60186.83 ng

response 248242

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.83
264.00	62.70	61.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031725\
Data File : BF141972.D
Acq On : 17 Mar 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 11:52:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

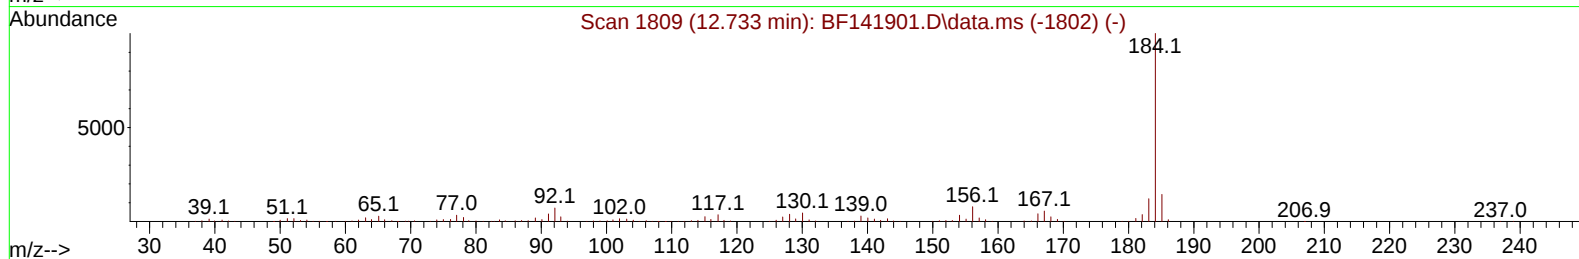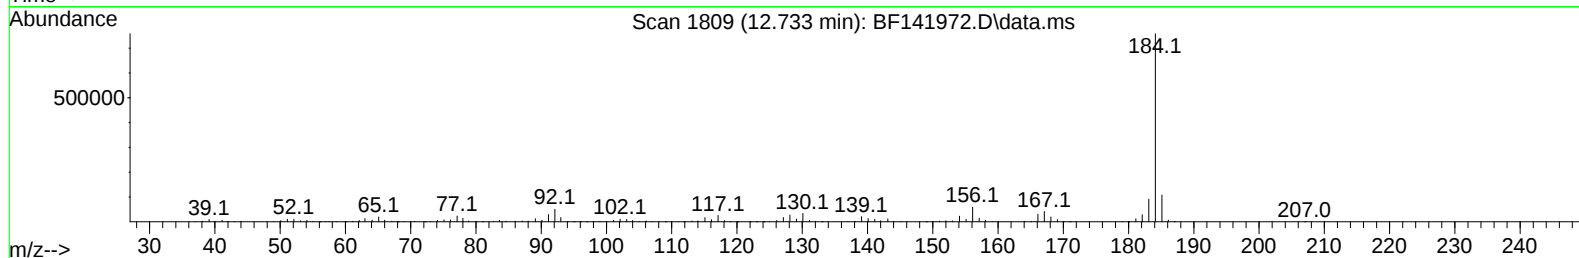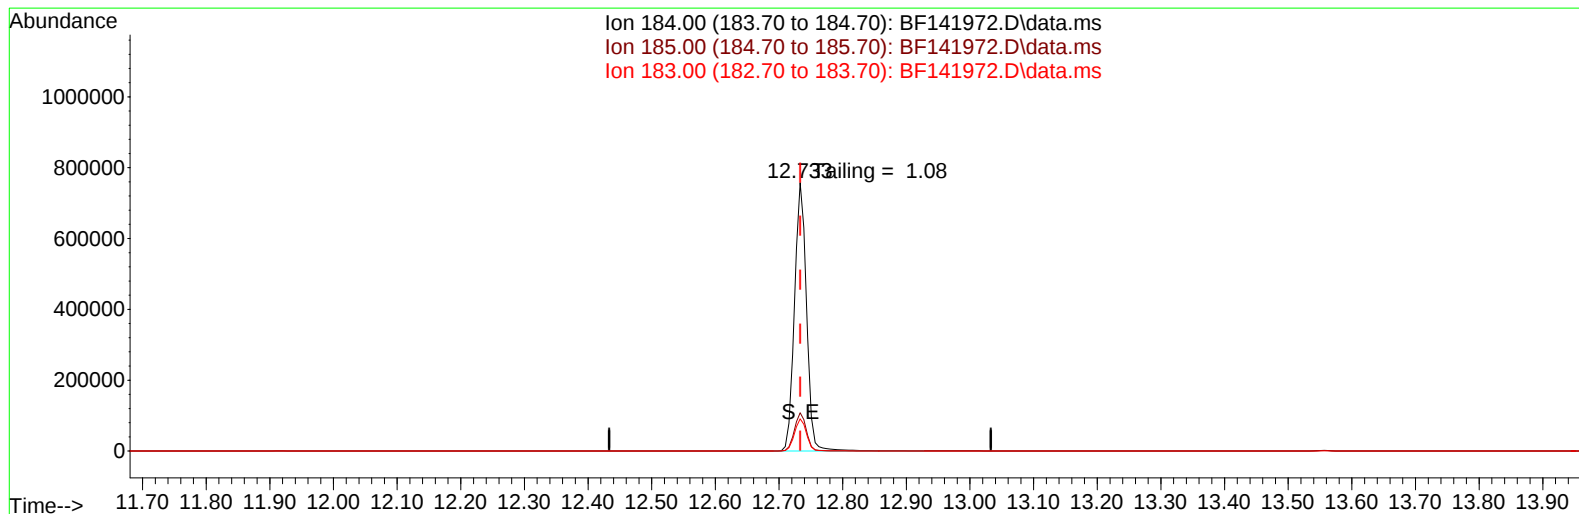

TIC: BF141972.D\data.ms

(77) Benzidine

12.733min (0.000) 175178.85 ng

response 1002071

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.27
183.00	12.10	12.01
0.00	0.00	0.00