


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031815\
 Data File : BF077808.D
 Acq On : 18 Mar 2015 22:04
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 04:03:48 2015

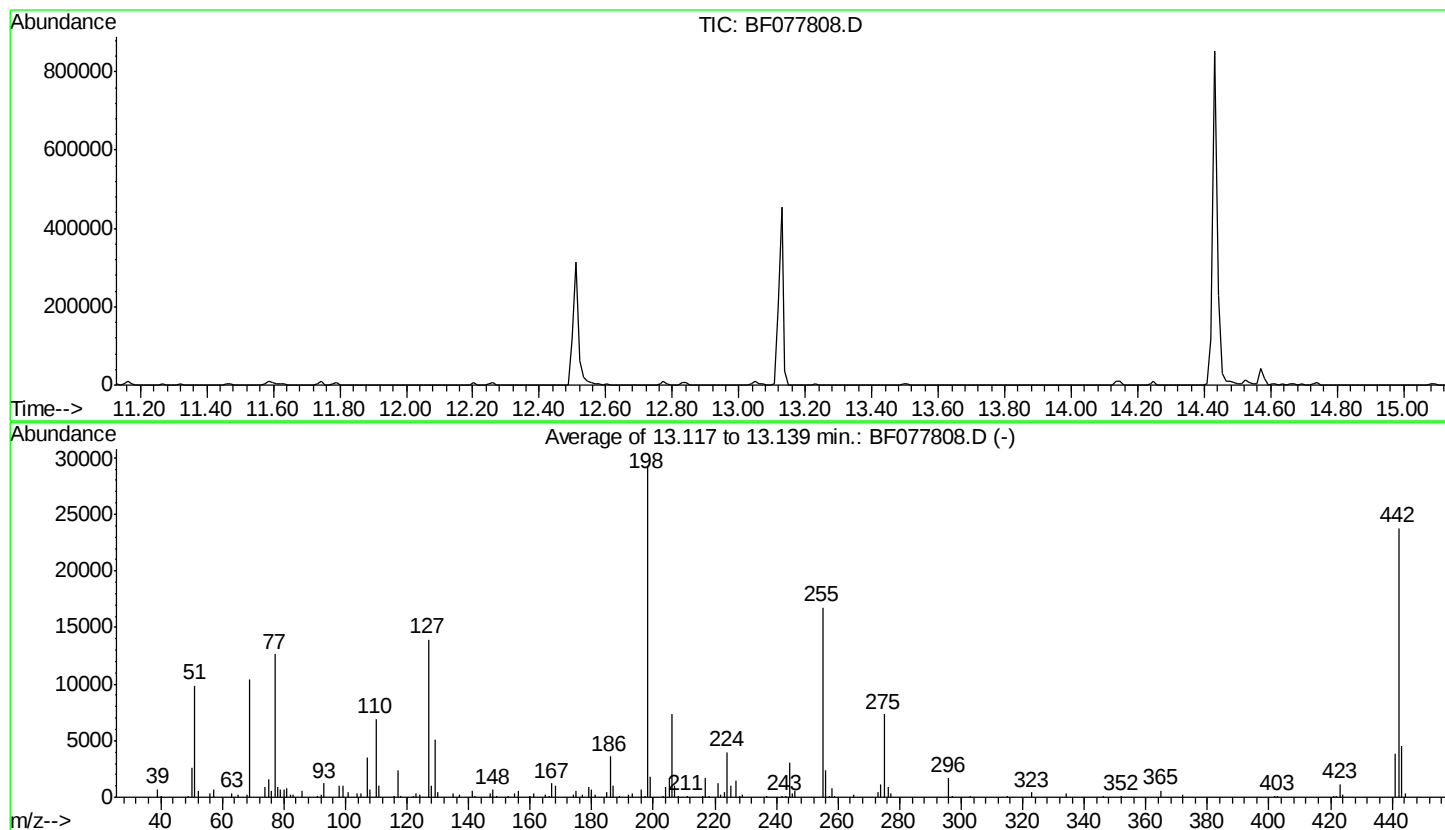

AutoFind: Scans 1070, 1071, 1072; Background Corrected with Scan 1067

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	9869	PASS
68	69	0.00	2	2.0	212	PASS
69	198	0.00	100	35.3	10354	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.5	13915	PASS
197	198	0.00	2	0.6	173	PASS
198	198	100	100	100.0	29302	PASS
199	198	5	9	6.4	1861	PASS
275	198	10	60	25.0	7333	PASS
365	198	1	100	2.1	616	PASS
441	442	0.01	24	16.0	3794	PASS
442	198	50	100	81.1	23759	PASS
443	442	15	24	18.9	4500	PASS