

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031815\
 Data File : BF077824.D
 Acq On : 19 Mar 2015 6:38
 Operator : TP/IZ
 Sample : G1535-01 5X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP1B-1-B-5(0-6)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	34	36	39	rBV	489511	497207	80.29%	10.918%
2	1.435	45	48	50	rBV	45047	55395	8.95%	1.216%
3	1.595	59	62	65	rVB	7700	8839	1.43%	0.194%
4	1.790	77	79	90	rVB	29284	43416	7.01%	0.953%
5	4.110	279	282	284	rVB	4422	6824	1.10%	0.150%
6	4.933	352	354	358	rBV	14402	18642	3.01%	0.409%
7	5.459	398	400	406	rBB	50738	54974	8.88%	1.207%
8	6.739	510	512	522	rVB	66281	72584	11.72%	1.594%
9	6.876	522	524	527	rBV	80951	74494	12.03%	1.636%
10	7.162	547	549	552	rBV	243688	217812	35.17%	4.783%
11	7.345	563	565	568	rBB	66623	62561	10.10%	1.374%
12	7.859	607	610	612	rBV	36002	40182	6.49%	0.882%
13	8.739	684	687	689	rBV	337048	299863	48.42%	6.585%
14	10.088	802	805	807	rBV	87360	98755	15.95%	2.169%
15	10.911	875	877	879	rBV	348859	356221	57.53%	7.822%
16	11.882	960	962	965	rBV	17261	25947	4.19%	0.570%
17	12.088	978	980	984	rVB	5631	11570	1.87%	0.254%
18	12.751	1036	1038	1039	rBV	348537	376818	60.85%	8.275%
19	12.774	1039	1040	1043	rVB	46554	43760	7.07%	0.961%
20	13.059	1061	1065	1067	rBV2	2004	6724	1.09%	0.148%
21	13.185	1072	1076	1077	rVV	4075	8168	1.32%	0.179%
22	13.379	1090	1093	1094	rBV	9999	12408	2.00%	0.272%
23	13.414	1094	1096	1099	rVB	10212	11775	1.90%	0.259%
24	13.505	1103	1104	1106	rBV2	12872	16127	2.60%	0.354%
25	13.688	1116	1120	1123	rBV2	7767	13192	2.13%	0.290%
26	13.757	1123	1126	1129	rBV4	8619	17714	2.86%	0.389%
27	13.882	1135	1137	1138	rBV2	4849	7380	1.19%	0.162%
28	13.974	1143	1145	1146	rBV2	4474	7237	1.17%	0.159%
29	14.042	1146	1151	1154	rBV4	8101	25428	4.11%	0.558%
30	14.099	1154	1156	1160	rVV5	4587	11979	1.93%	0.263%
31	14.179	1160	1163	1165	rVB3	6389	12128	1.96%	0.266%
32	14.248	1167	1169	1172	rBV	110657	125058	20.20%	2.746%
33	14.374	1178	1180	1182	rVB2	8463	11079	1.79%	0.243%
34	14.534	1192	1194	1196	rVB	110486	119752	19.34%	2.630%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031815\
Data File : BF077824.D
Acq On : 19 Mar 2015 6:38
Operator : TP/IZ
Sample : G1535-01 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP1B-1-B-5(0-6)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.602	1196	1200	1201	rVB3	7520	14981	2.42%	0.329%
36	14.637	1201	1203	1205	rBV3	10415	18405	2.97%	0.404%
37	14.694	1206	1208	1210	rBV	12239	17476	2.82%	0.384%
38	14.740	1210	1212	1214	rBV	131459	155065	25.04%	3.405%
39	14.785	1214	1216	1217	rBV2	9777	16388	2.65%	0.360%
40	14.900	1224	1226	1227	rBV2	9688	16778	2.71%	0.368%
41	14.945	1228	1230	1233	rVB3	18946	36159	5.84%	0.794%
42	15.002	1233	1235	1236	rBV2	9091	17181	2.77%	0.377%
43	15.517	1278	1280	1282	rVB2	18471	25053	4.05%	0.550%
44	15.768	1300	1302	1305	rBV3	16512	41829	6.75%	0.919%
45	16.043	1323	1326	1330	rBV	458375	619234	100.00%	13.598%
46	17.380	1440	1443	1447	rBV	43044	141031	22.78%	3.097%
47	17.700	1469	1471	1475	rBV2	33764	65787	10.62%	1.445%
48	17.768	1475	1477	1478	rBV	40805	50117	8.09%	1.101%
49	17.837	1480	1483	1490	rVB	361651	546457	88.25%	12.000%


Sum of corrected areas: 4553954

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031815\
Data File : BF077824.D
Acq On : 19 Mar 2015 6:38
Operator : TP/IZ
Sample : G1535-01 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP1B-1-B-5(0-6)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

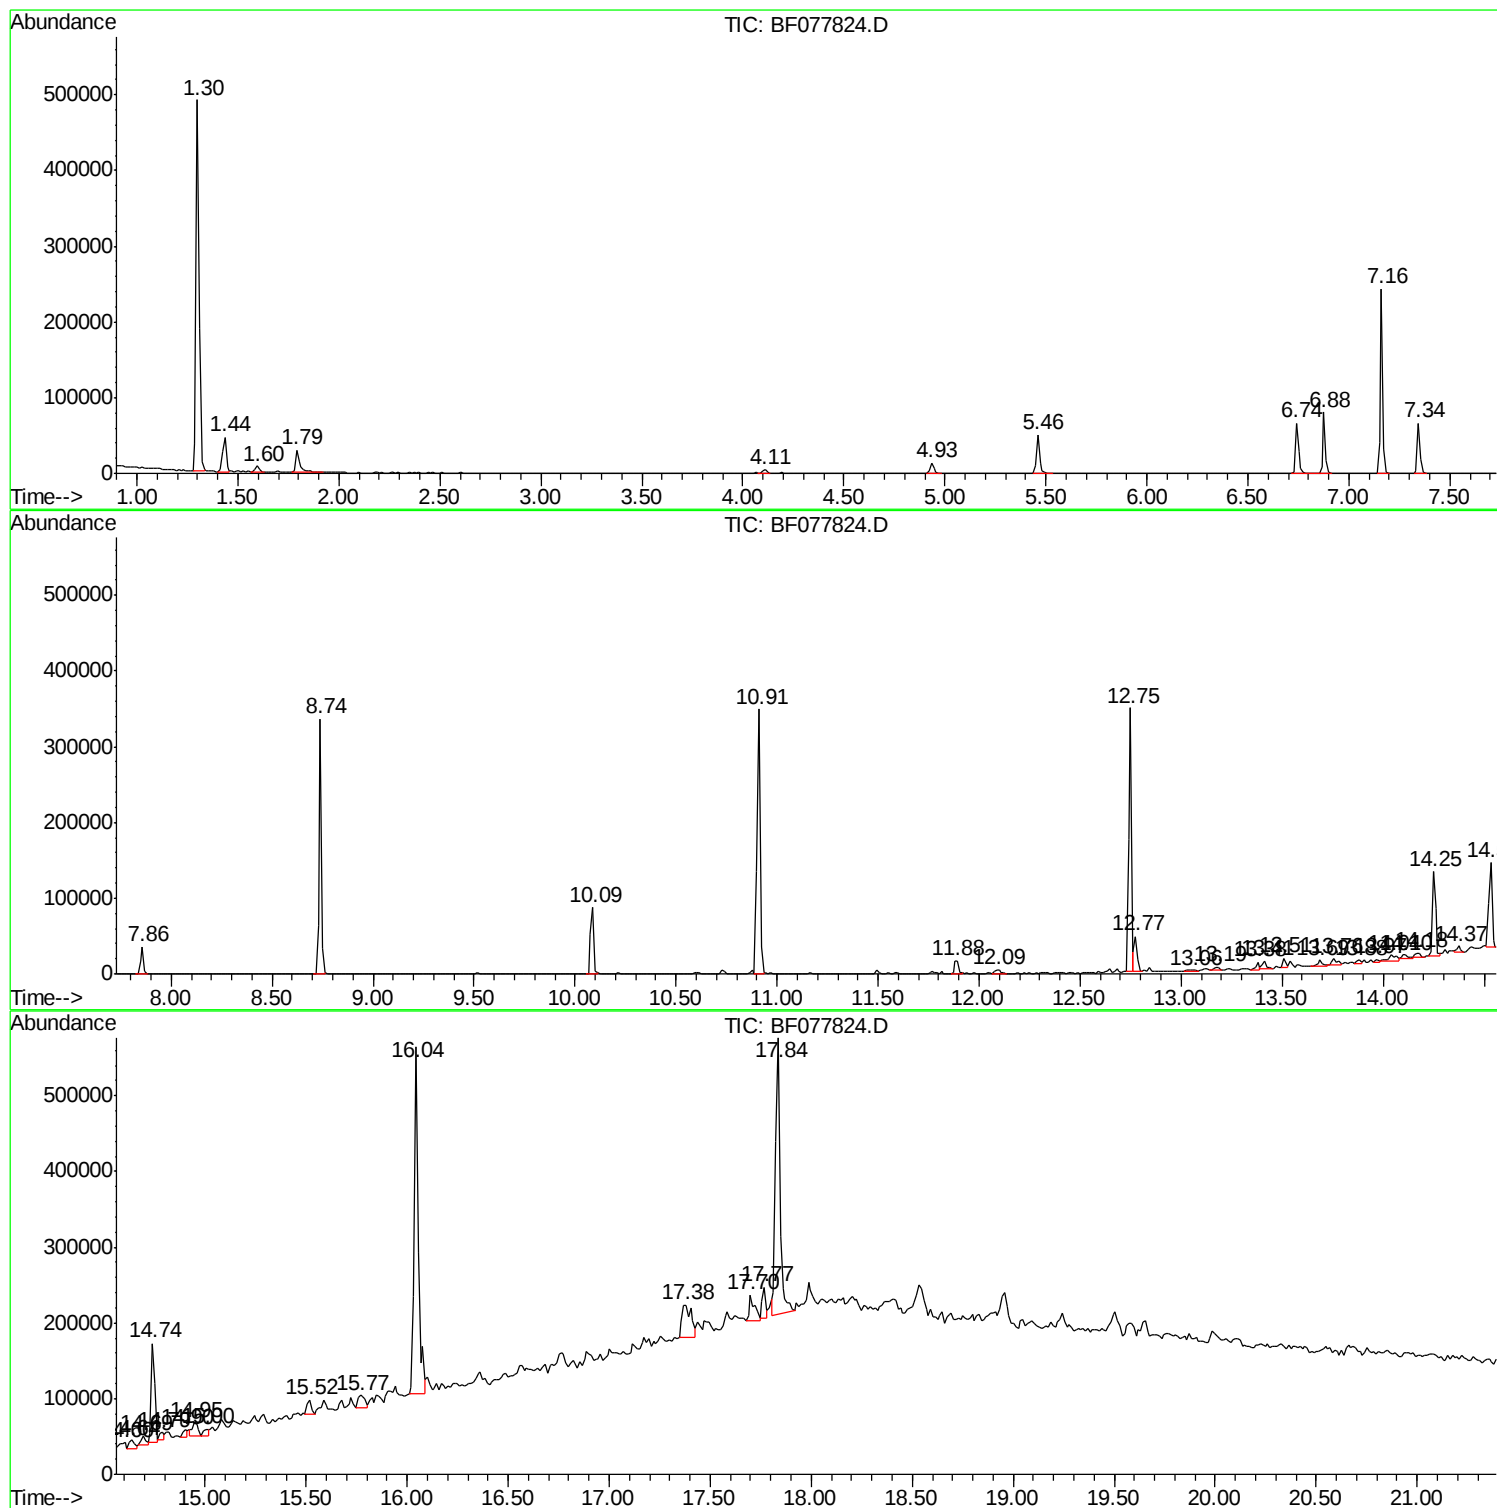

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031815\
Data File : BF077824.D
Acq On : 19 Mar 2015 6:38
Operator : TP/IZ
Sample : G1535-01 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP1B-1-B-5(0-6)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2,2-dimethoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.30	45.65 ng	497207	1,4-Dichlorobenzene-d4	7.16

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	72
2			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
3			2-Hydroxy-2-methylbutyric acid	118	C5H10O3	003739-30-8	9
4			Propanoic acid, 2-methyl-, propy...	130	C7H14O2	000644-49-5	9
5			N-Ethylformamide	73	C3H7NO	000627-45-2	5

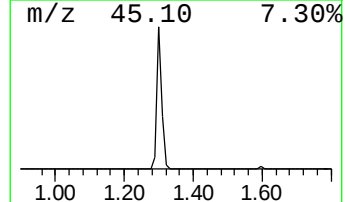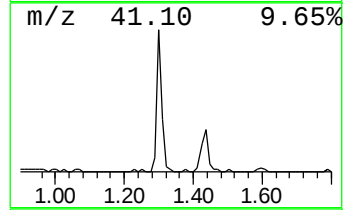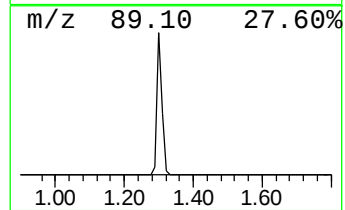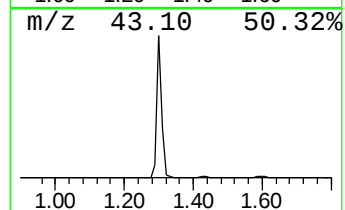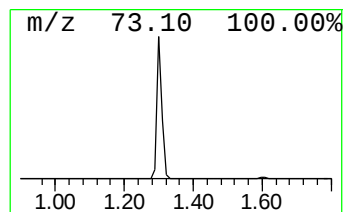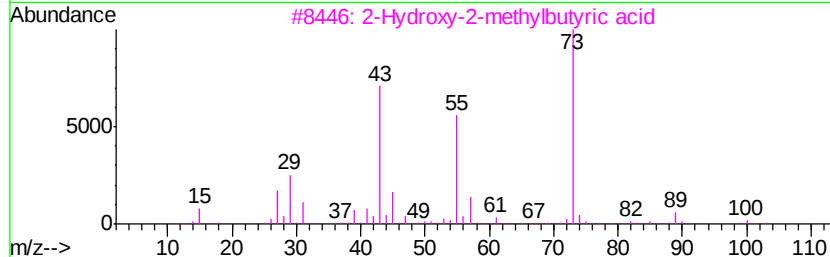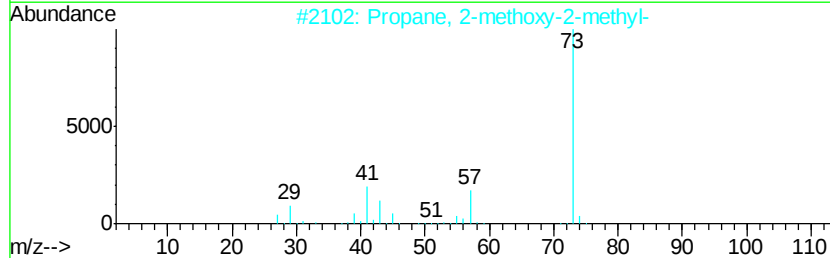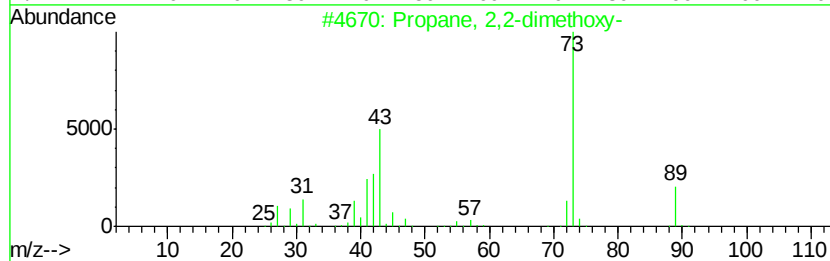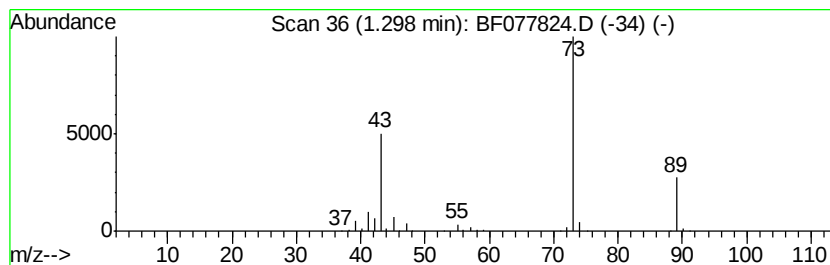

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031815\
Data File : BF077824.D
Acq On : 19 Mar 2015 6:38
Operator : TP/IZ
Sample : G1535-01 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP1B-1-B-5(0-6)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.88 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.88	6.84 ng	74494	1,4-Dichlorobenzene-d4	7.16

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	17
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

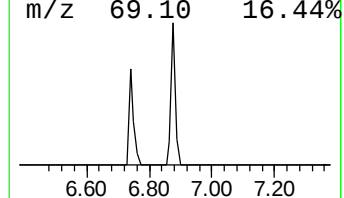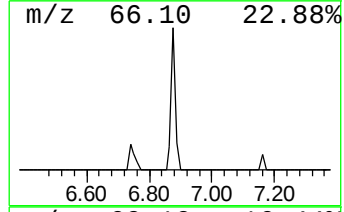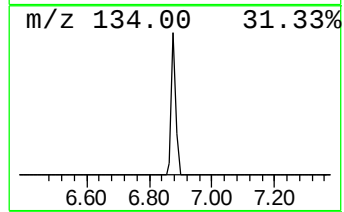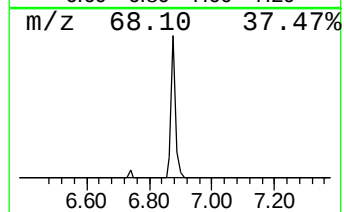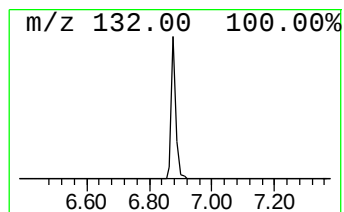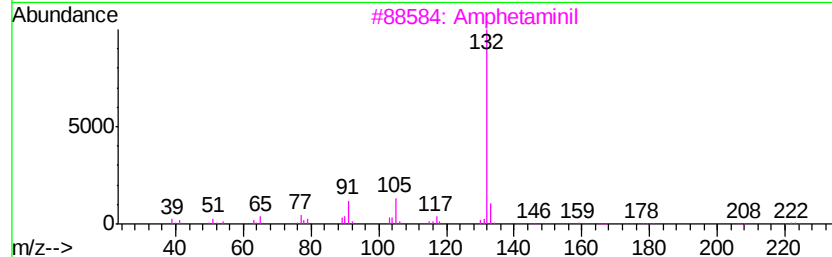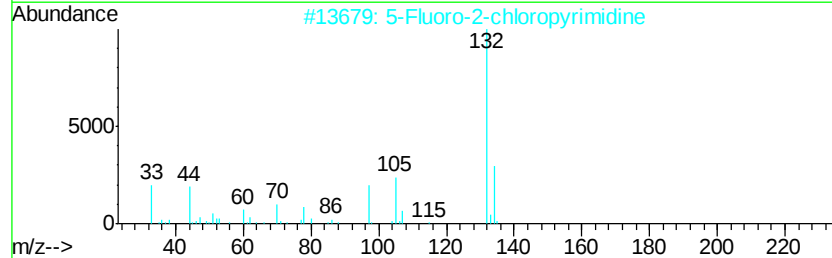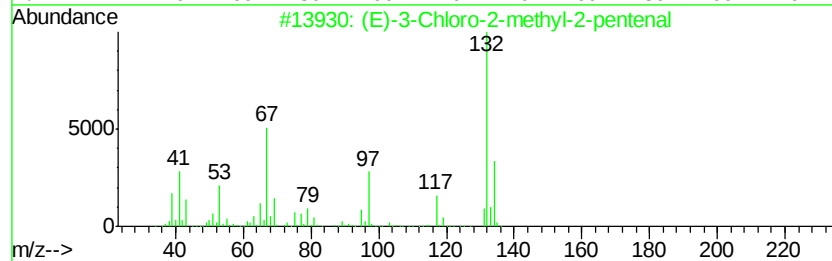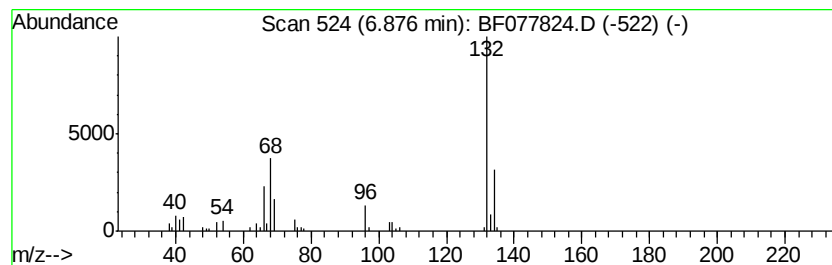

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031815\
Data File : BF077824.D
Acq On : 19 Mar 2015 6:38
Operator : TP/IZ
Sample : G1535-01 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP1B-1-B-5(0-6)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2,2-dime...	1.30	45.6	ng	497207	1	7.16	217812	20.0
unknown6.88	6.88	6.8	ng	74494	1	7.16	217812	20.0