
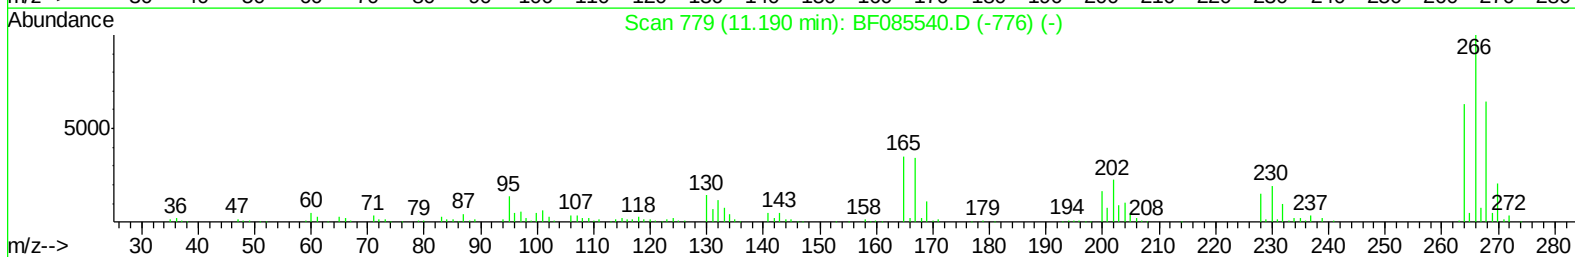
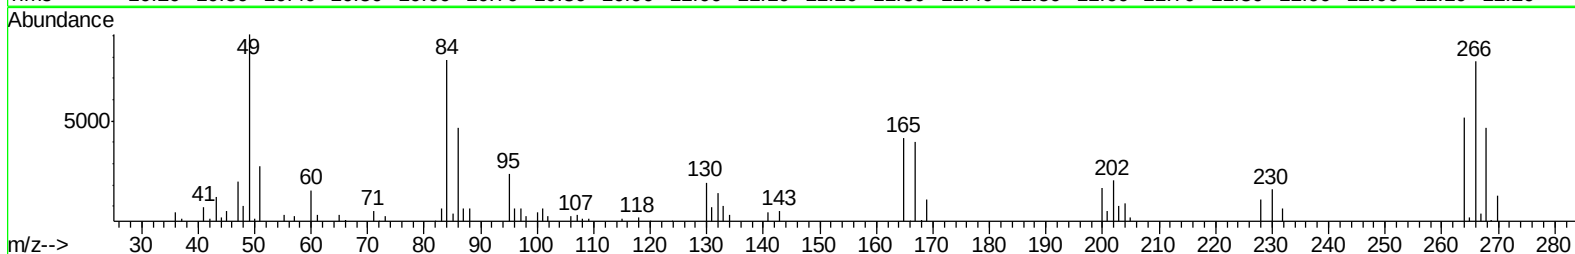


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085535.D
Acq On : 18 Mar 2016 15:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 03:03:51 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

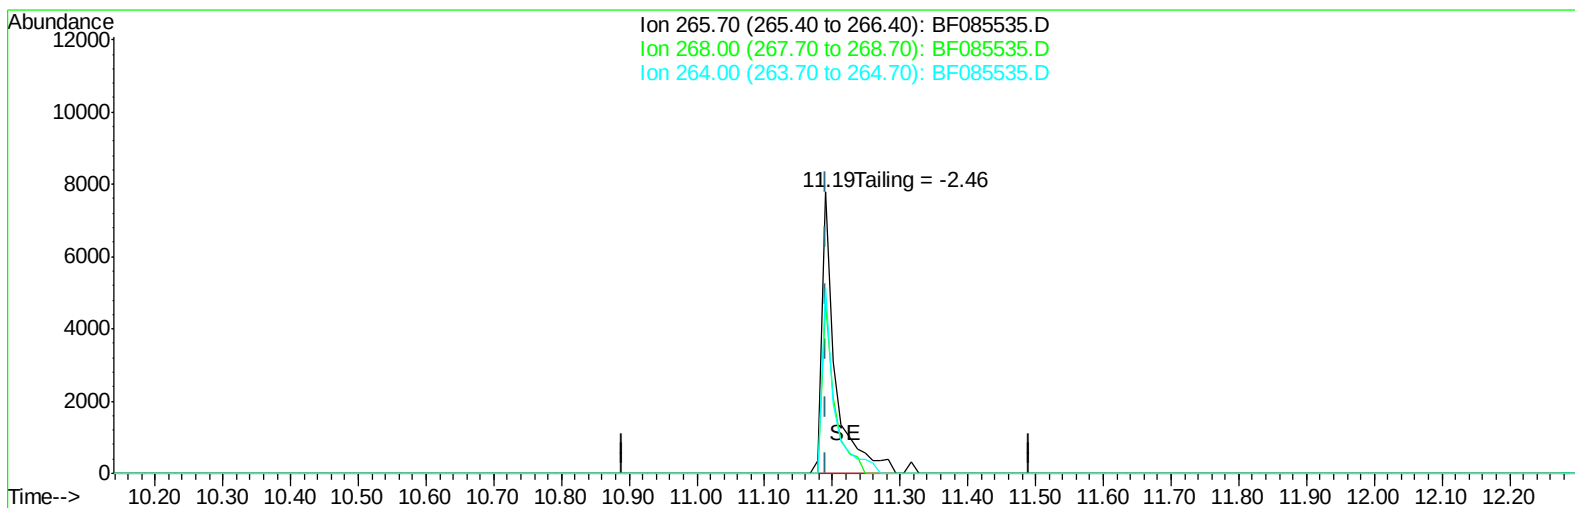

TIC: BF085535.D

(69) Pentachlorophenol (C)




11.191min (+0.000) 0.00ng m

response 10666

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	60.29
264.00	63.30	65.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085535.D
Acq On : 18 Mar 2016 15:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 03:03:51 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

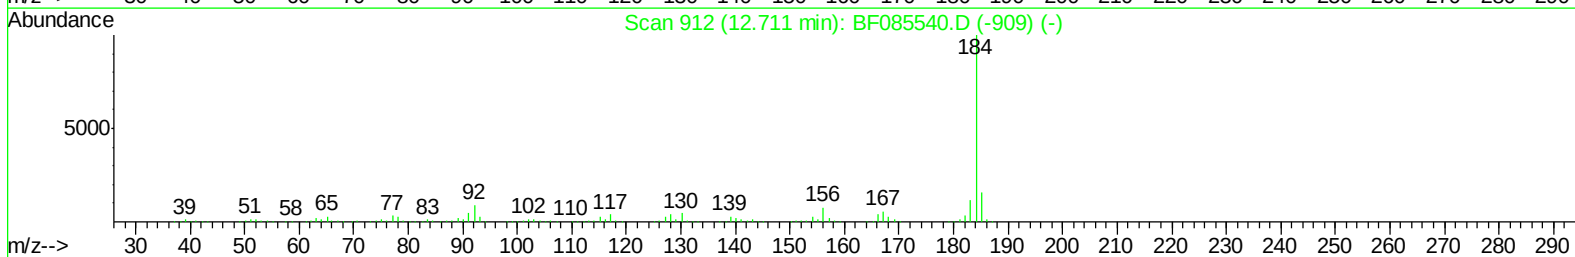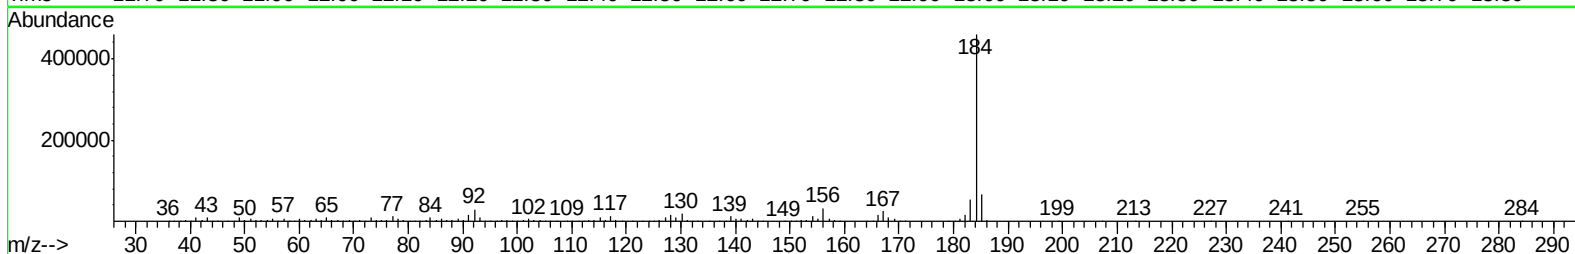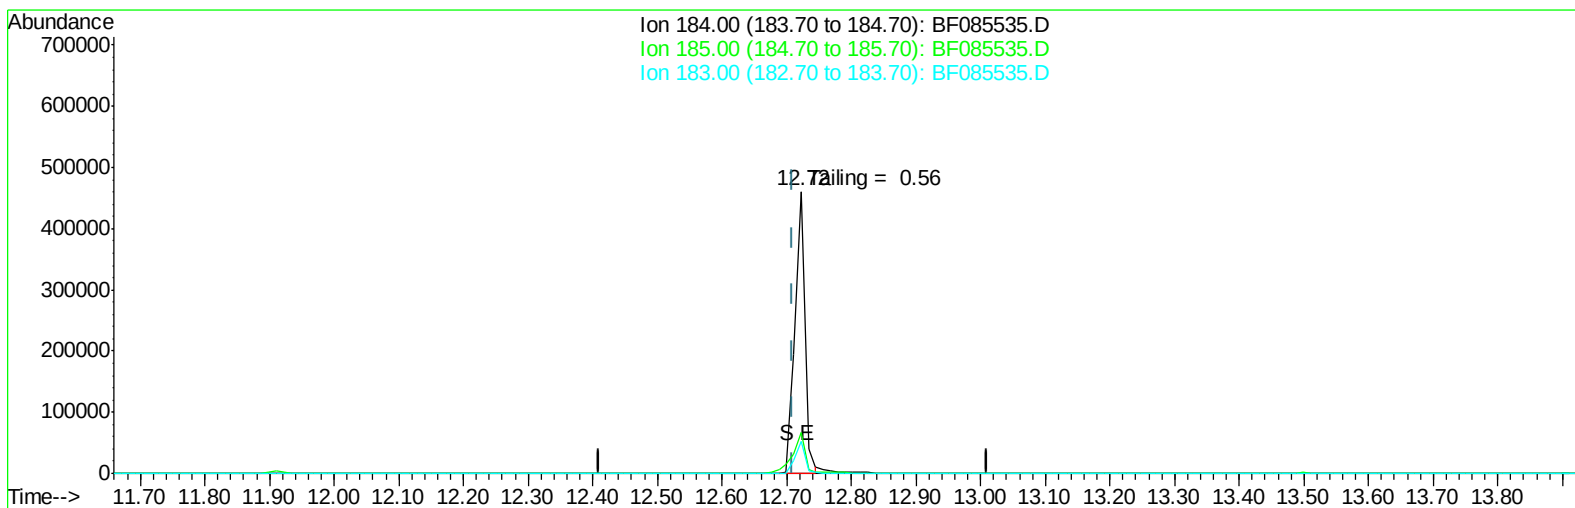

TIC: BF085535.D

(76) Benzidine

12.722min (+0.012) 48457.28ng

response 501900

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.41
183.00	11.80	11.43
0.00	0.00	0.00