
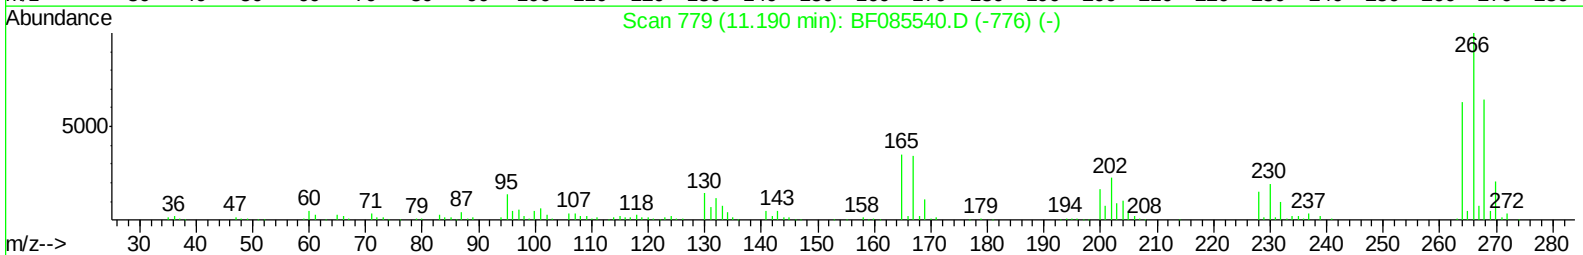
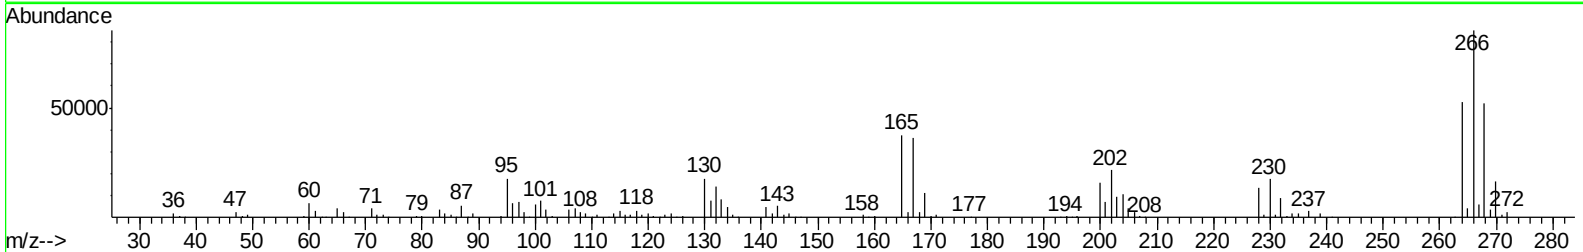


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085570.D
Acq On : 19 Mar 2016 14:00
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 05:30:47 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

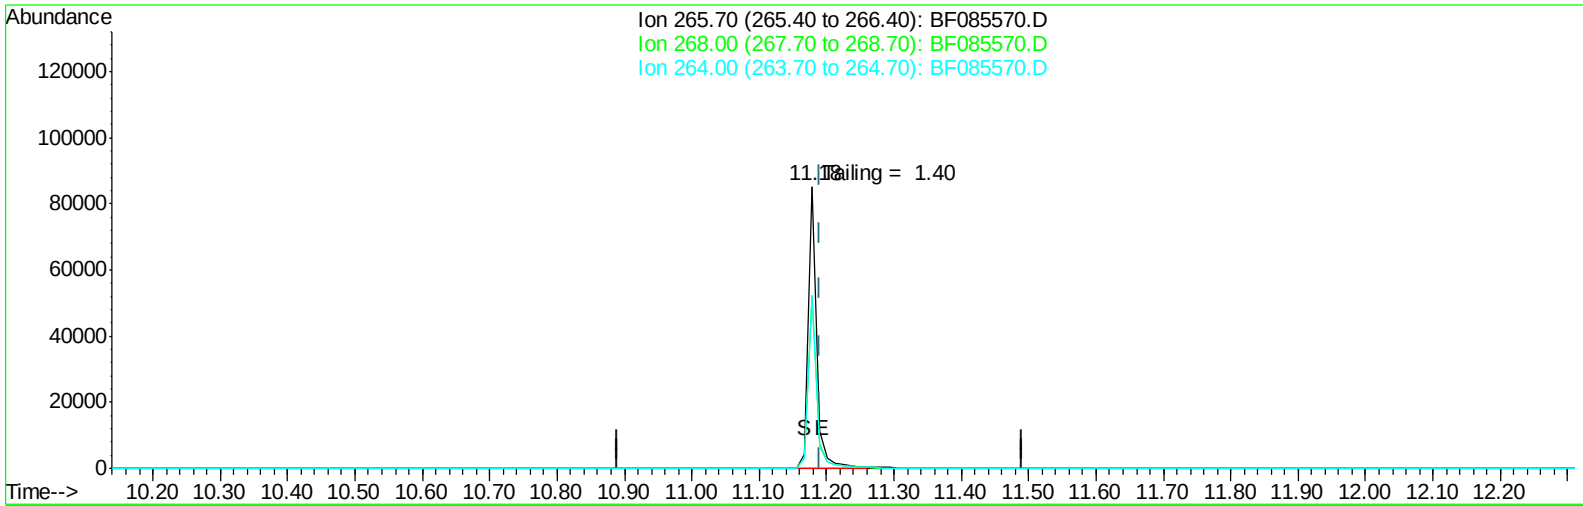

TIC: BF085570.D

(69) Pentachlorophenol (C)




11.179min (-0.011) 37598.37ng

response 75103

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.37
264.00	63.30	61.58
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085570.D
Acq On : 19 Mar 2016 14:00
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 05:30:47 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

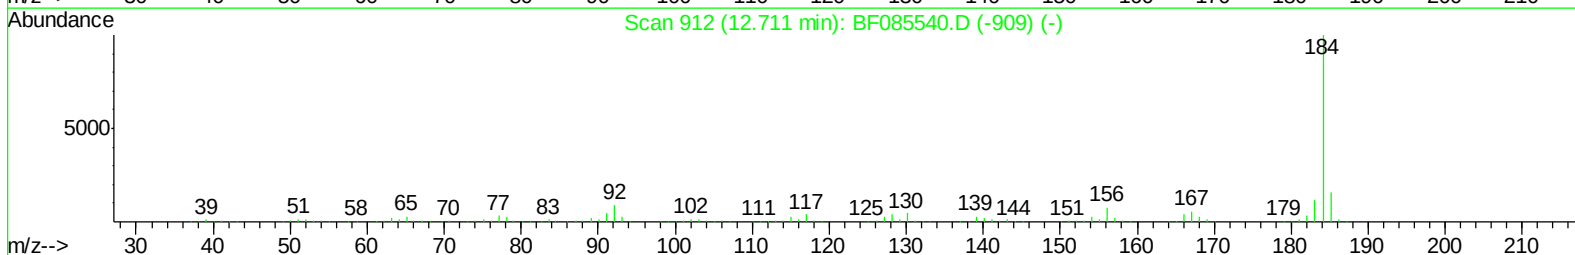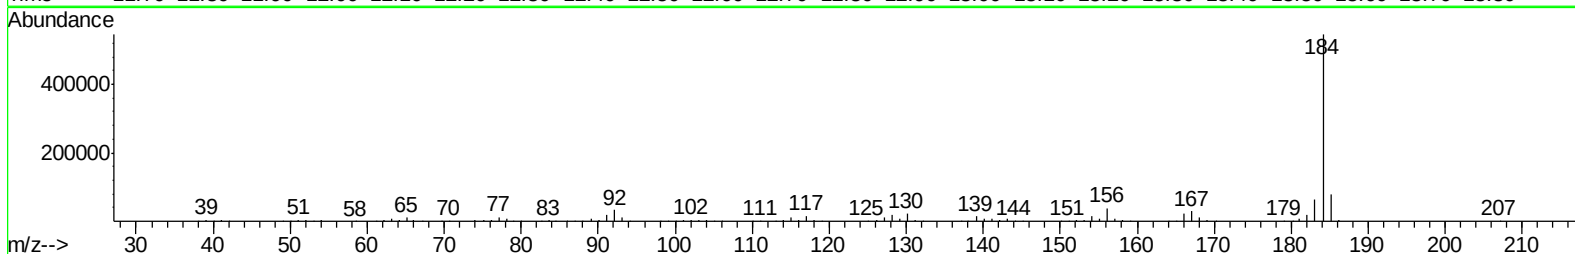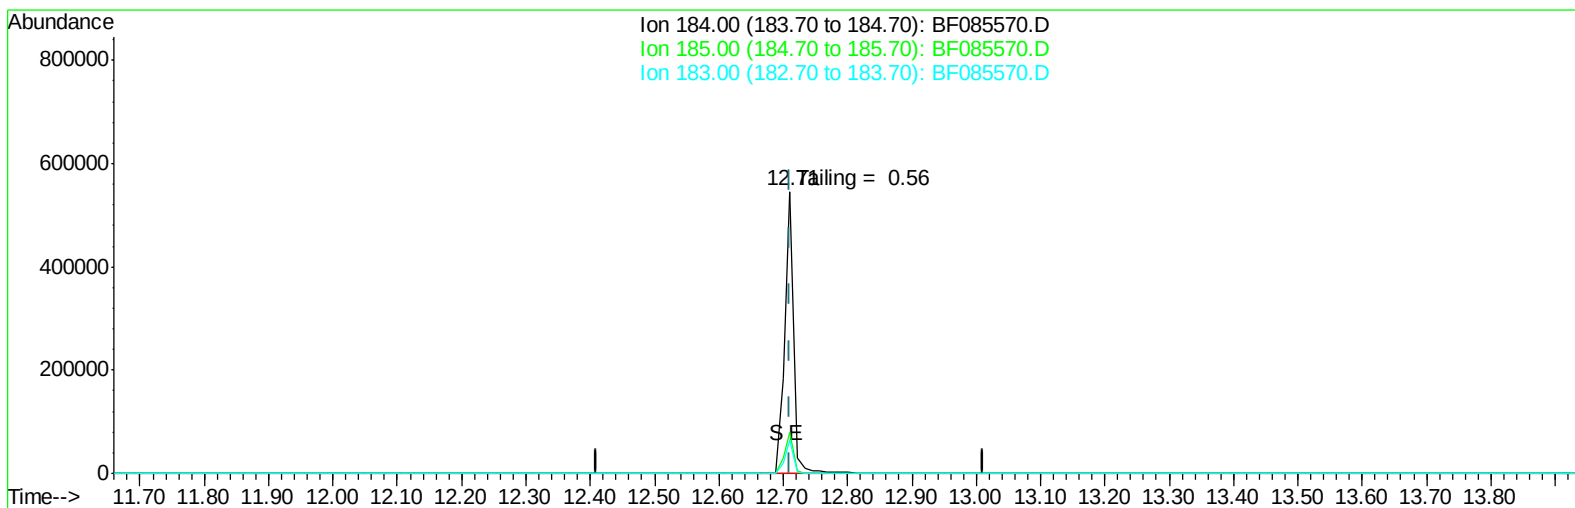

TIC: BF085570.D

(76) Benzidine

12.711min (+0.000) 25089.34ng

response 545041

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.52
183.00	11.80	11.73
0.00	0.00	0.00