
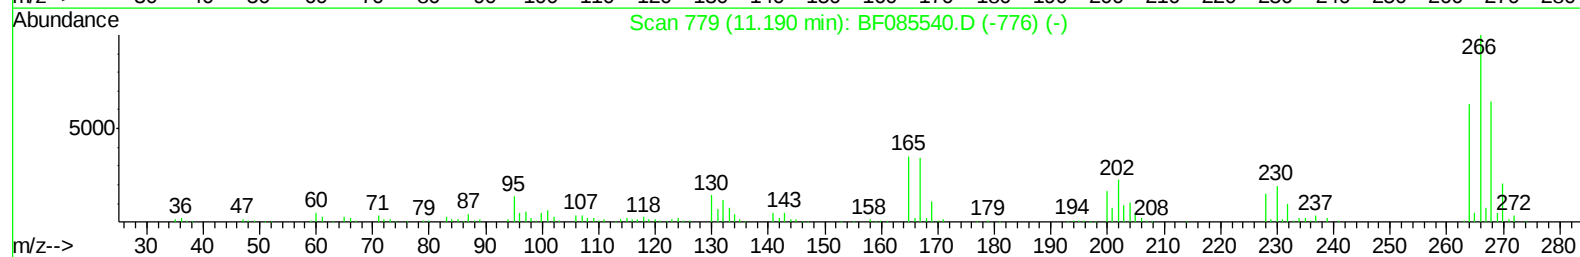
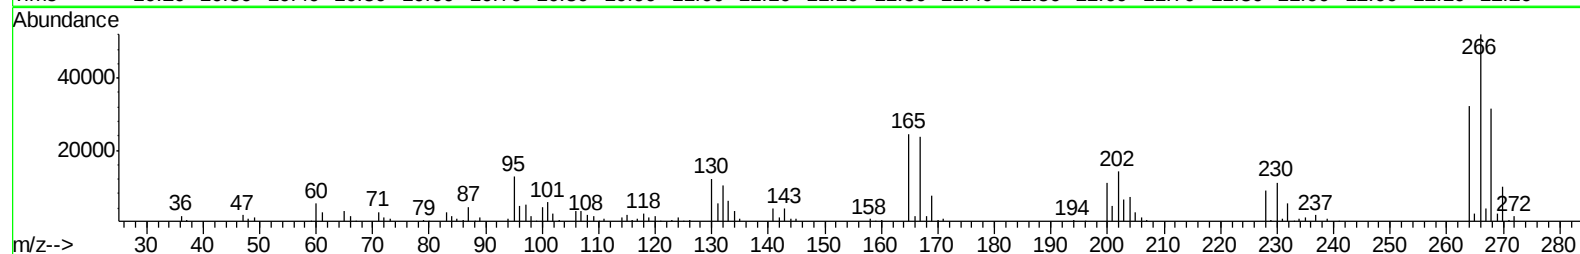


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085594.D
Acq On : 20 Mar 2016 2:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 05:32:00 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

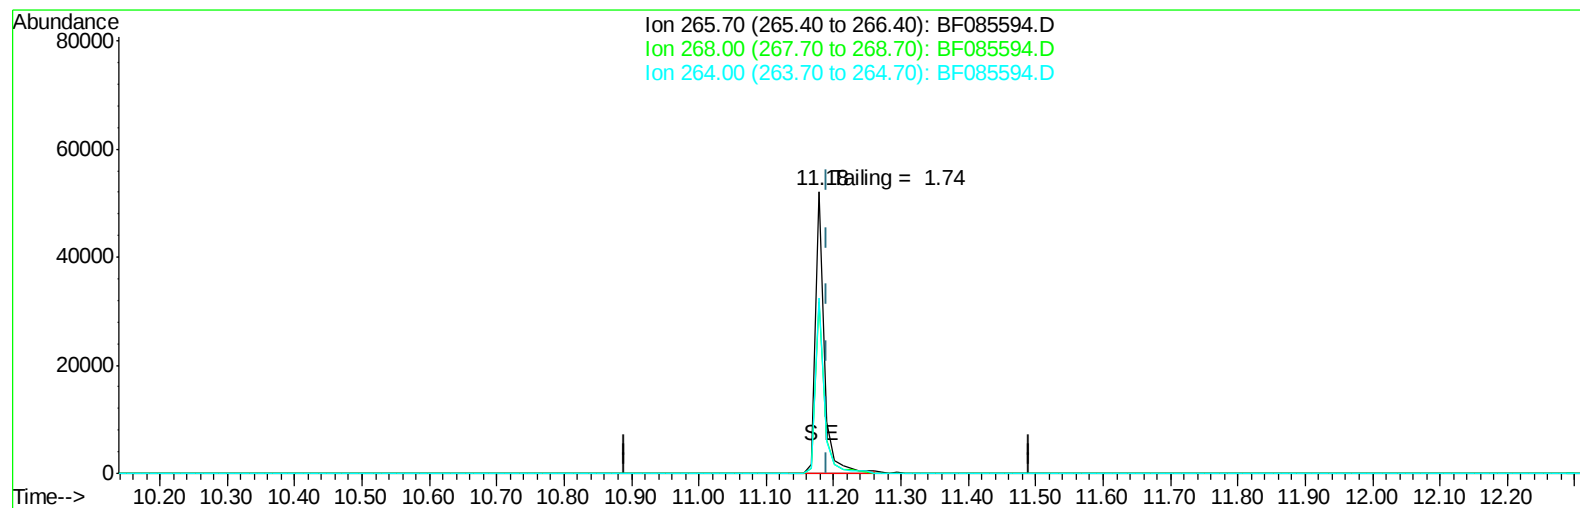

TIC: BF085594.D

(69) Pentachlorophenol (C)




11.179min (-0.011) 29578.52ng

response 48029

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	60.88
264.00	63.30	62.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085594.D
Acq On : 20 Mar 2016 2:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 05:32:00 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 23:31:39 2016
Response via : Initial Calibration

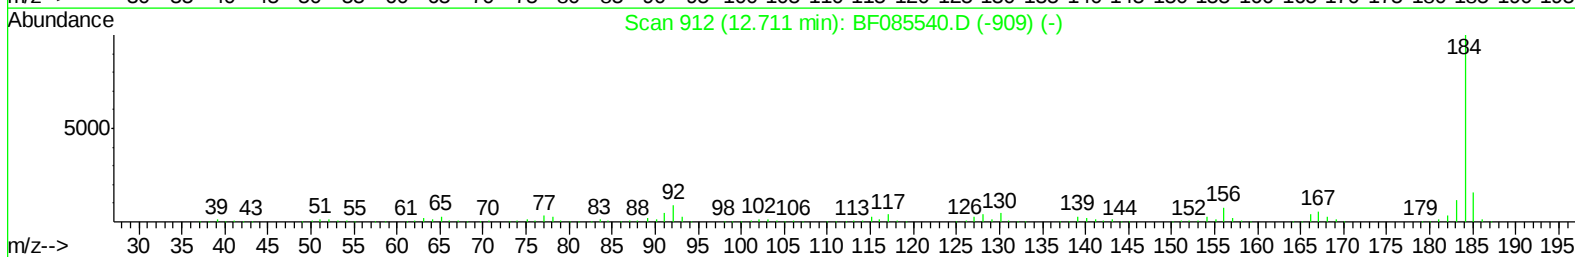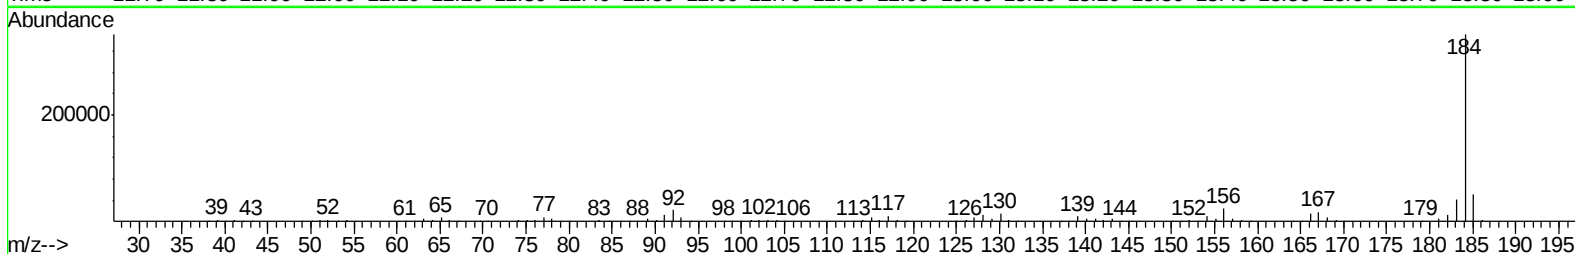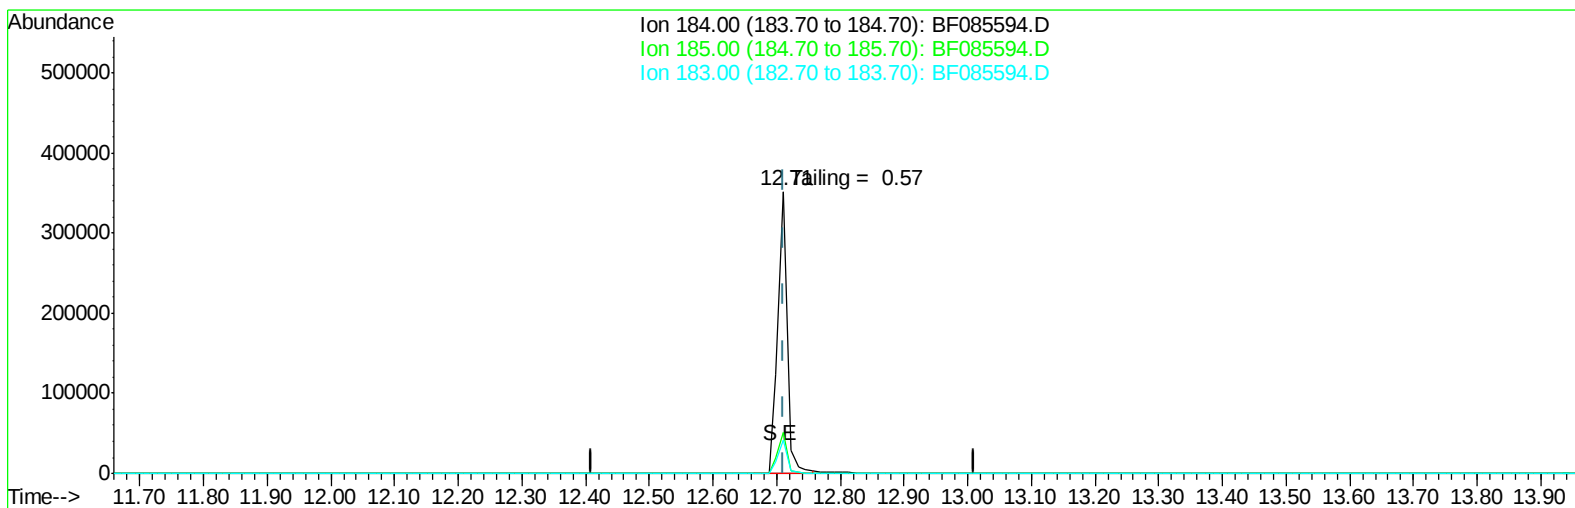

TIC: BF085594.D

(76) Benzidine

12.711min (+0.000) 0.00ng

response 364526

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.46
183.00	11.80	11.63
0.00	0.00	0.00