

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF031816\  
 Data File : BF085558.D  
 Acq On : 19 Mar 2016 7:03  
 Operator : UM/SJ  
 Sample : H1788-09  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 TW-5

Quant Time: Mar 21 01:29:23 2016  
 Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031816.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Mar 18 23:31:39 2016  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|-------|------|----------|--------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 6.85  | 152  | 119843   | 20.00  | ng    | -0.01    |
| 21) Naphthalene-d8          | 8.14  | 136  | 520819   | 20.00  | ng    | 0.00     |
| 38) Acenaphthene-d10        | 9.89  | 164  | 231288   | 20.00  | ng    | -0.01    |
| 63) Phenanthrene-d10        | 11.37 | 188  | 452376   | 20.00  | ng    | -0.01    |
| 75) Chrysene-d12            | 14.00 | 240  | 351406   | 20.00  | ng    | -0.01    |
| 86) Perylene-d12            | 15.43 | 264  | 295516   | 20.00  | ng    | -0.01    |
| System Monitoring Compounds |       |      |          |        |       |          |
| 5) 2-Fluorophenol           | 5.45  | 112  | 495368   | 69.43  | ng    | 0.00     |
| 7) Phenol-d6                | 6.48  | 99   | 402860   | 44.02  | ng    | -0.01    |
| 23) Nitrobenzene-d5         | 7.42  | 82   | 791603   | 88.23  | ng    | -0.01    |
| 41) 2,4,6-Tribromophenol    | 10.68 | 330  | 312676   | 138.01 | ng    | -0.01    |
| 44) 2-Fluorobiphenyl        | 9.21  | 172  | 1212581  | 91.06  | ng    | -0.01    |
| 78) Terphenyl-d14           | 12.96 | 244  | 1282441  | 87.82  | ng    | 0.00     |


| Target Compounds | Qvalue |
|------------------|--------|
|------------------|--------|


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF031816\  
Data File : BF085558.D  
Acq On : 19 Mar 2016 7:03  
Operator : UM/SJ  
Sample : H1788-09  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
TW-5

Quant Time: Mar 21 01:29:23 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031816.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 18 23:31:39 2016  
Response via : Initial Calibration

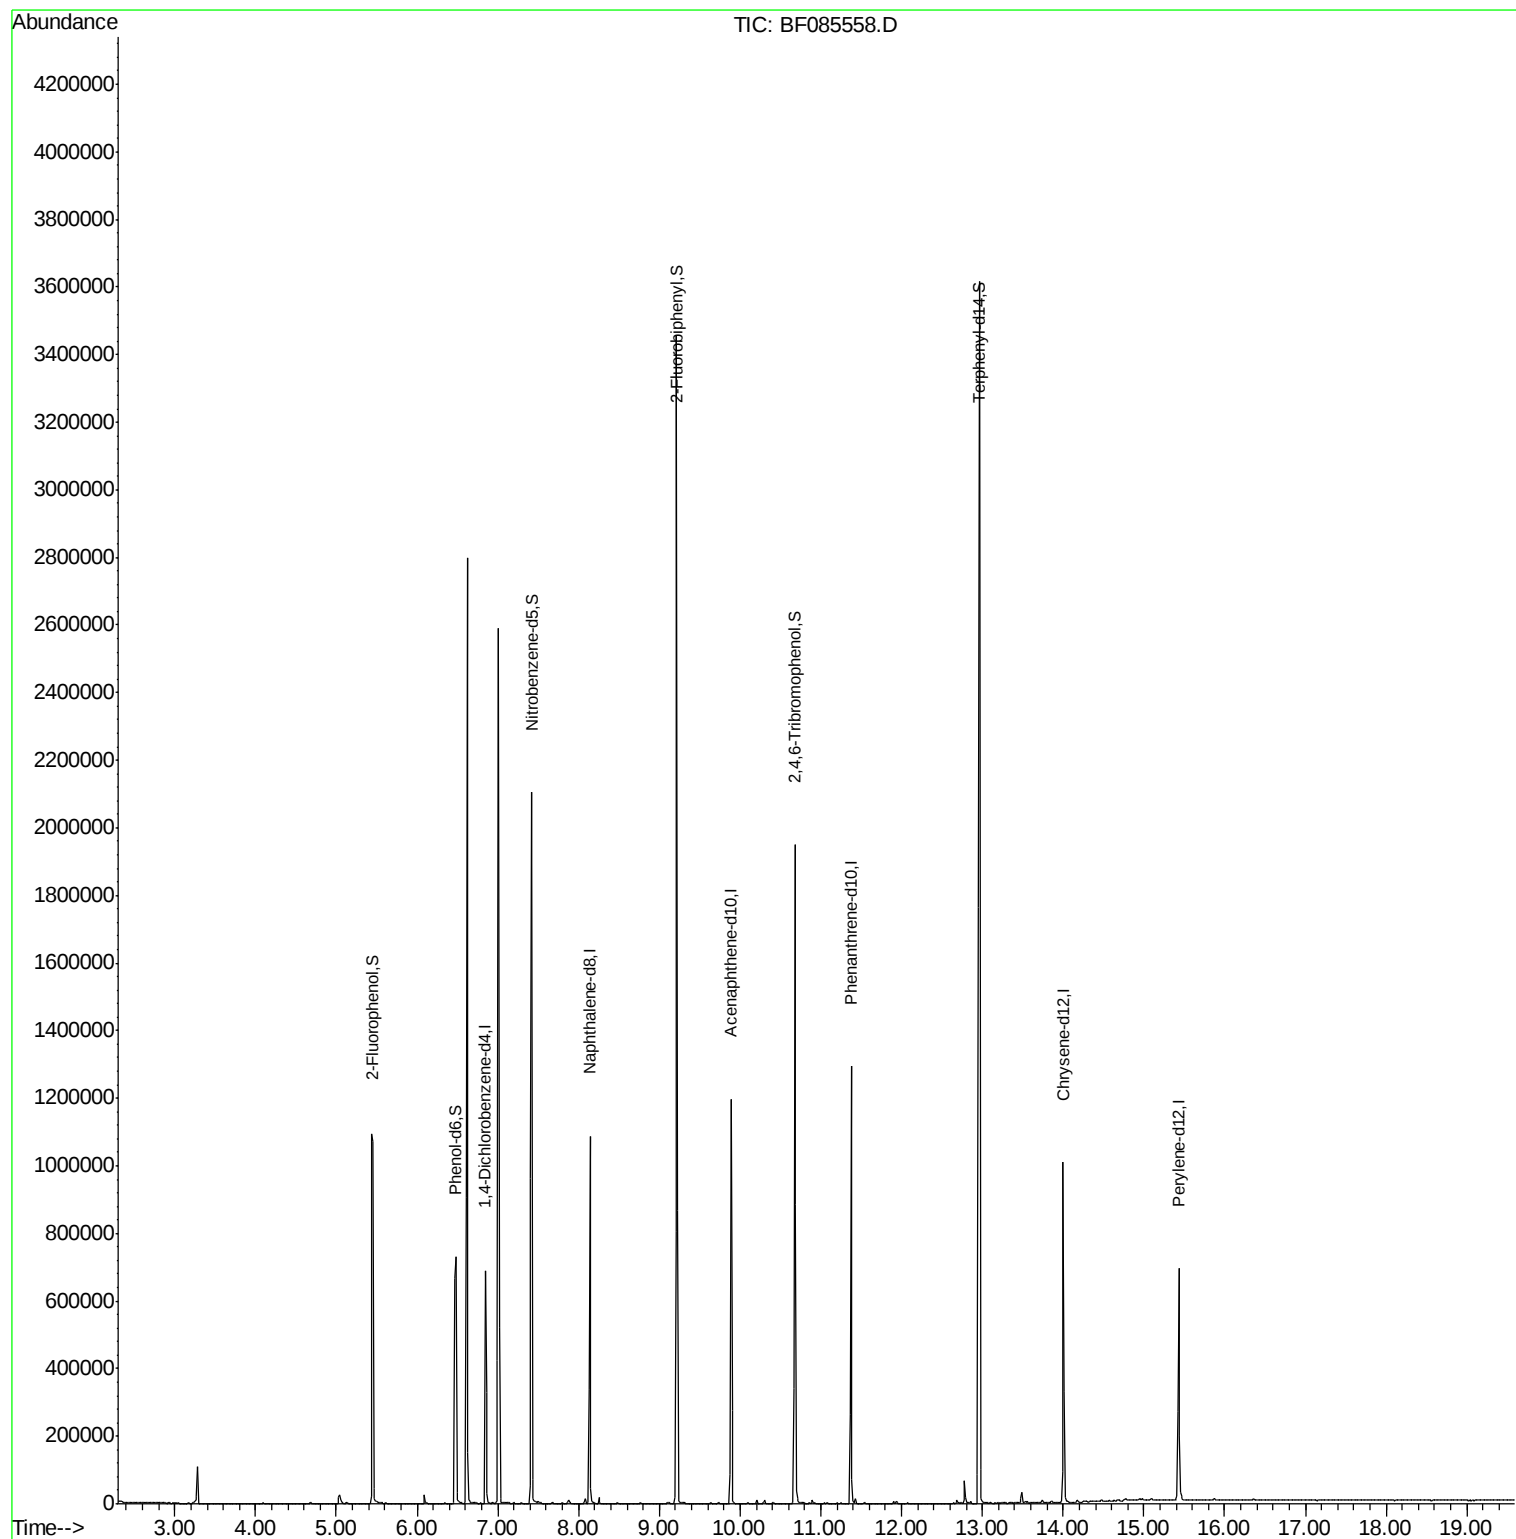

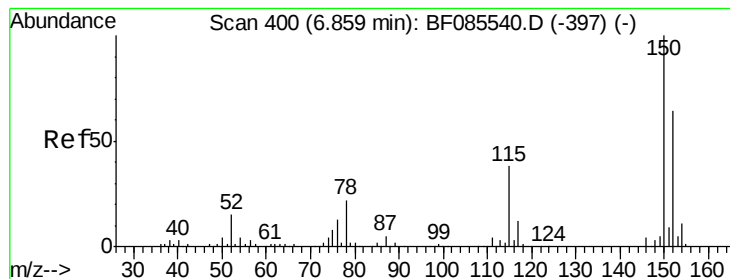

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.85 min Scan# 399

Delta R.T. -0.01 min

Lab File: BF085558.D

Acq: 19 Mar 2016 7:03

Instrument :

BNA\_F

ClientSampleId :

TW-5


Tgt Ion:152 Resp: 119843

Ion Ratio Lower Upper

152 100

150 163.1 124.2 186.2




115 73.6 47.0 70.6#

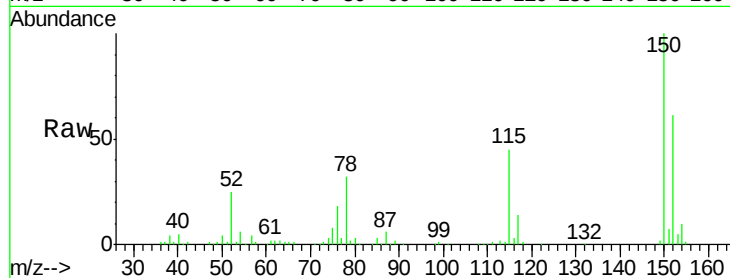

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

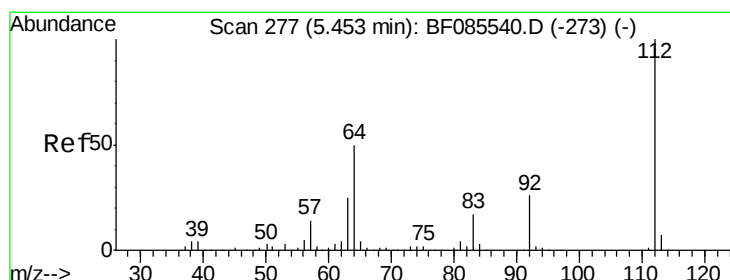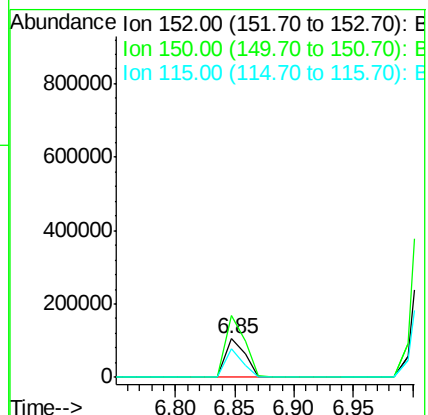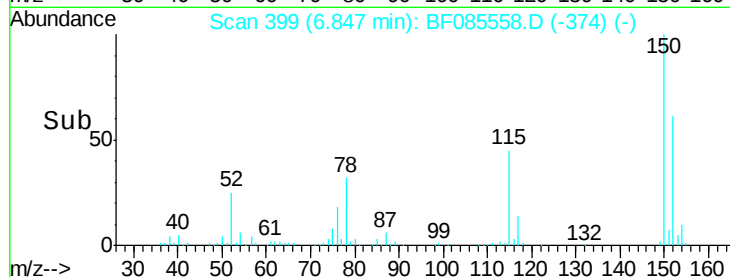

#5

2-Fluorophenol

Concen: 69.43 ng

RT: 5.45 min Scan# 277

Delta R.T. 0.00 min

Lab File: BF085558.D

Acq: 19 Mar 2016 7:03


Tgt Ion:112 Resp: 495368

Ion Ratio Lower Upper

112 100

64 44.6 39.9 59.9



63 22.2 20.2 30.2

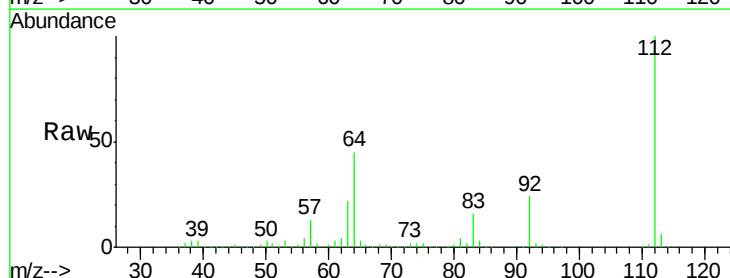

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

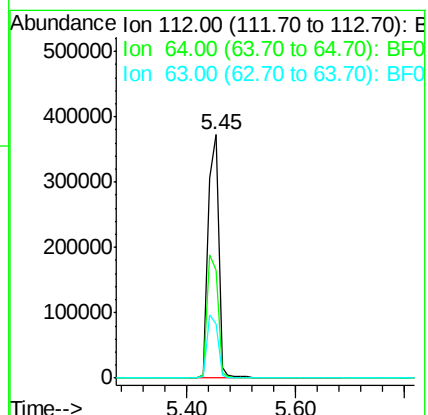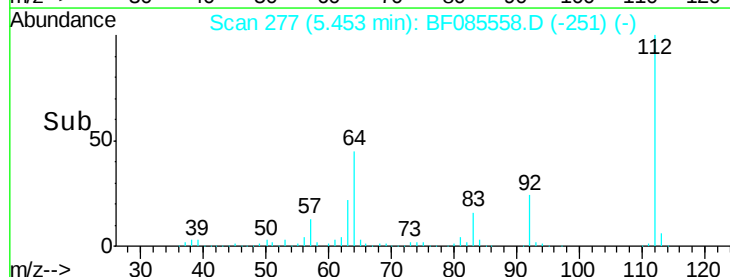



#7

Phenol-d6

Concen: 44.02 ng

RT: 6.48 min Scan# 367

Delta R.T. -0.01 min

Lab File: BF085558.D

Acq: 19 Mar 2016 7:03

Instrument :

BNA\_F

ClientSampleId :

TW-5


Tgt Ion: 99 Resp: 402860

Ion Ratio Lower Upper

99 100

42 11.6 11.1 16.7



71 26.8 24.9 37.3

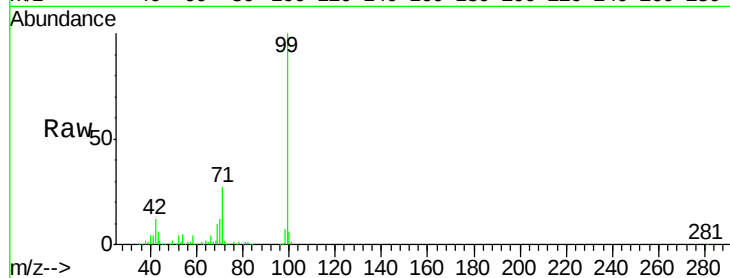

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

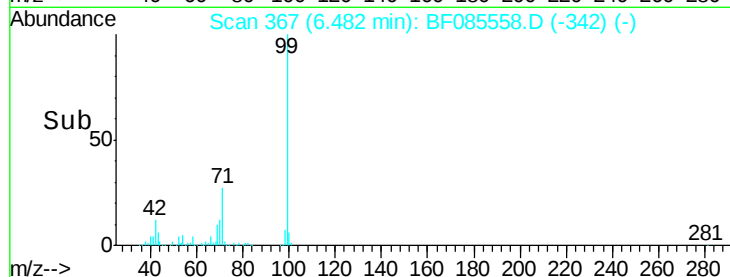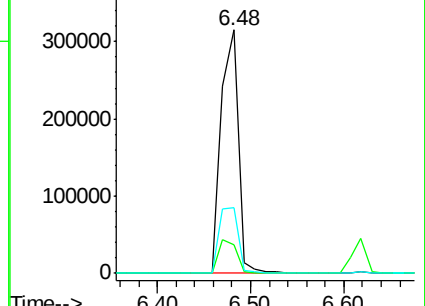

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.14 min Scan# 512

Delta R.T. 0.00 min

Lab File: BF085558.D

Acq: 19 Mar 2016 7:03

Tgt Ion: 136 Resp: 520819


Ion Ratio Lower Upper

136 100

137 11.1 9.1 13.7

54 5.8 7.4 11.0#

68 5.1 5.8 8.8#


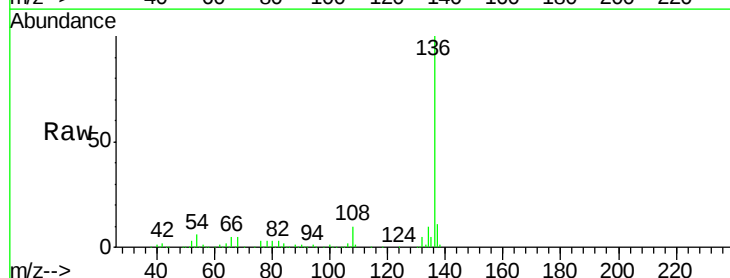



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

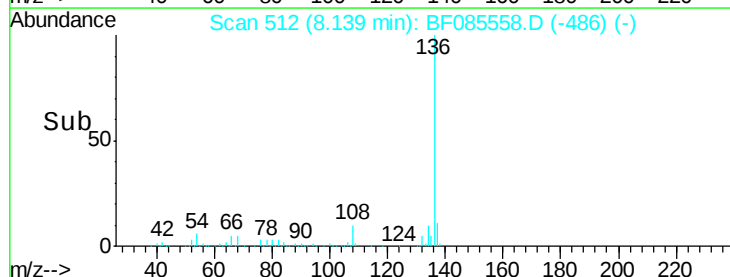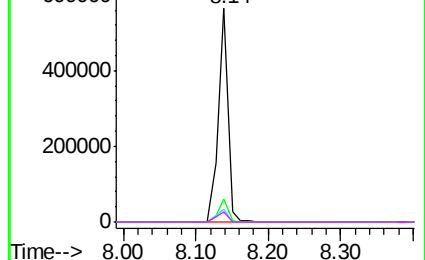

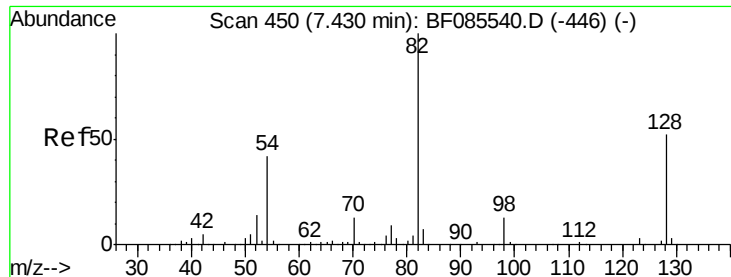

#23

Nitrobenzene-d5

Concen: 88.23 ng

RT: 7.42 min Scan# 449

Delta R.T. -0.01 min

Lab File: BF085558.D

Acq: 19 Mar 2016 7:03

Instrument :

BNA\_F

ClientSampled :

TW-5


Tgt Ion: 82 Resp: 791603

Ion Ratio Lower Upper

82 100

128 46.8 41.8 62.8




54 45.2 33.4 50.0

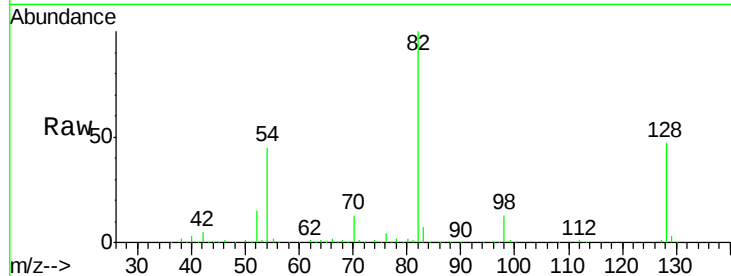

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

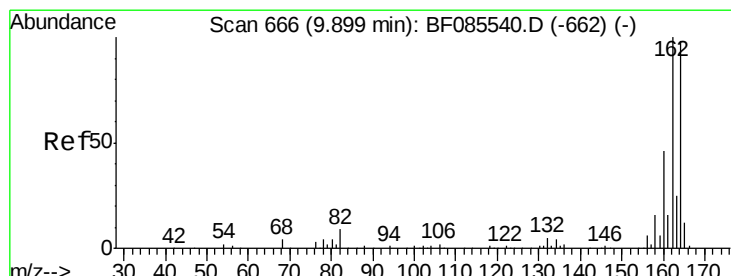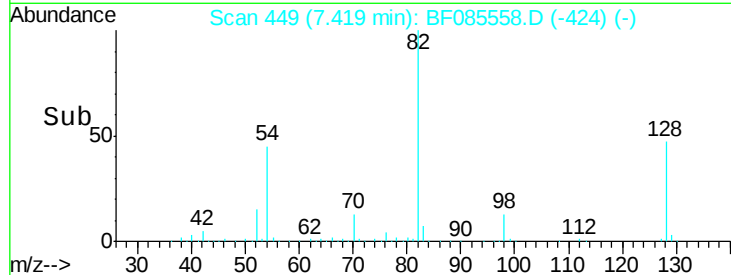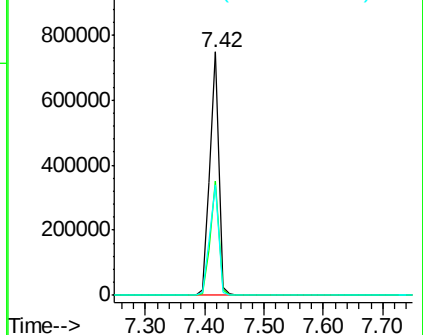

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.89 min Scan# 665

Delta R.T. -0.01 min

Lab File: BF085558.D

Acq: 19 Mar 2016 7:03


Tgt Ion: 164 Resp: 231288

Ion Ratio Lower Upper

164 100

162 101.1 82.1 123.1



160 46.0 37.4 56.2

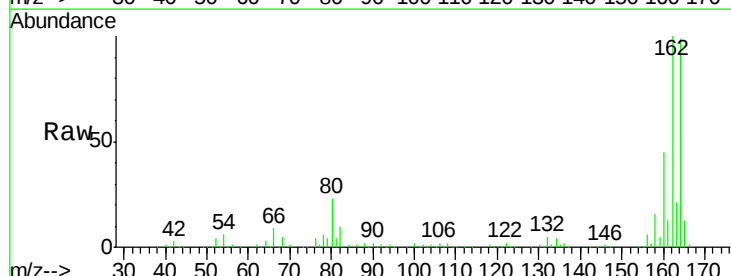


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

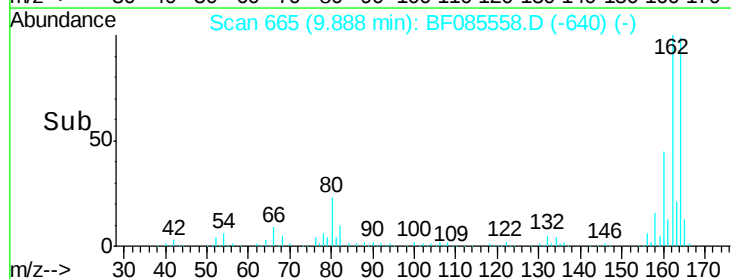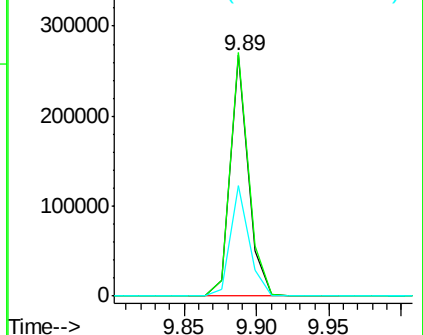


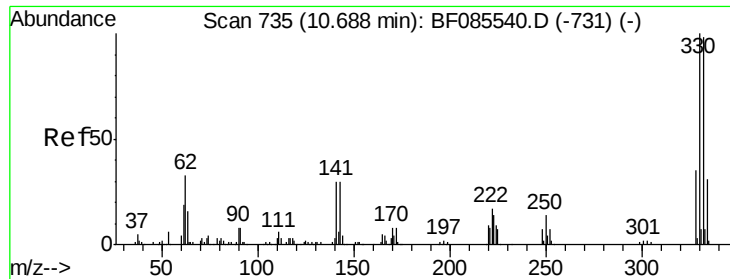




#41  
 2,4,6-Tribromophenol  
 Concen: 138.01 ng  
 RT: 10.68 min Scan# 734  
 Delta R.T. -0.01 min  
 Lab File: BF085558.D  
 Acq: 19 Mar 2016 7:03

Instrument :  
 BNA\_F  
 ClientSampleId :  
 TW-5

Tgt Ion:330 Resp: 312676  
 Ion Ratio Lower Upper  
 330 100  
 332 97.0 78.2 117.2  
 141 31.2 31.5 47.3#

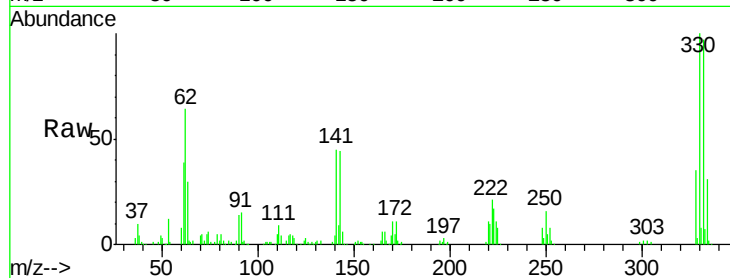


Abundance Ion 329.80 (329.50 to 330.50): E  
 Ion 331.80 (331.50 to 332.50): E  
 Ion 141.00 (140.70 to 141.70): E

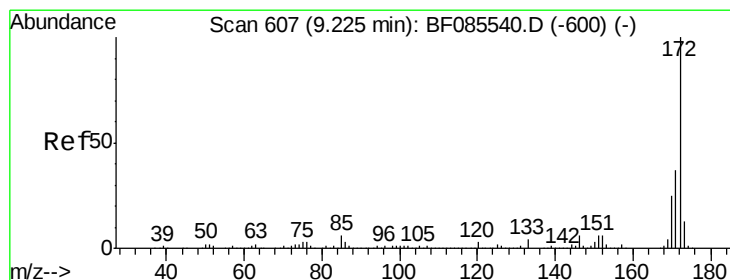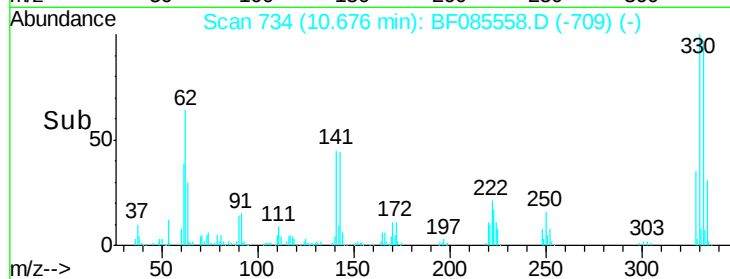
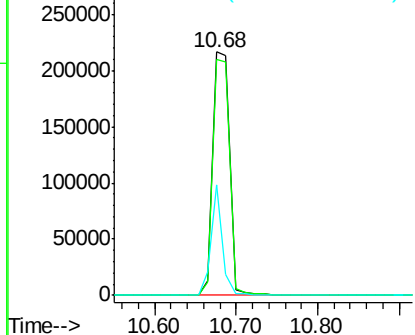



#44  
 2-Fluorobiphenyl  
 Concen: 91.06 ng  
 RT: 9.21 min Scan# 606  
 Delta R.T. -0.01 min  
 Lab File: BF085558.D  
 Acq: 19 Mar 2016 7:03

Tgt Ion:172 Resp: 1212581  
 Ion Ratio Lower Upper  
 172 100  
 171 36.6 29.4 44.2  
 170 24.6 19.8 29.6

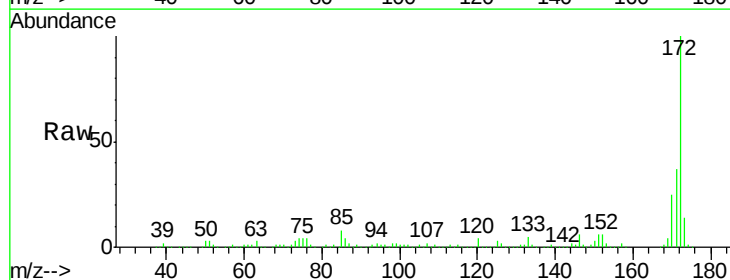

Abundance Ion 172.00 (171.70 to 172.70): E  
 Ion 171.00 (170.70 to 171.70): E  
 Ion 170.00 (169.70 to 170.70): E



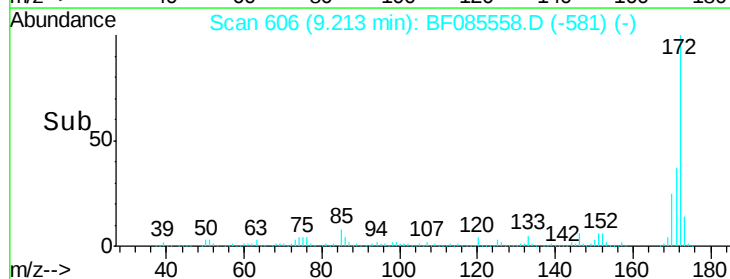
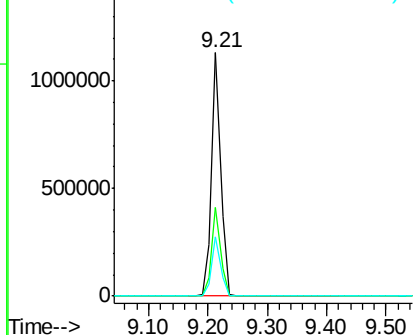


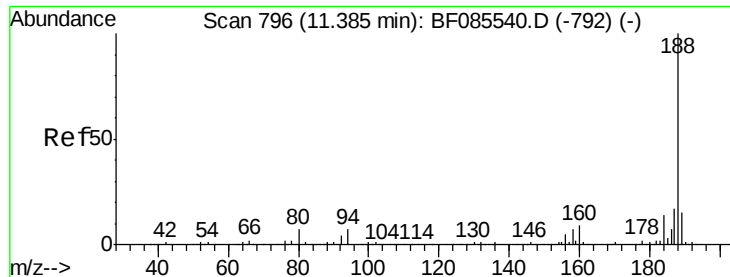

#63  
Phenanthrene-d10  
Concen: 20.00 ng  
RT: 11.37 min Scan# 795  
Delta R.T. -0.01 min  
Lab File: BF085558.D  
Acq: 19 Mar 2016 7:03




Instrument :  
BNA\_F  
ClientSampleId :  
TW-5


Tgt Ion:188 Resp: 452376  
Ion Ratio Lower Upper  
188 100  
94 9.2 5.4 8.0#  
80 9.6 5.5 8.3#

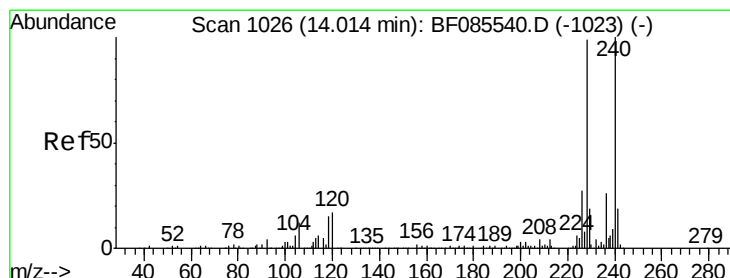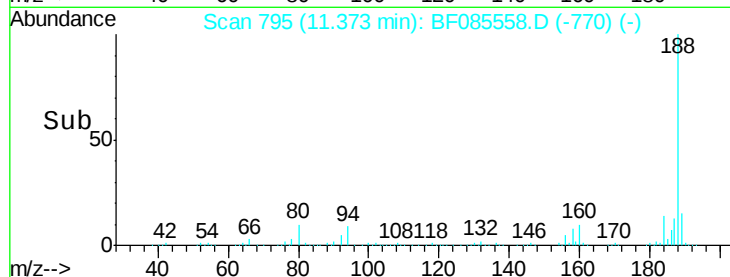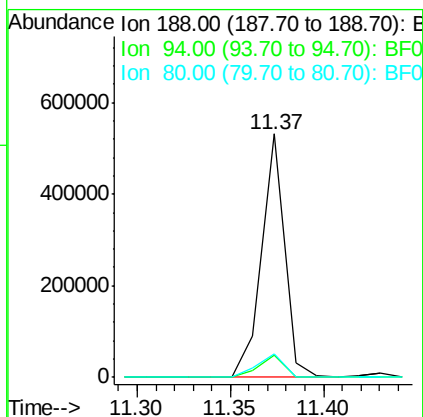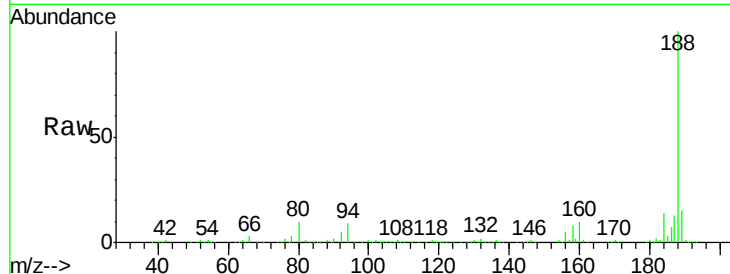

#75  
Chrysene-d12  
Concen: 20.00 ng  
RT: 14.00 min Scan# 1025  
Delta R.T. -0.01 min  
Lab File: BF085558.D  
Acq: 19 Mar 2016 7:03

Tgt Ion:240 Resp: 351406  
Ion Ratio Lower Upper  
240 100  
120 16.5 13.8 20.8  
236 26.6 20.6 30.8


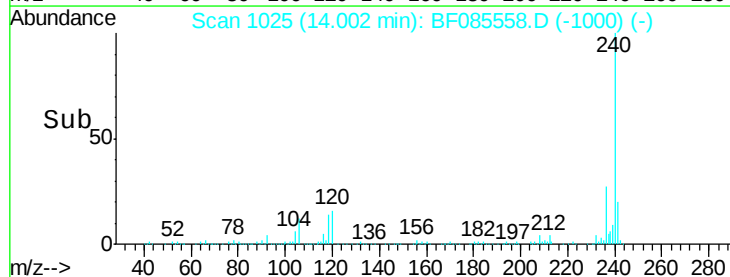
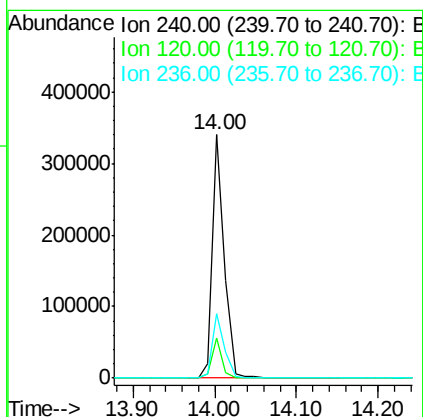
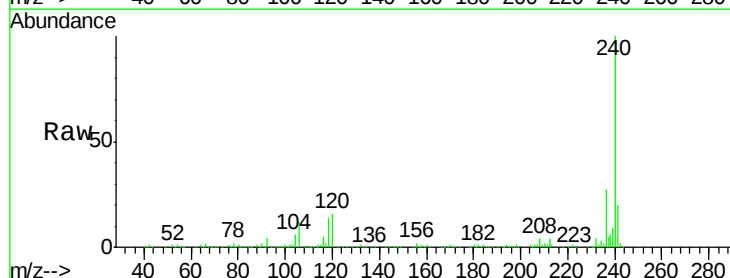


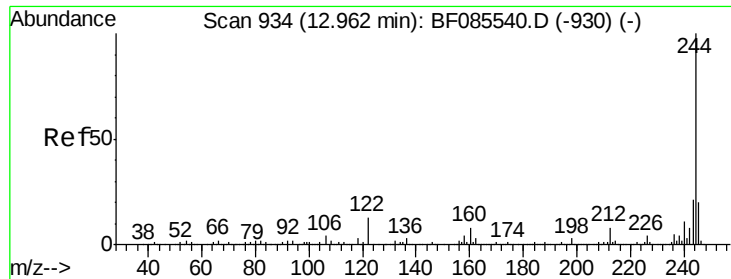

#78  
 Terphenyl-d14  
 Concen: 87.82 ng  
 RT: 12.96 min Scan# 934  
 Delta R.T. 0.00 min  
 Lab File: BF085558.D  
 Acq: 19 Mar 2016 7:03

Instrument :  
 BNA\_F  
 ClientSampleId :  
 TW-5

Tgt Ion:244 Resp: 1282441  
 Ion Ratio Lower Upper  
 244 100  
 212 7.2 6.1 9.1  
 122 10.2 10.2 15.4#

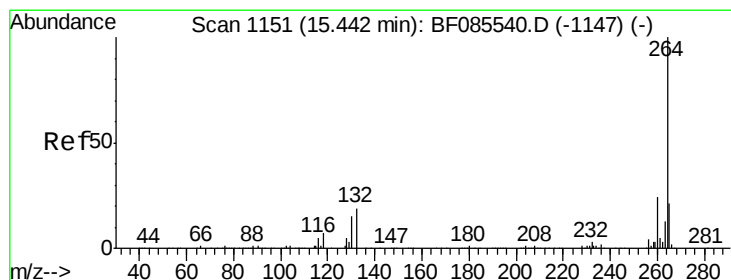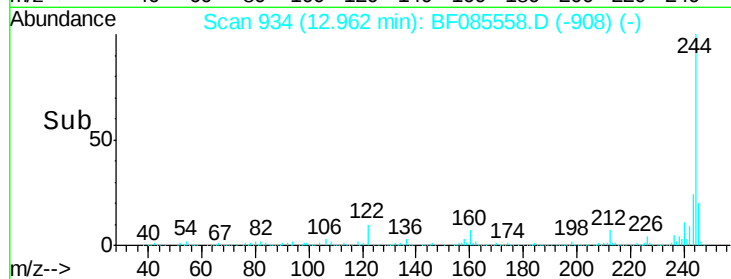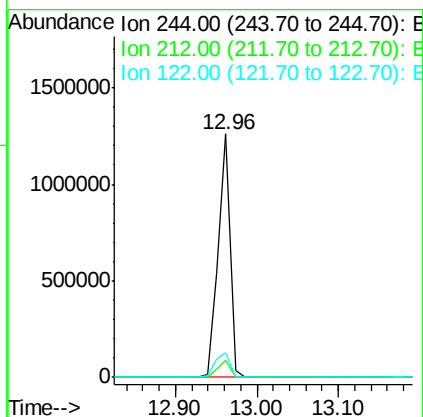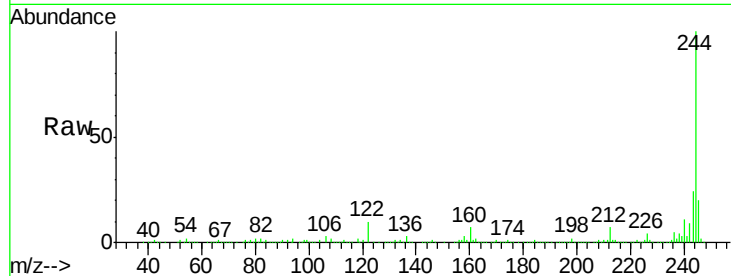

#86  
 Perylene-d12  
 Concen: 20.00 ng  
 RT: 15.43 min Scan# 1150  
 Delta R.T. -0.01 min  
 Lab File: BF085558.D  
 Acq: 19 Mar 2016 7:03

Tgt Ion:264 Resp: 295516  
 Ion Ratio Lower Upper  
 264 100  
 260 24.7 19.4 29.2  
 265 21.3 17.2 25.8

