

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
 Data File : BF085555.D
 Acq On : 19 Mar 2016 5:40
 Operator : UM/SJ
 Sample : H1788-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TW-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.442	274	276	279	rBV	1267974	1382307	34.76%	5.318%
2	6.470	364	366	369	rBV	632623	874059	21.98%	3.363%
3	6.619	376	379	381	rBV	2771446	2691543	67.67%	10.355%
4	6.847	397	399	402	rBV	678413	757993	19.06%	2.916%
5	7.007	410	413	416	rBV	2668091	2538962	63.84%	9.768%
6	7.419	446	449	451	rBV	2161713	2232986	56.14%	8.590%
7	8.139	509	512	514	rBV	1127737	1044359	26.26%	4.018%
8	9.213	603	606	609	rBV	3532305	3701304	93.06%	14.239%
9	9.888	663	665	668	rBV	1149044	1088825	27.38%	4.189%
10	10.676	731	734	737	rBV2	1902010	2394669	60.21%	9.212%
11	11.374	792	795	797	rBV	1371048	1167166	29.35%	4.490%
12	12.688	908	910	913	rBV	44140	55428	1.39%	0.213%
13	12.768	916	917	921	rVB	24245	41114	1.03%	0.158%
14	12.962	931	934	936	rBV	4005738	3977266	100.00%	15.301%
15	14.002	1023	1025	1028	rBV	1010241	1065294	26.78%	4.098%
16	14.631	1079	1080	1083	rVB2	90586	103563	2.60%	0.398%
17	15.431	1147	1150	1153	rBV	699641	876867	22.05%	3.373%


Sum of corrected areas: 25993705

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085555.D
Acq On : 19 Mar 2016 5:40
Operator : UM/SJ
Sample : H1788-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

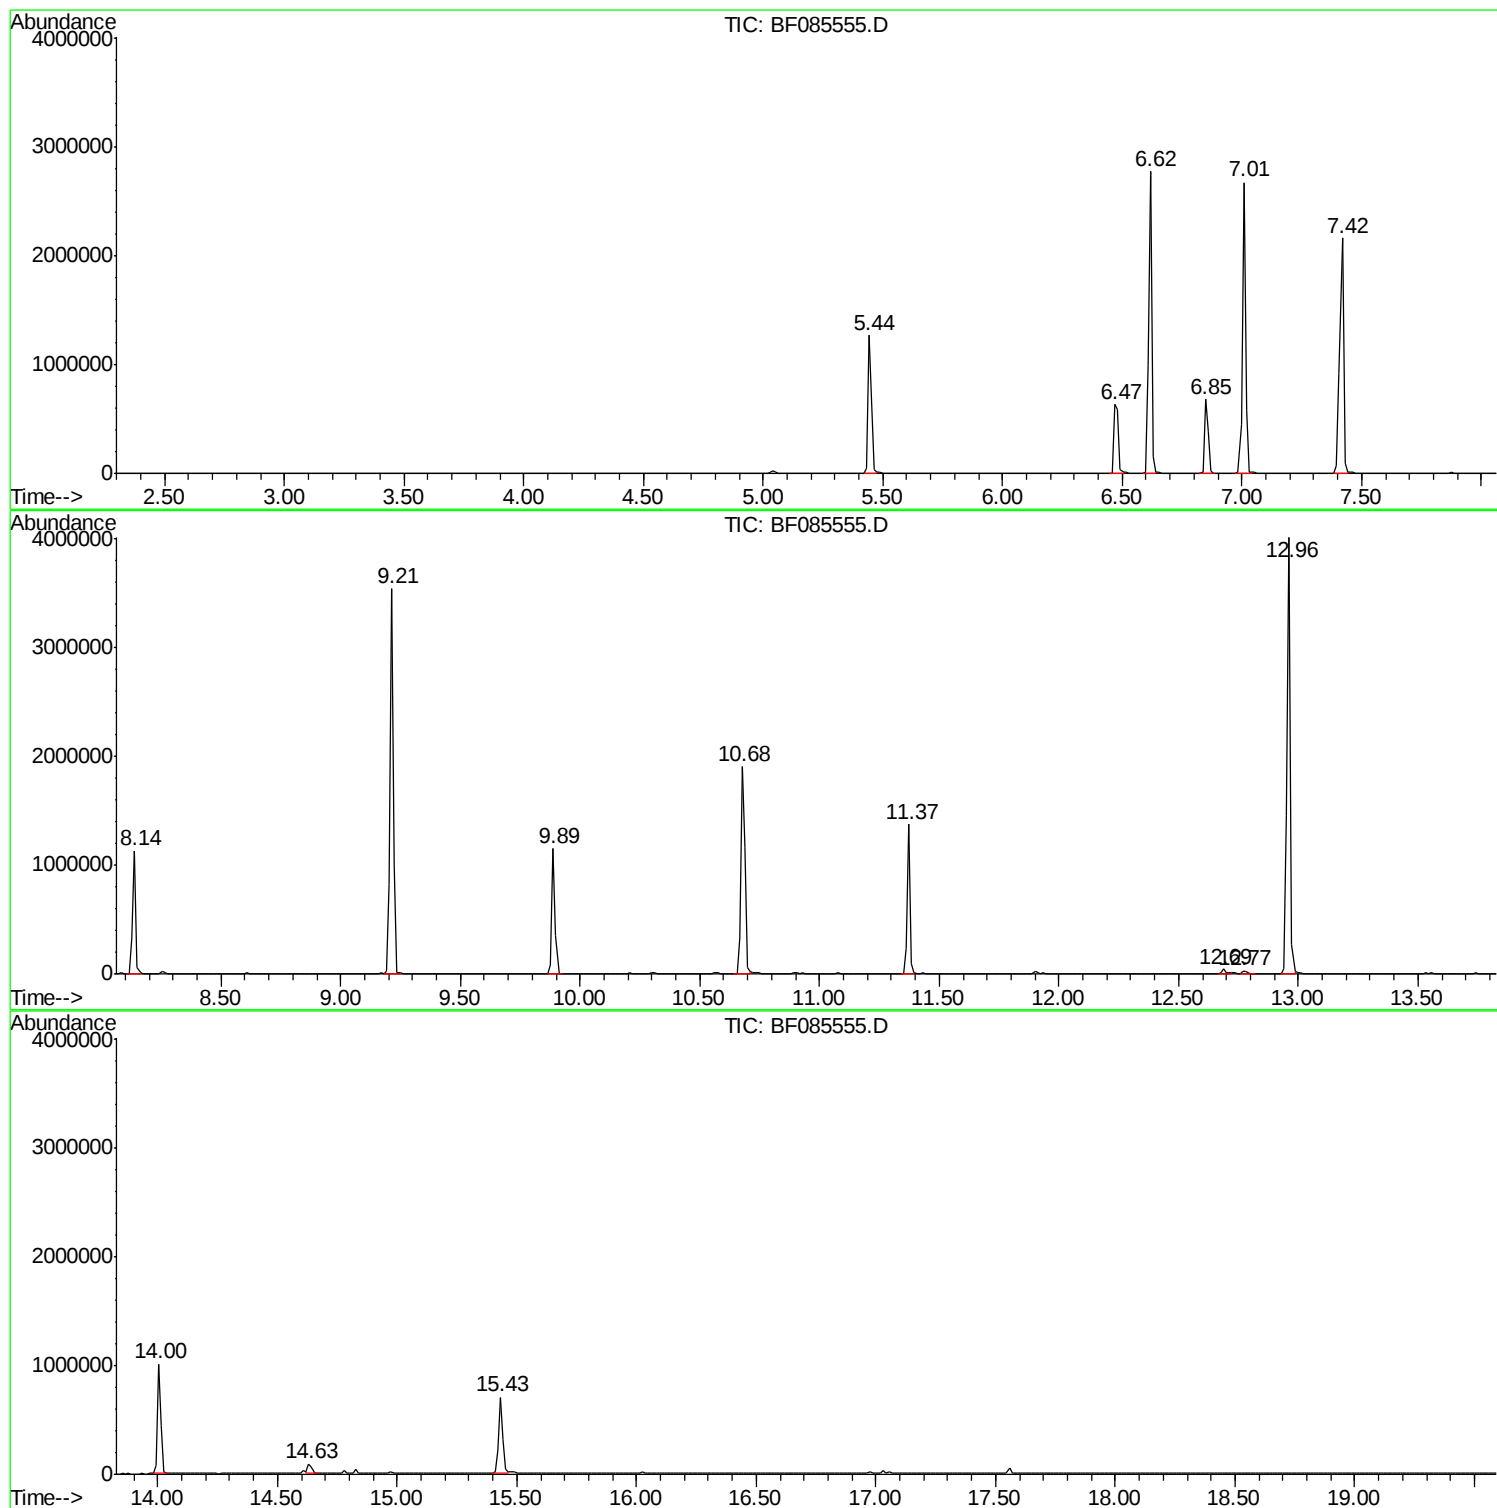

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085555.D
Acq On : 19 Mar 2016 5:40
Operator : UM/SJ
Sample : H1788-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	71.02 ng	2691540	1,4-Dichlorobenzene-d4	6.85

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
4			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

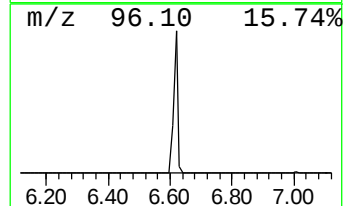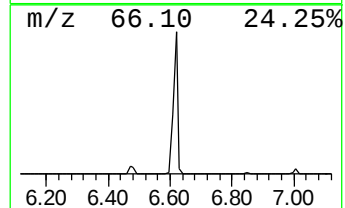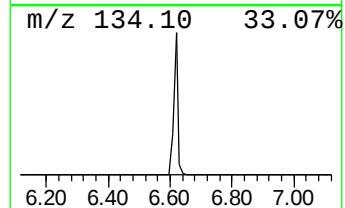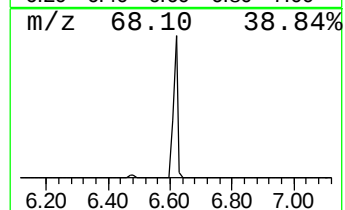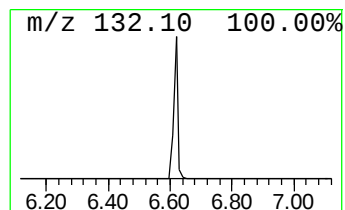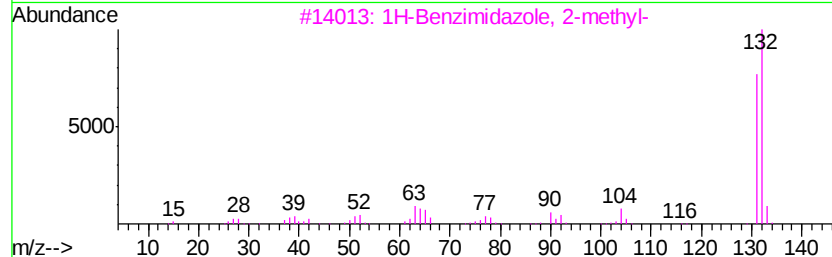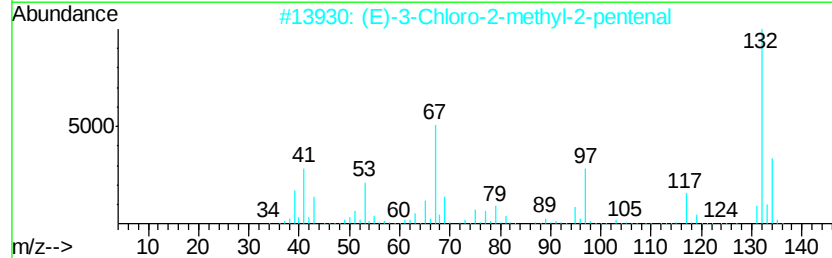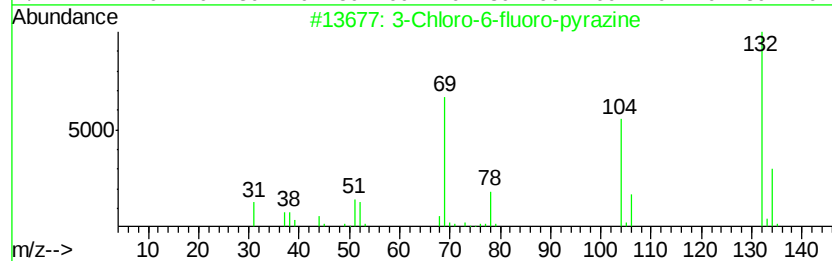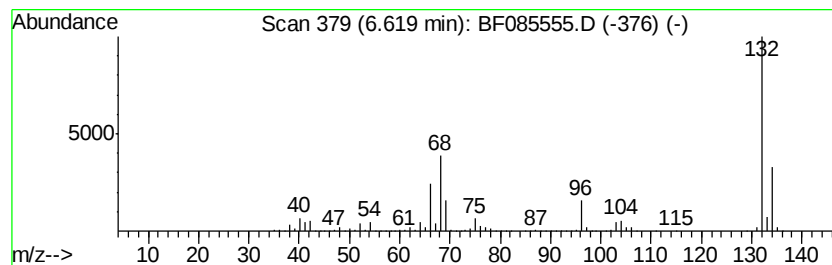

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085555.D
Acq On : 19 Mar 2016 5:40
Operator : UM/SJ
Sample : H1788-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.62	6.62	71.0	ng	2691540	1	6.85	757993	20.0