

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
 Data File : BF085557.D
 Acq On : 19 Mar 2016 6:35
 Operator : UM/SJ
 Sample : H1788-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TW-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.030	239	240	246	rBV	29802	46179	1.12%	0.174%
2	5.441	274	276	279	rBV	1327929	1510651	36.73%	5.682%
3	6.482	364	367	369	rBV	801496	1035668	25.18%	3.895%
4	6.619	376	379	381	rBV	2871928	2742364	66.68%	10.314%
5	6.847	397	399	402	rBV	700792	797970	19.40%	3.001%
6	7.007	410	413	416	rBV	2619684	2509232	61.01%	9.438%
7	7.419	446	449	451	rBV	2151860	2233158	54.30%	8.399%
8	8.082	504	507	509	rBV	53238	49622	1.21%	0.187%
9	8.139	509	512	514	rBV	1173473	1067947	25.97%	4.017%
10	9.213	603	606	609	rBV	3503995	3678896	89.46%	13.837%
11	9.888	663	665	668	rBV	1160082	1116757	27.15%	4.200%
12	10.676	731	734	737	rBV2	1936005	2488400	60.51%	9.359%
13	11.373	793	795	797	rBV	1401881	1186456	28.85%	4.462%
14	12.688	907	910	916	rBV	30994	41458	1.01%	0.156%
15	12.779	916	918	921	rBV	91276	97970	2.38%	0.368%
16	12.962	931	934	936	rBV	4037331	4112529	100.00%	15.468%
17	14.002	1023	1025	1028	rBV	1066942	1037045	25.22%	3.900%
18	15.431	1147	1150	1153	rBV	704724	835361	20.31%	3.142%


Sum of corrected areas: 26587663

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085557.D
Acq On : 19 Mar 2016 6:35
Operator : UM/SJ
Sample : H1788-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-4

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

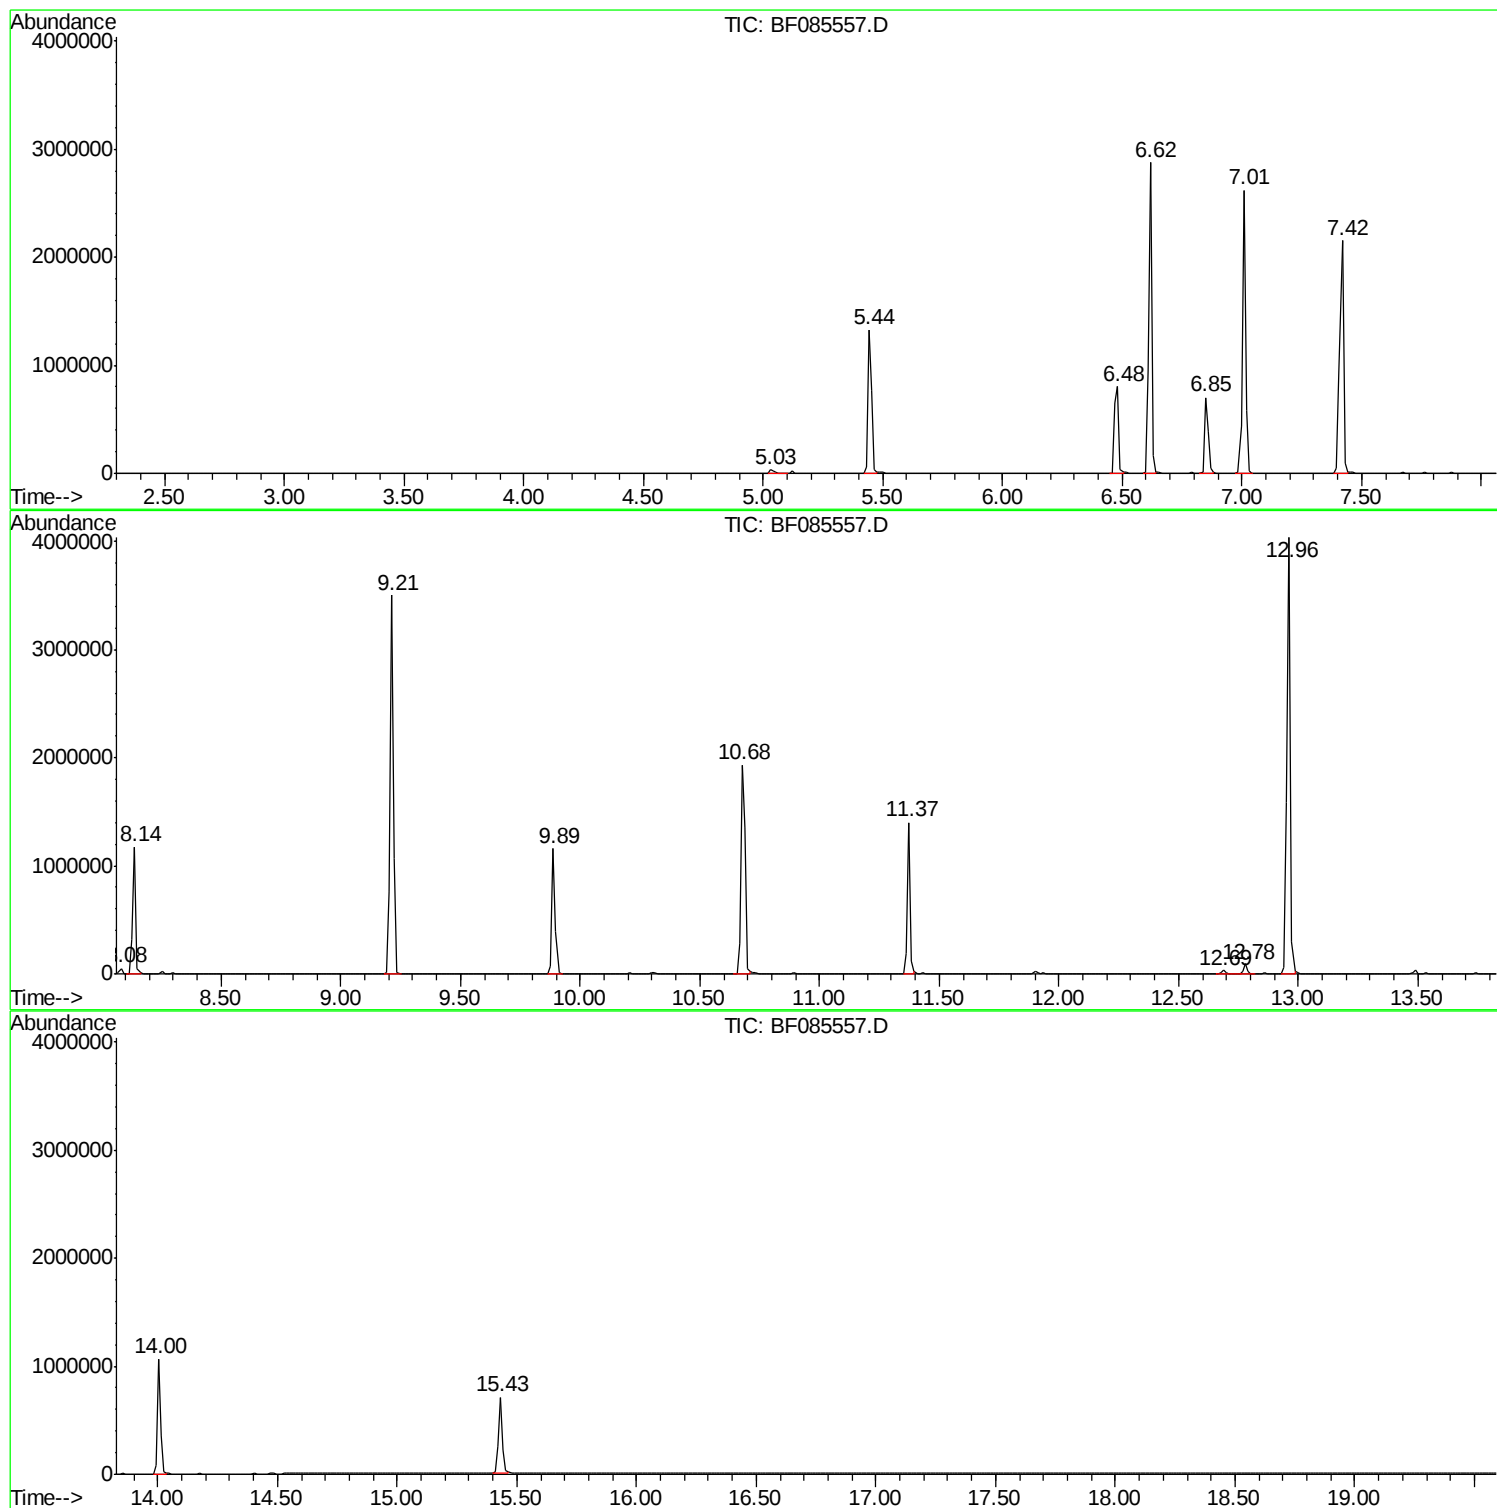

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085557.D
Acq On : 19 Mar 2016 6:35
Operator : UM/SJ
Sample : H1788-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-4










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	68.73 ng	2742360	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

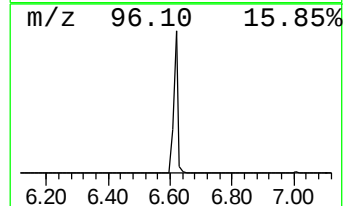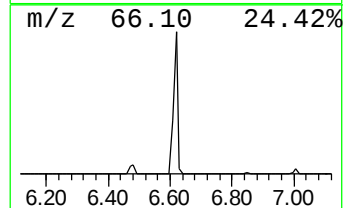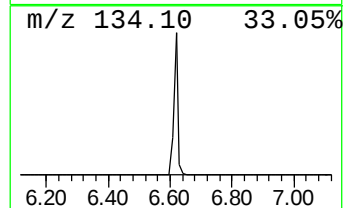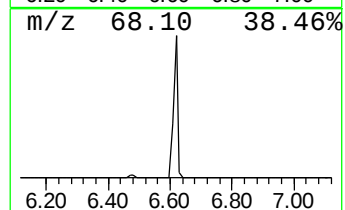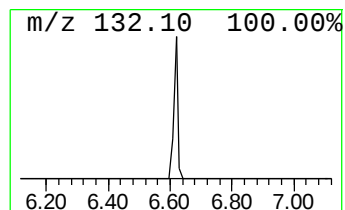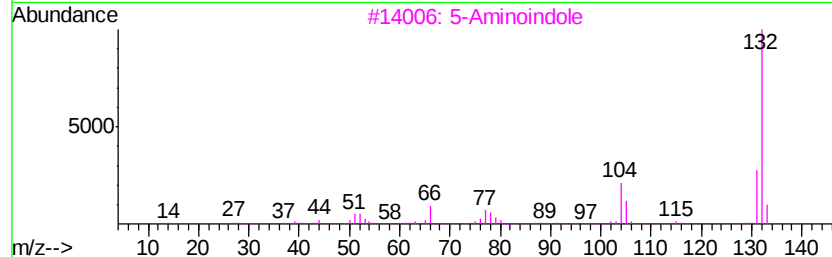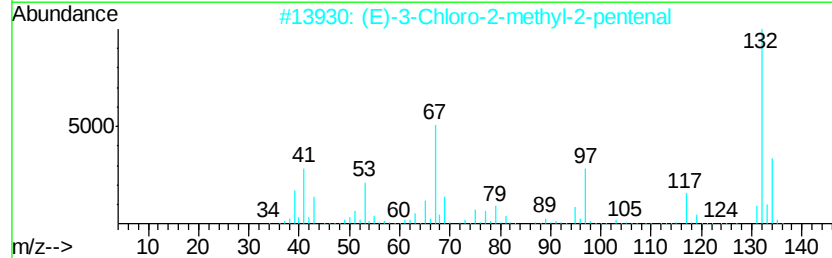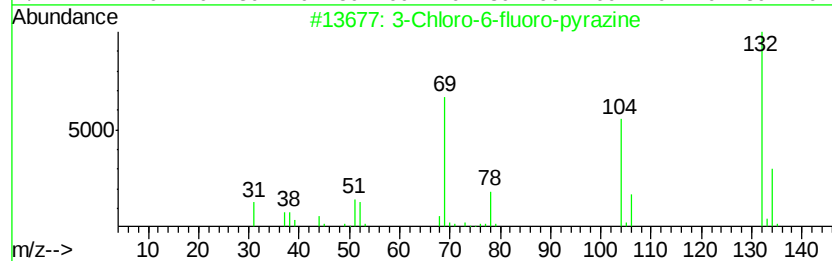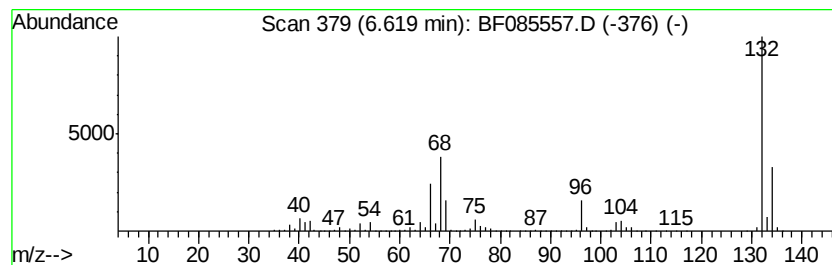

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085557.D
Acq On : 19 Mar 2016 6:35
Operator : UM/SJ
Sample : H1788-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-4

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.62	6.62	68.7	ng	2742360	1	6.85	797970	20.0