

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
 Data File : BF085584.D
 Acq On : 19 Mar 2016 20:28
 Operator : UM/SJ
 Sample : H1799-10 25X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AOU2-SB37A(COMP7-21)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.441	274	276	283	rBV	108482	107870	9.45%	1.442%
2	6.470	365	366	373	rBV	78201	115126	10.09%	1.539%
3	6.619	377	379	381	rBV	121134	122519	10.74%	1.638%
4	6.847	397	399	402	rBV	733224	768514	67.35%	10.275%
5	7.007	411	413	415	rBV	124788	105887	9.28%	1.416%
6	7.407	446	448	451	rBV	44235	64861	5.68%	0.867%
7	8.139	509	512	514	rBV	1300302	1141045	100.00%	15.256%
8	8.847	572	574	578	rVB	13731	14597	1.28%	0.195%
9	9.213	603	606	608	rBV	178013	151170	13.25%	2.021%
10	9.750	651	653	655	rBV	25883	20245	1.77%	0.271%
11	9.887	663	665	667	rBV	1172958	1080715	94.71%	14.449%
12	10.093	681	683	685	rBV	28955	24090	2.11%	0.322%
13	10.287	689	700	701	rBV2	11008	50059	4.39%	0.669%
14	10.436	711	713	715	rVB	105451	86041	7.54%	1.150%
15	10.676	732	734	737	rBV	70833	69769	6.11%	0.933%
16	11.373	792	795	796	rBV	1207853	1053470	92.33%	14.085%
17	11.396	796	797	799	rVV	188125	138810	12.17%	1.856%
18	11.442	799	801	804	rVB2	18838	24227	2.12%	0.324%
19	11.876	836	839	840	rBV	13508	14886	1.30%	0.199%
20	11.899	840	841	843	rVB	15936	14246	1.25%	0.190%
21	11.979	847	848	852	rBV3	20267	38422	3.37%	0.514%
22	12.585	899	901	903	rVB	104343	90188	7.90%	1.206%
23	12.813	918	921	923	rVB	74168	83644	7.33%	1.118%
24	12.951	931	933	936	rVB	131475	113206	9.92%	1.514%
25	13.133	946	949	951	rVB	11765	20655	1.81%	0.276%
26	13.236	957	958	962	rVB2	9113	13272	1.16%	0.177%
27	13.511	981	982	989	rVB4	8341	18377	1.61%	0.246%
28	14.002	1023	1025	1032	rBV	763336	805954	70.63%	10.776%
29	14.391	1054	1059	1061	rBV3	12623	23375	2.05%	0.313%
30	15.019	1112	1114	1119	rBV	38133	75981	6.66%	1.016%
31	15.317	1138	1140	1142	rVB	18523	24629	2.16%	0.329%
32	15.374	1142	1145	1147	rVB	32088	41959	3.68%	0.561%
33	15.431	1147	1150	1153	rBV	582325	725985	63.62%	9.707%
34	15.739	1174	1177	1179	rBV4	6305	15936	1.40%	0.213%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085584.D
Acq On : 19 Mar 2016 20:28
Operator : UM/SJ
Sample : H1799-10 25X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AOU2-SB37A(COMP7-21)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.945	1193	1195	1196	rBV2	22282	17720	1.55%	0.237%
36	16.357	1228	1231	1234	rBV3	15046	29286	2.57%	0.392%
37	16.528	1245	1246	1251	rVB5	11243	16930	1.48%	0.226%
38	16.825	1269	1272	1276	rBV2	16293	39733	3.48%	0.531%
39	17.237	1305	1308	1311	rBV	12985	28709	2.52%	0.384%
40	17.923	1366	1368	1371	rBV4	8488	15392	1.35%	0.206%
41	18.037	1376	1378	1382	rVV4	7869	16357	1.43%	0.219%
42	18.128	1384	1386	1393	rVB7	11645	34063	2.99%	0.455%
43	18.425	1411	1412	1414	rVB2	30649	21344	1.87%	0.285%


Sum of corrected areas: 7479264

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085584.D
Acq On : 19 Mar 2016 20:28
Operator : UM/SJ
Sample : H1799-10 25X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AOU2-SB37A(COMP7-21)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

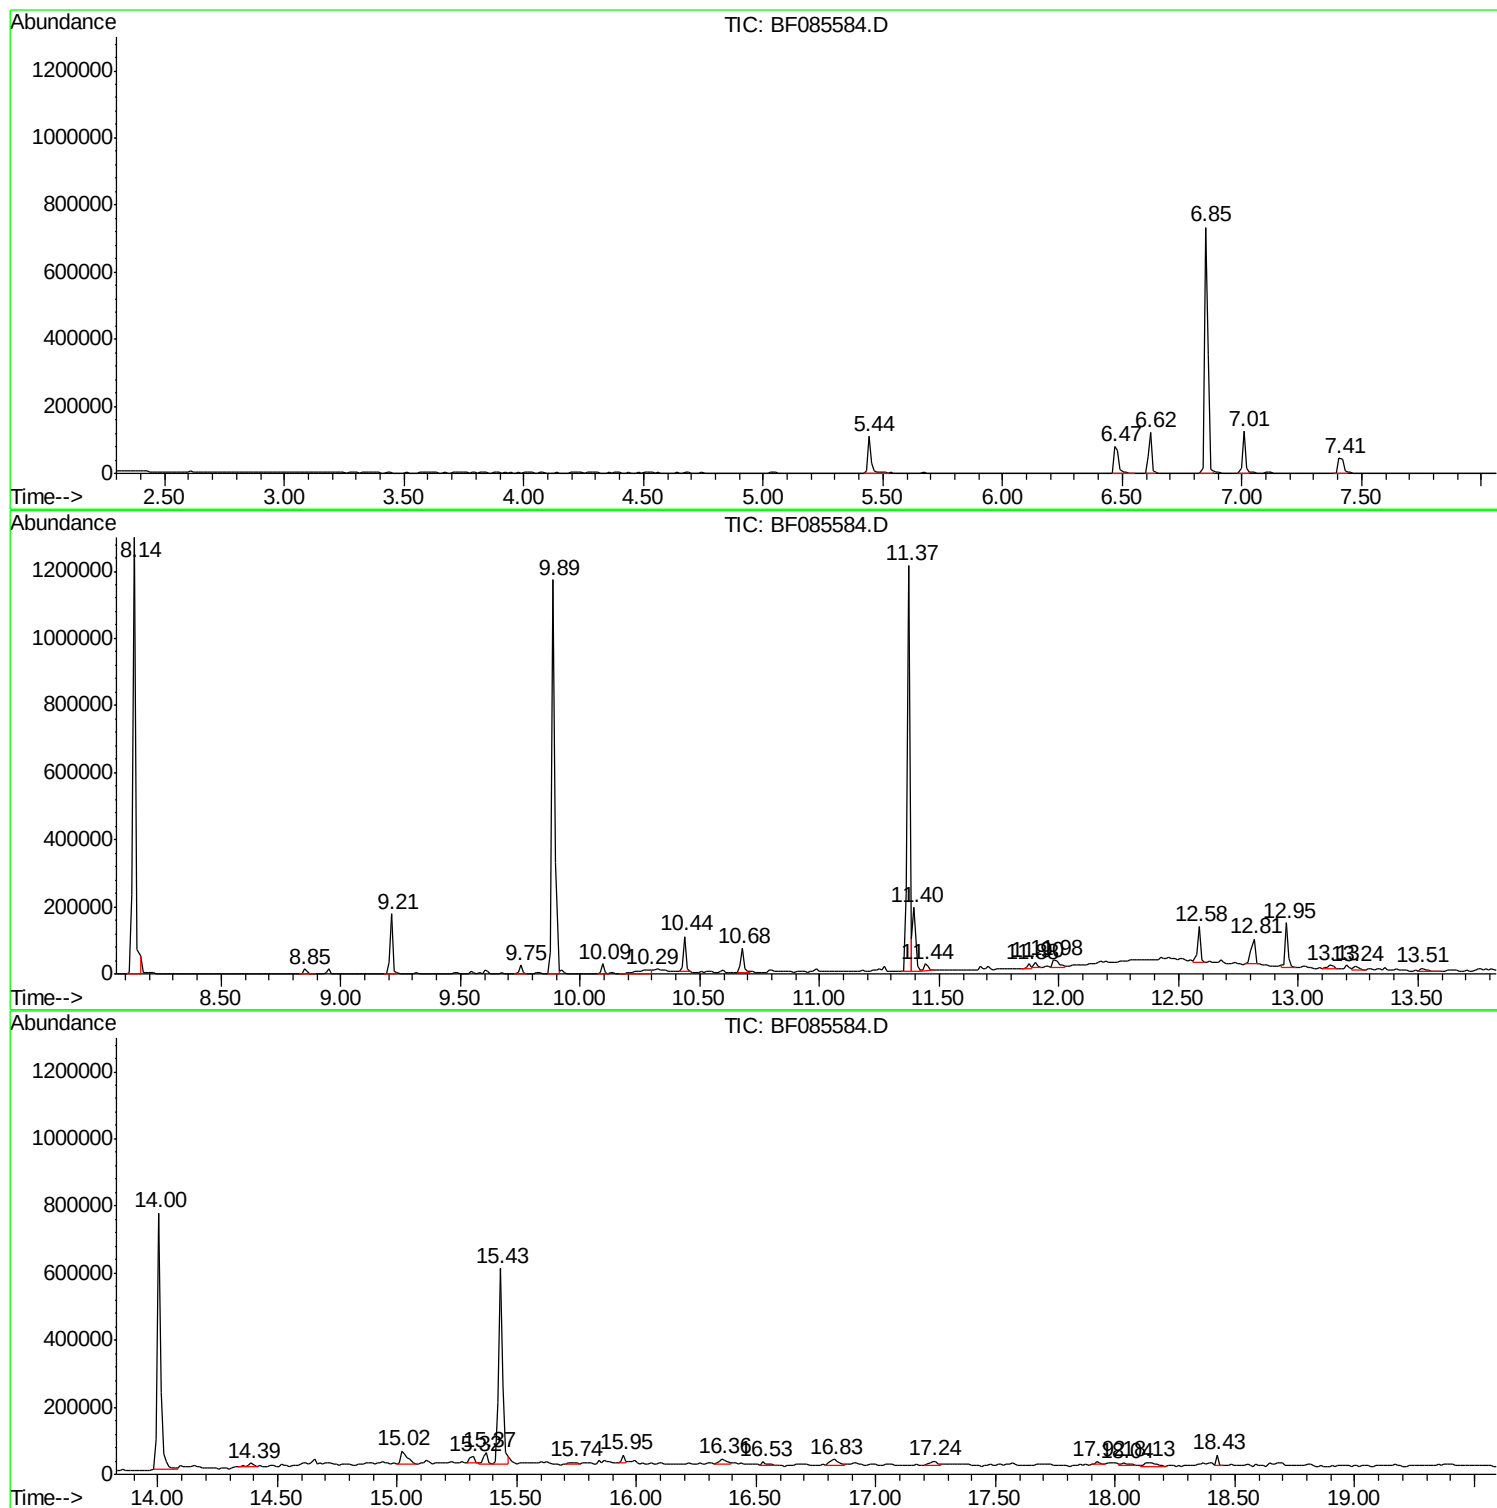

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085584.D
Acq On : 19 Mar 2016 20:28
Operator : UM/SJ
Sample : H1799-10 25X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AOU2-SB37A(COMP7-21)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	3.19 ng	122519	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
2		Amphetaminil	250	C17H18N2	017590-01-1	12
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Xenon	132	Xe	007440-63-3	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

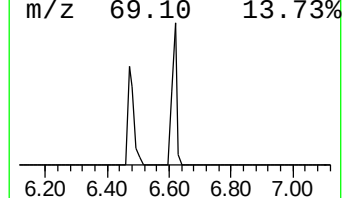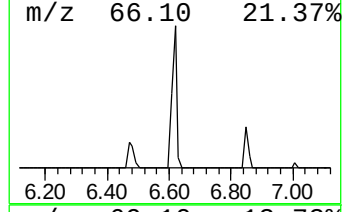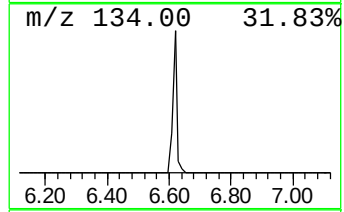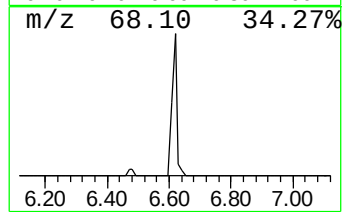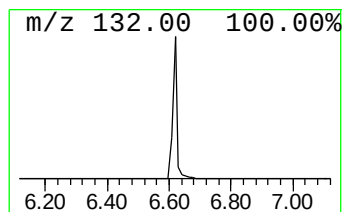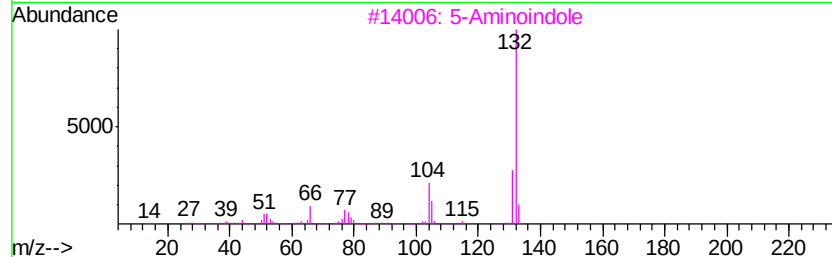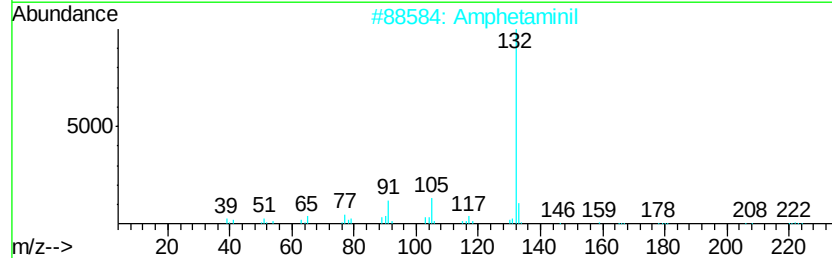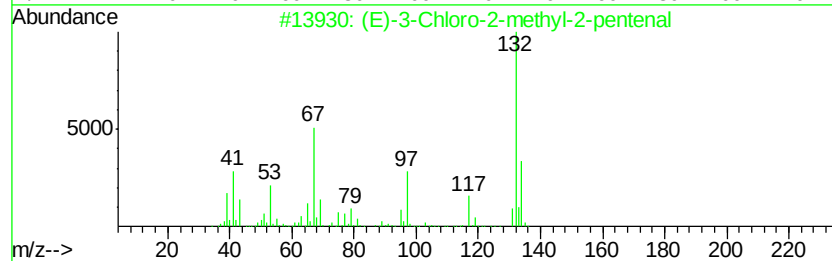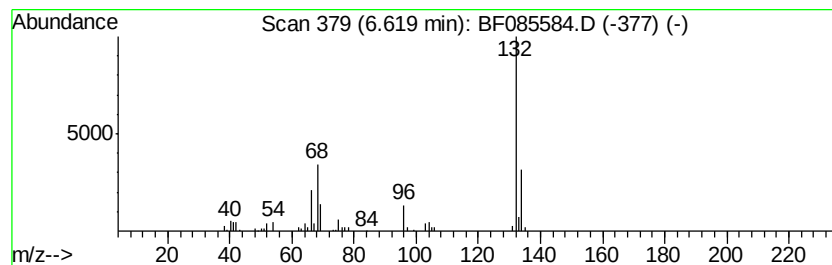

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031816\
Data File : BF085584.D
Acq On : 19 Mar 2016 20:28
Operator : UM/SJ
Sample : H1799-10 25X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AOU2-SB37A(COMP7-21)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.62	6.62	3.2	ng	122519	1	6.85	768514	20.0