


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031816\
 Data File : BF085570.D
 Acq On : 19 Mar 2016 14:00
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 18 23:31:39 2016

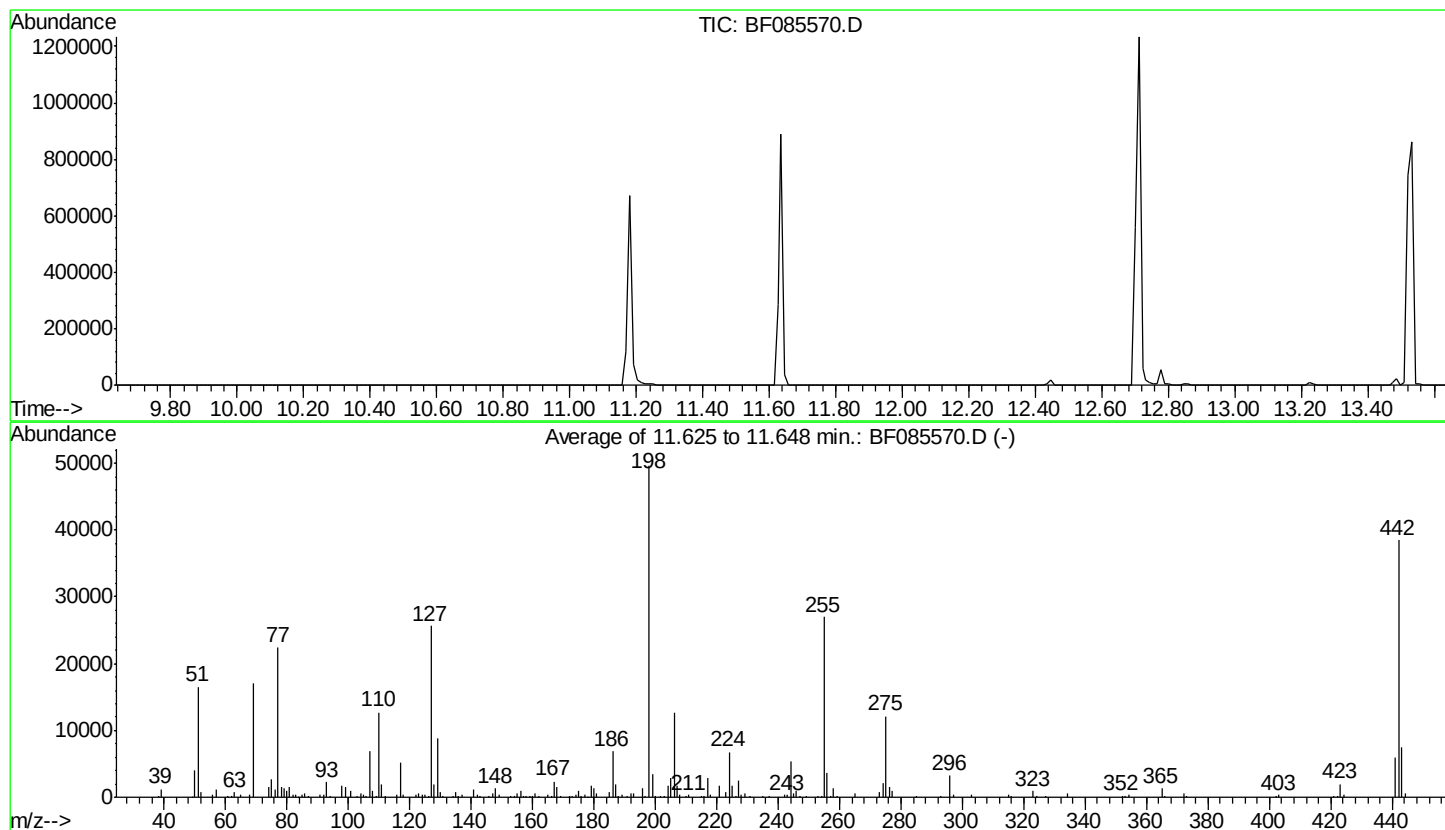

AutoFind: Scans 817, 818, 819; Background Corrected with Scan 814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	16530	PASS
68	69	0.00	2	2.0	339	PASS
69	198	0.00	100	34.3	17010	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	25660	PASS
197	198	0.00	2	0.5	236	PASS
198	198	100	100	100.0	49647	PASS
199	198	5	9	6.8	3365	PASS
275	198	10	60	24.3	12089	PASS
365	198	1	100	2.6	1267	PASS
441	442	0.01	24	15.6	6012	PASS
442	198	50	100	77.5	38469	PASS
443	442	15	24	19.5	7508	PASS