


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF031816\  
 Data File : BF085594.D  
 Acq On : 20 Mar 2016 2:29  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031816.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Mar 18 23:31:39 2016

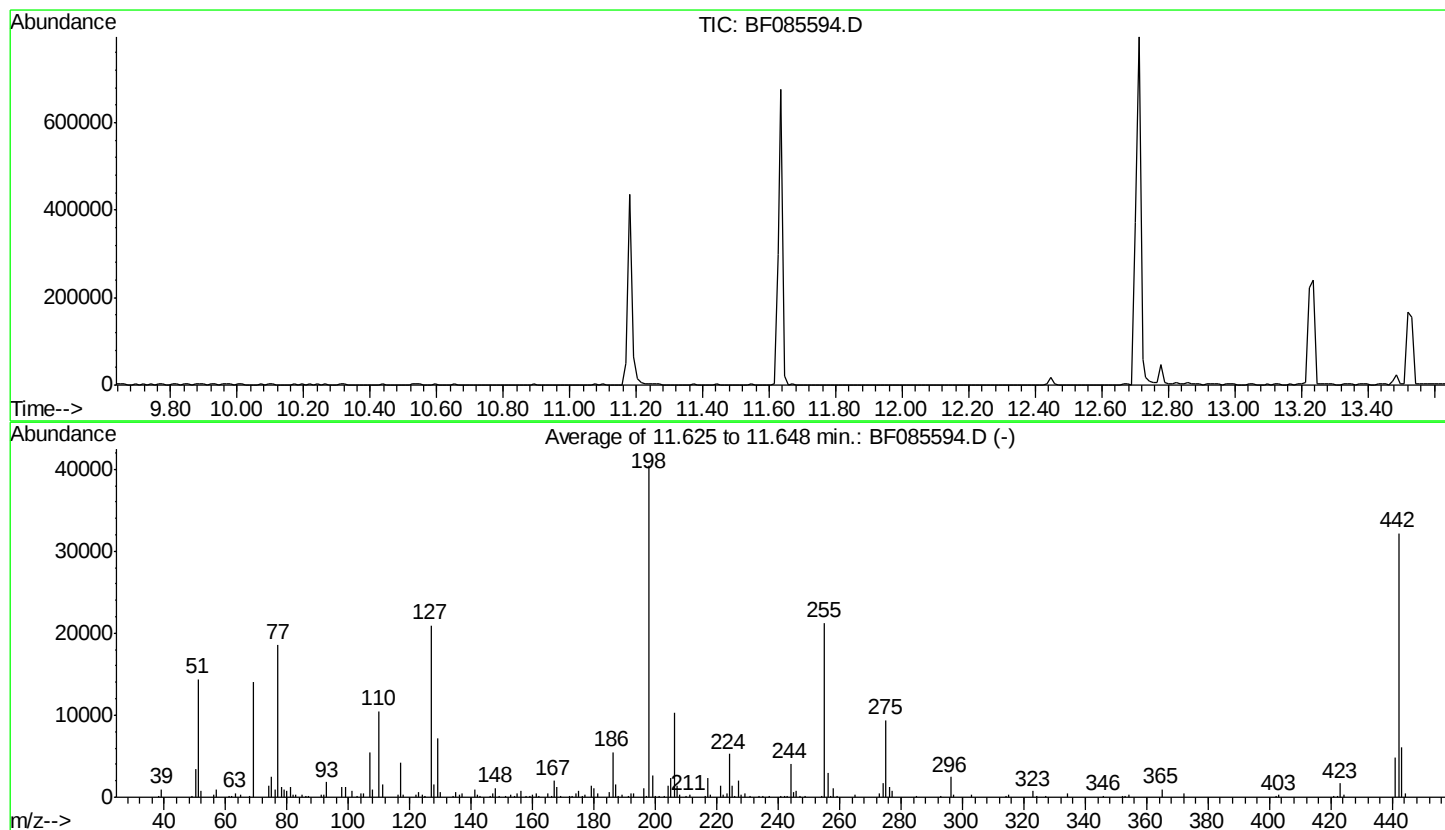

AutoFind: Scans 817, 818, 819; Background Corrected with Scan 814

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.6      | 14408   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 228     | PASS             |
| 69          | 198          | 0.00         | 100          | 34.9      | 14088   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 51.8      | 20936   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 221     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 40423   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 2684    | PASS             |
| 275         | 198          | 10           | 60           | 23.3      | 9414    | PASS             |
| 365         | 198          | 1            | 100          | 2.4       | 983     | PASS             |
| 441         | 442          | 0.01         | 24           | 15.1      | 4866    | PASS             |
| 442         | 198          | 50           | 100          | 79.6      | 32157   | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 6169    | PASS             |