




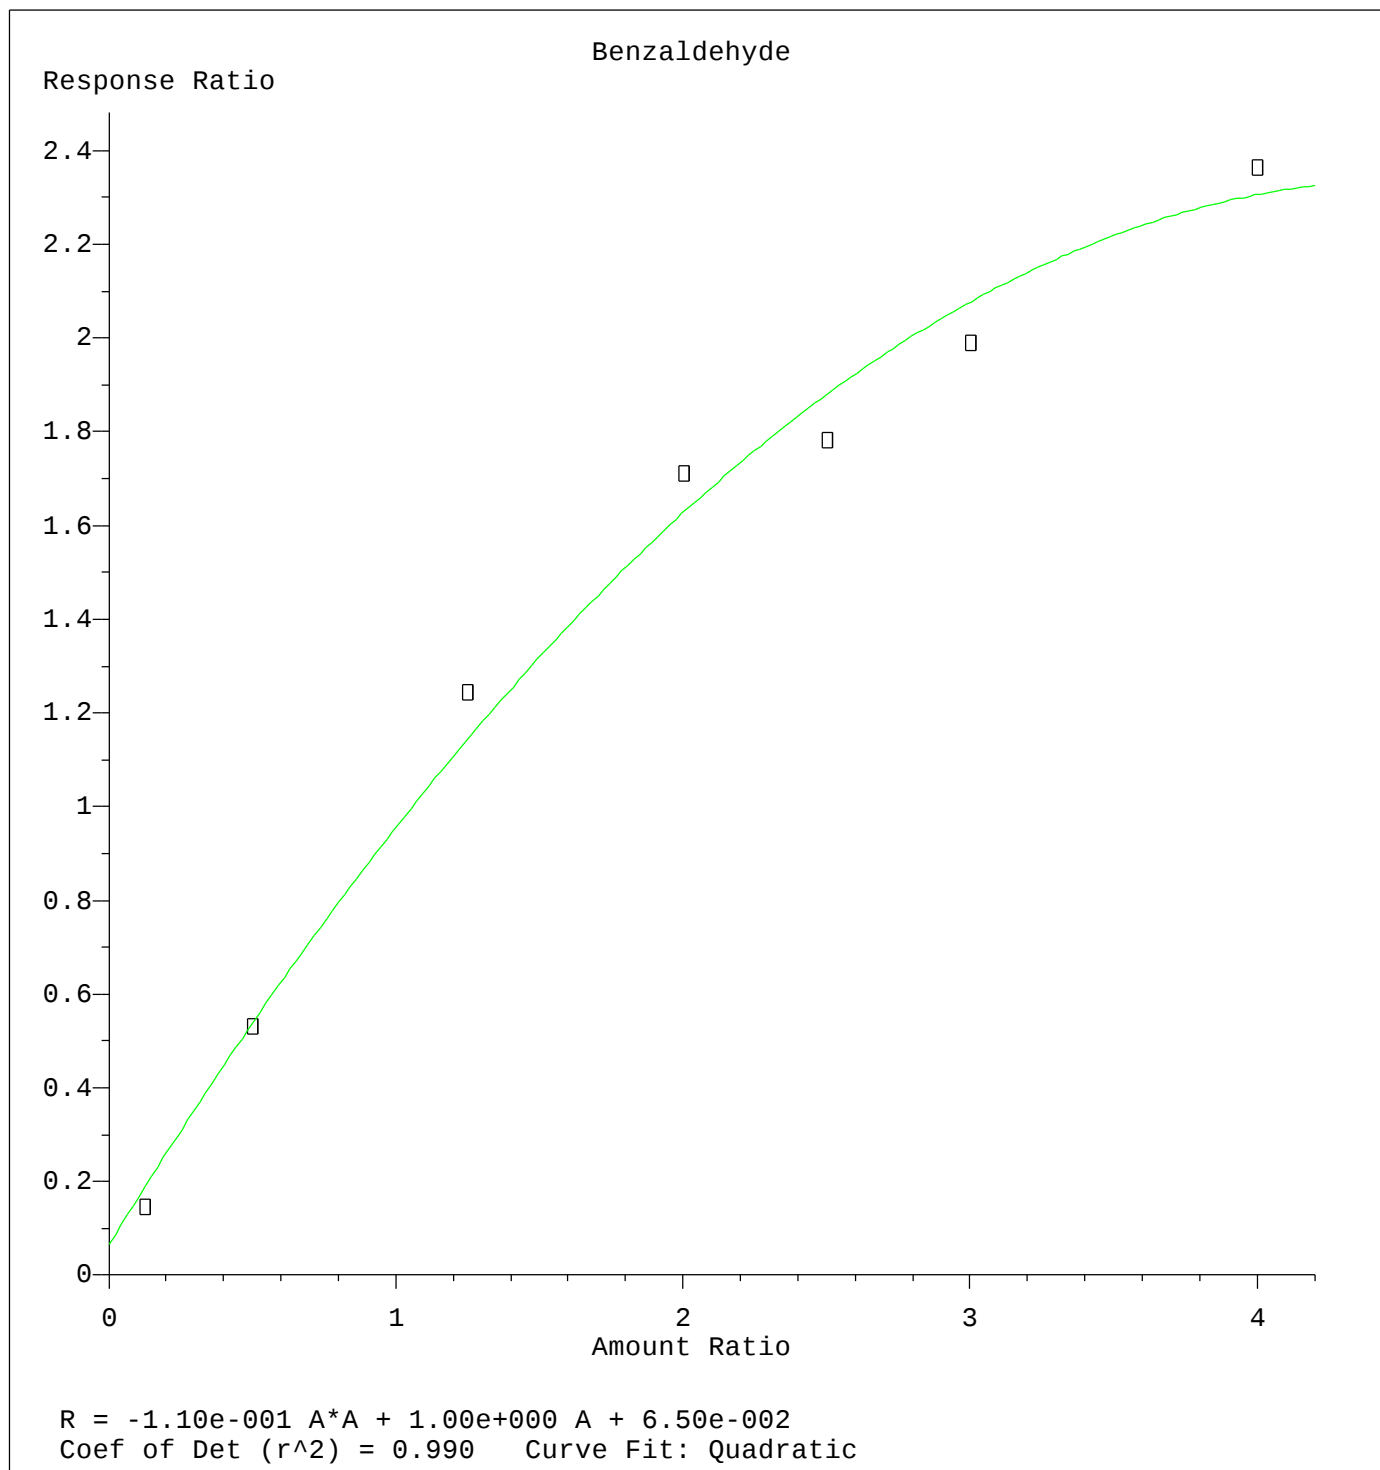

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
Calibration Table Last Updated: Sat Mar 18 05:21:29 2017

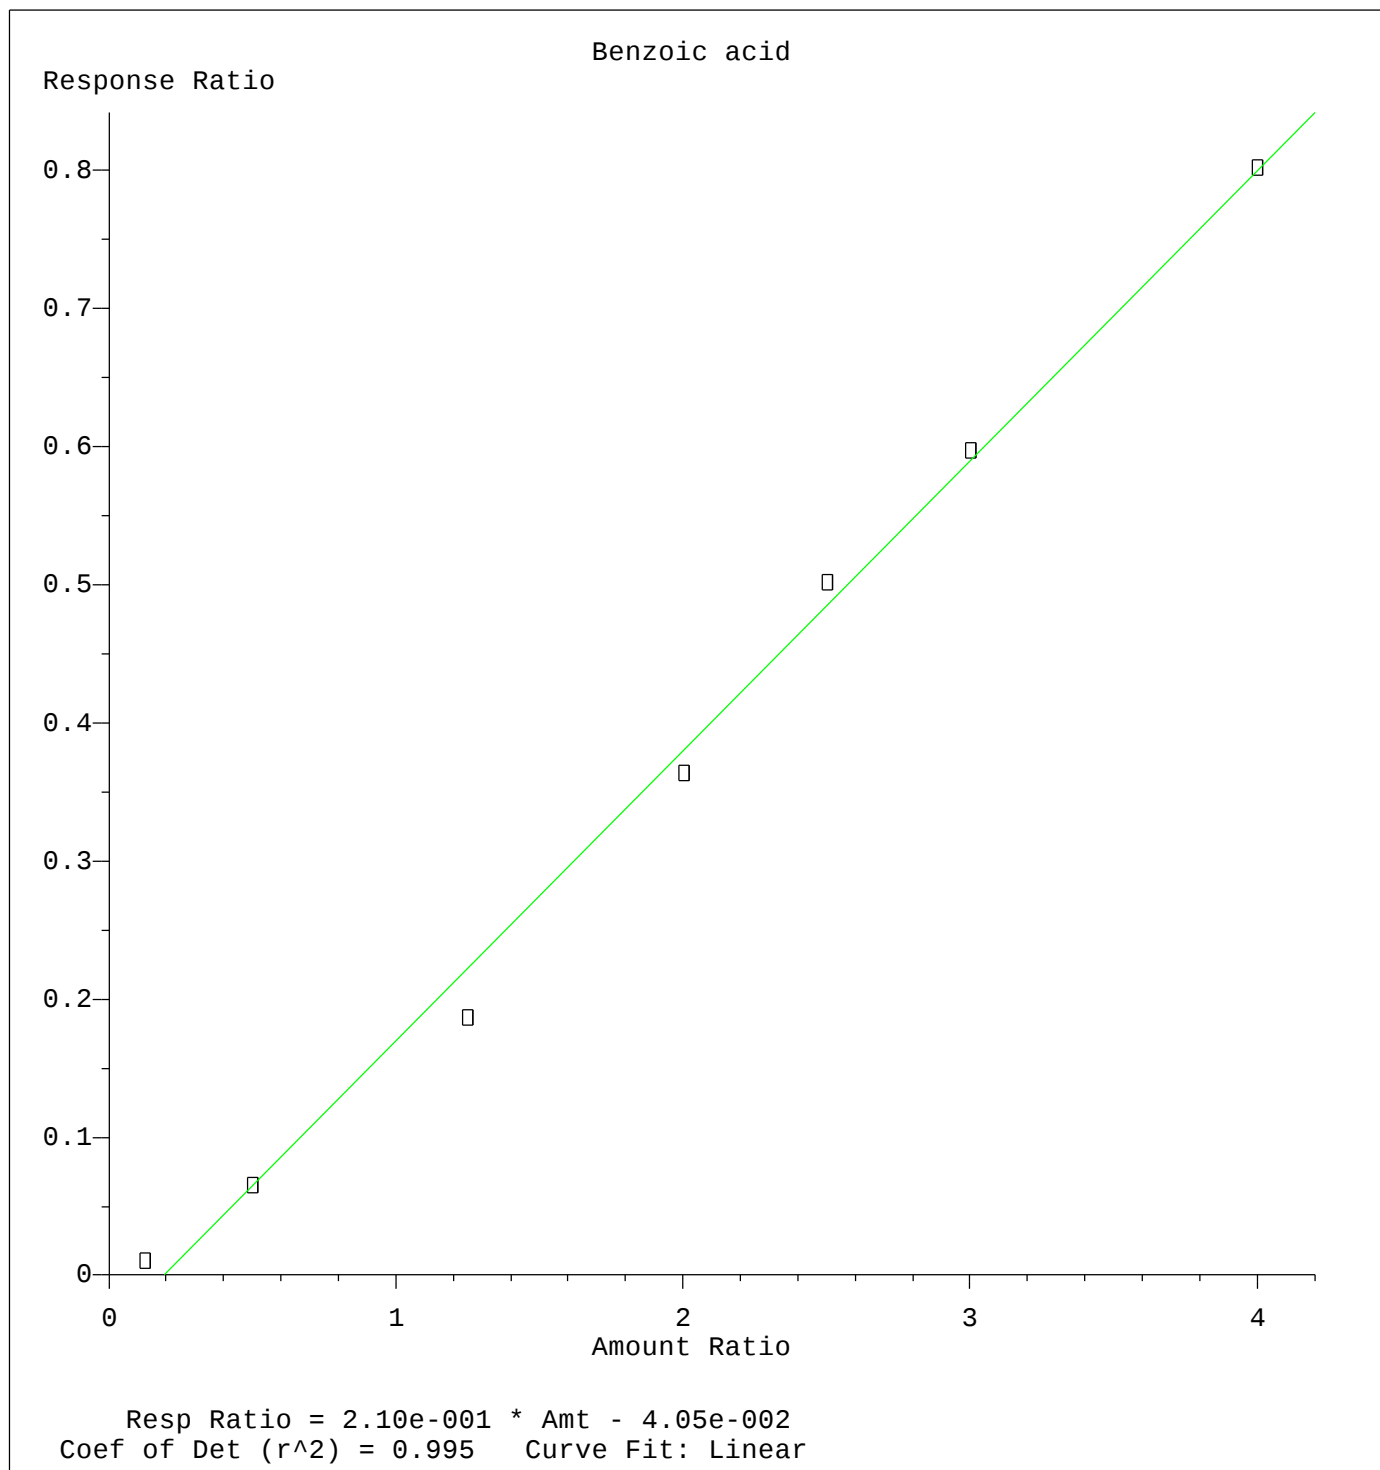


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
Calibration Table Last Updated: Sat Mar 18 05:21:29 2017

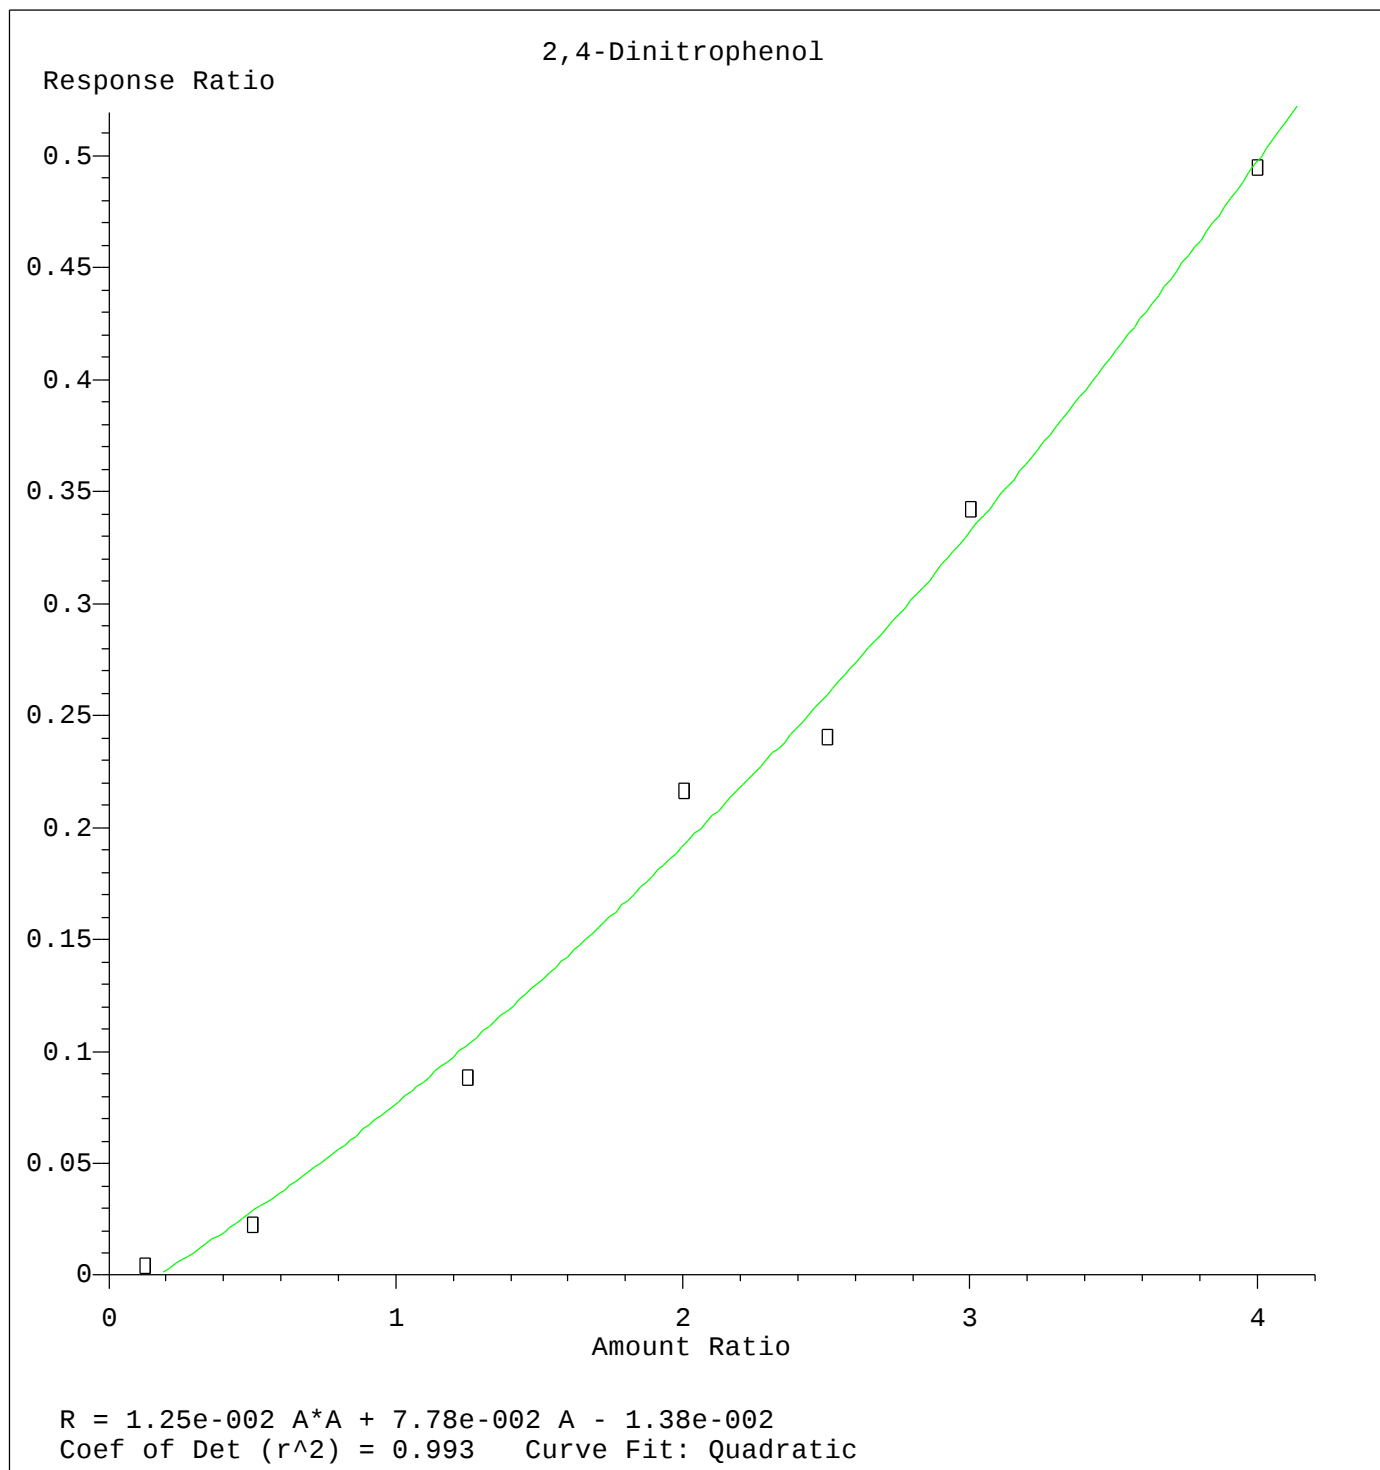

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
Calibration Table Last Updated: Sat Mar 18 05:21:29 2017

4,6-Dinitro-2-methylphenol

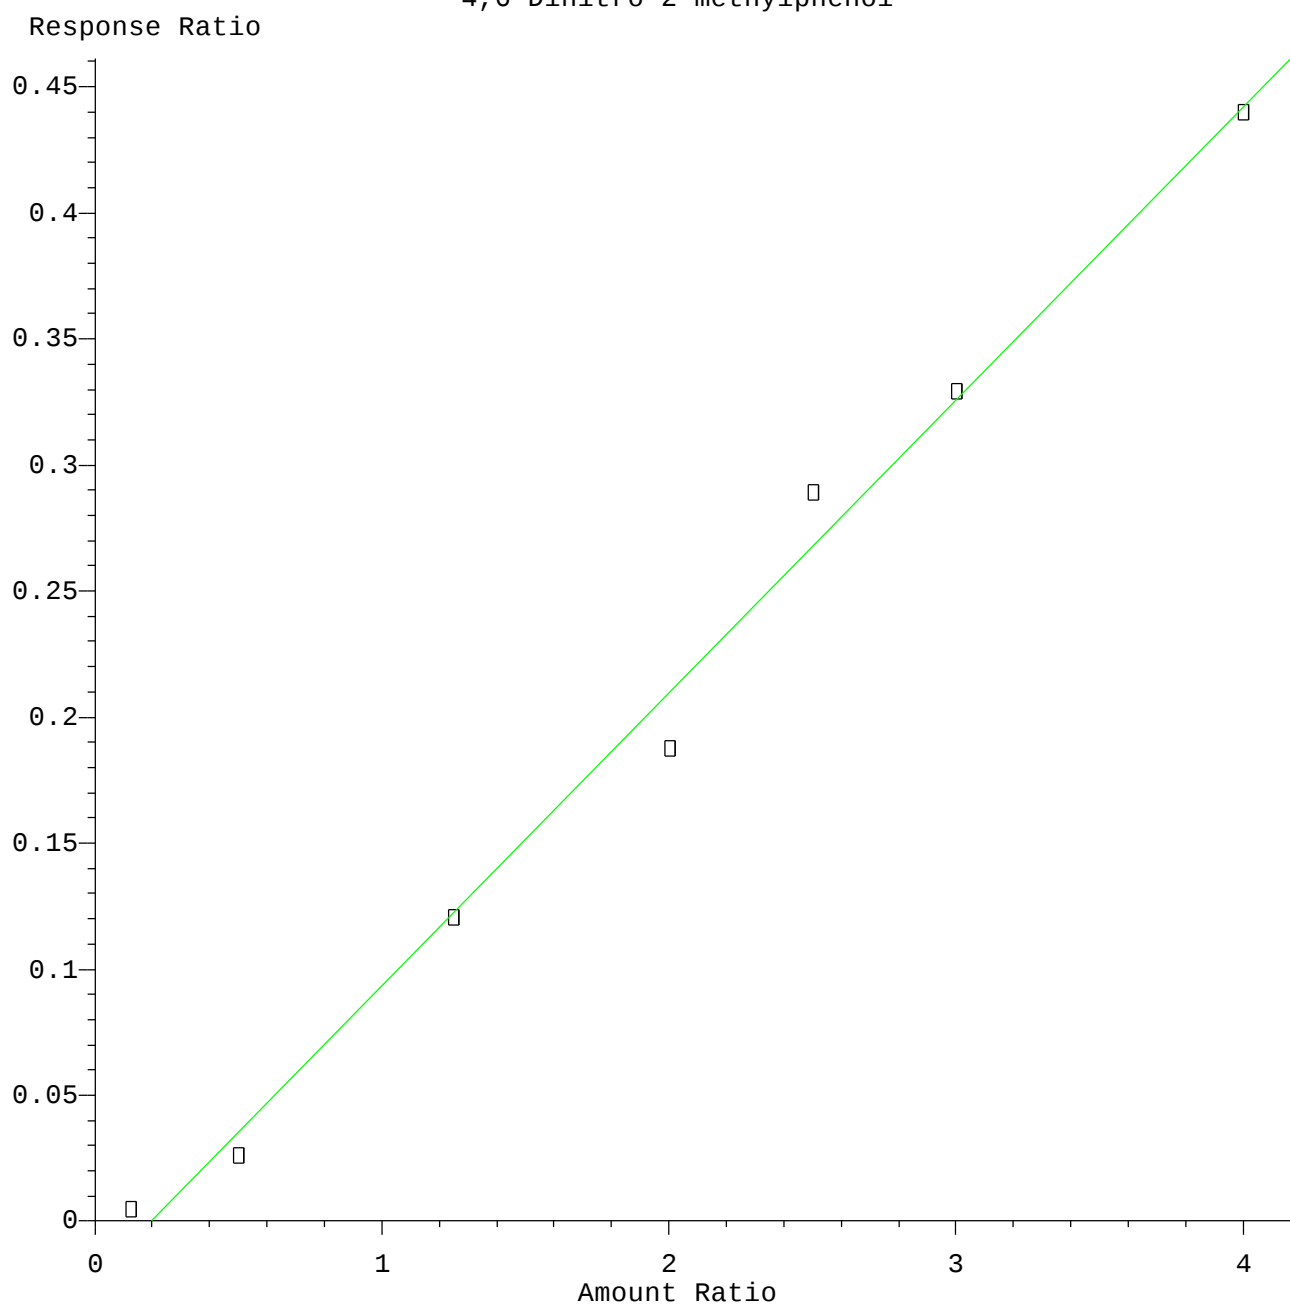

Resp Ratio = $1.16 \times 10^{-1} \times \text{Amt} - 2.28 \times 10^{-2}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
Calibration Table Last Updated: Sat Mar 18 05:21:29 2017