
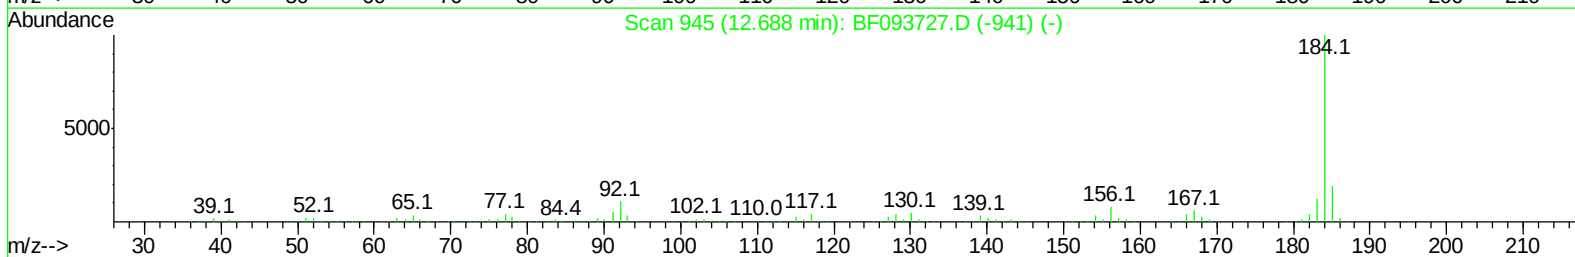
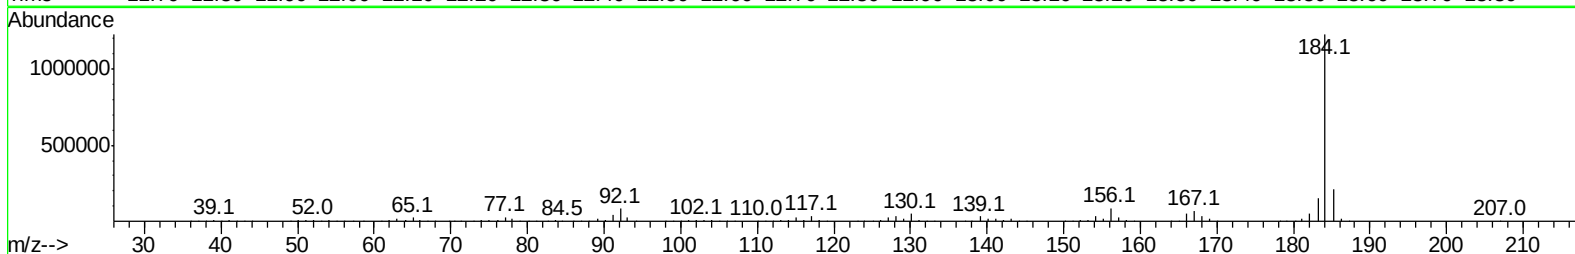


Data Path : Z:\HPCHEM1\BNA F\DATA\BF031817\
Data File : BF093723.D
Acq On : 18 Mar 2017 00:09
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 04:42:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 18 05:21:29 2017
Response via : Initial Calibration

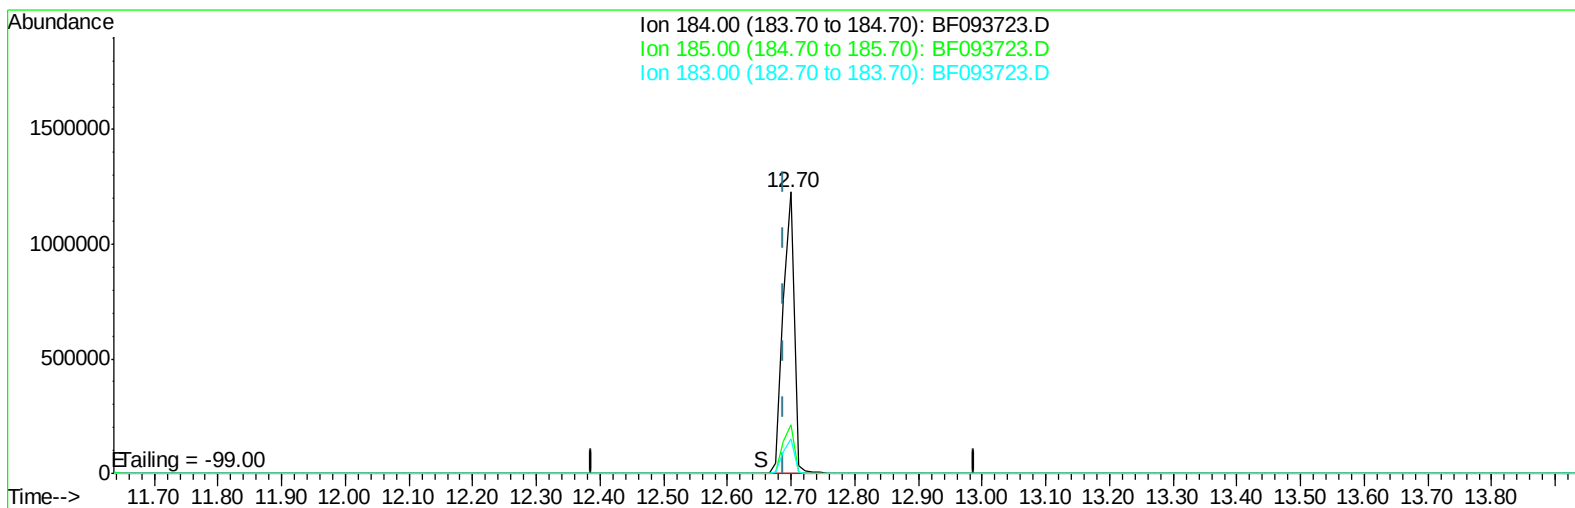

TIC: BF093723.D

(76) Benzidine




12.699min (+0.011) 0.00ng m

response 1428374

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	17.35
183.00	12.20	12.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031817\
Data File : BF093723.D
Acq On : 18 Mar 2017 00:09
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 04:42:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 18 05:21:29 2017
Response via : Initial Calibration

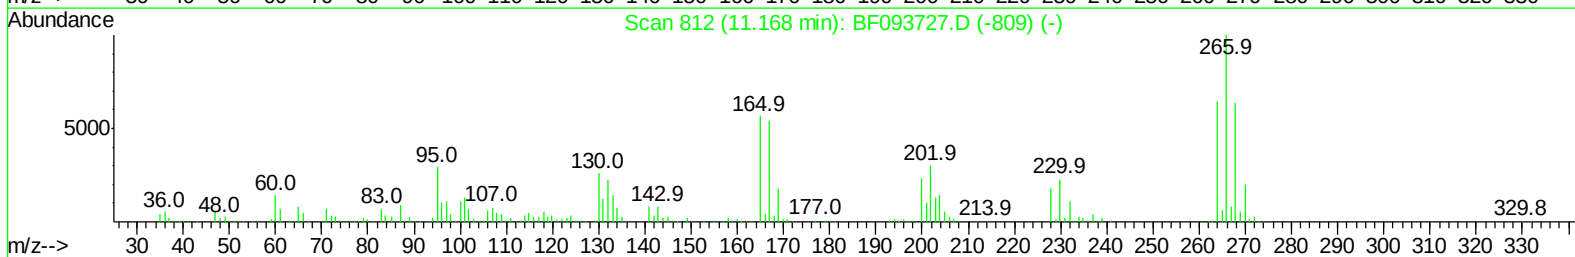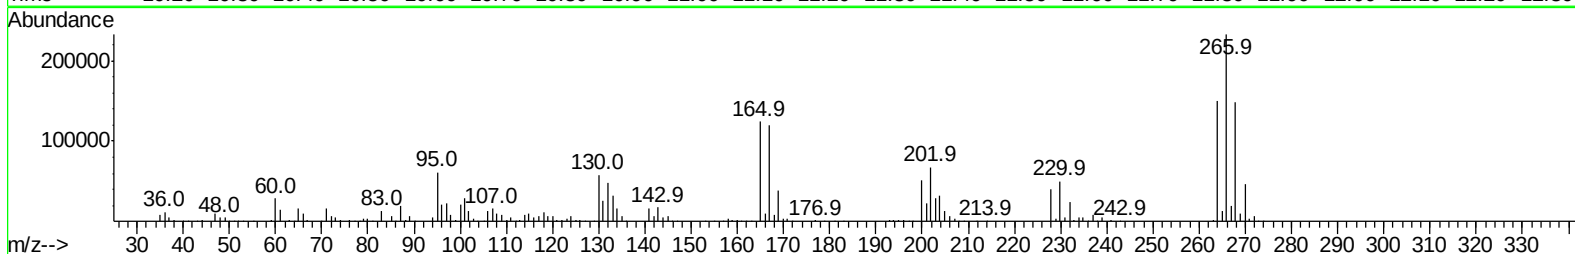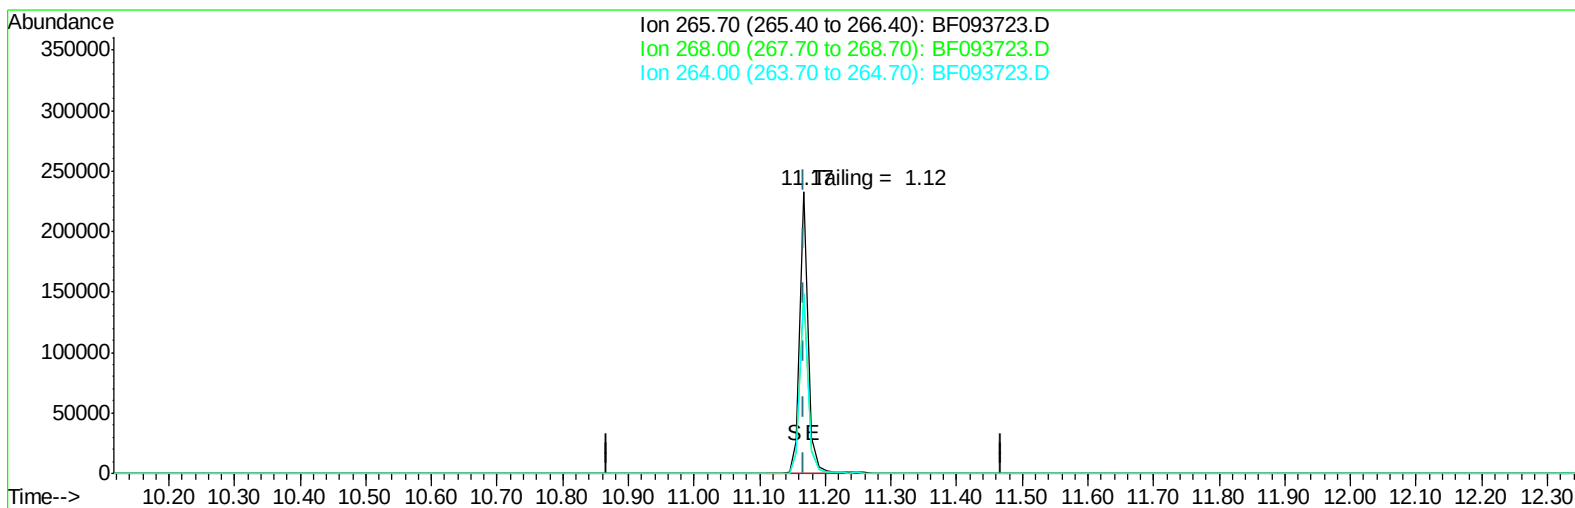

TIC: BF093723.D

(69) Pentachlorophenol (C)

11.168min (+0.000) 0.00ng

response 208668

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.63
264.00	64.60	64.16
0.00	0.00	0.00