
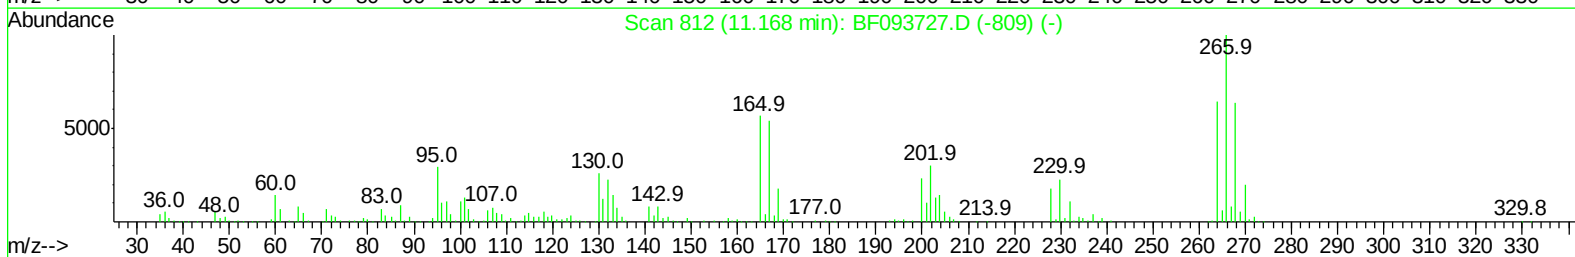
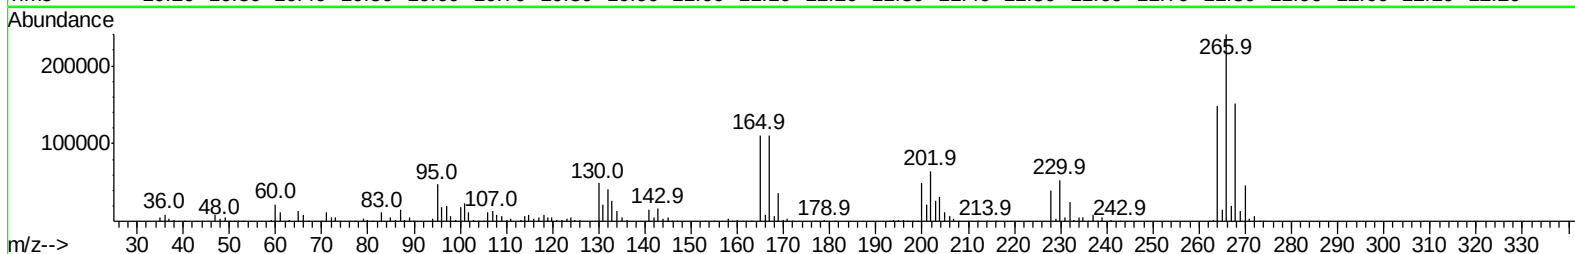


Data Path : Z:\HPCHEM1\BNA F\DATA\BF031817\
Data File : BF093732.D
Acq On : 18 Mar 2017 5:05
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 04:44:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 18 05:21:29 2017
Response via : Initial Calibration

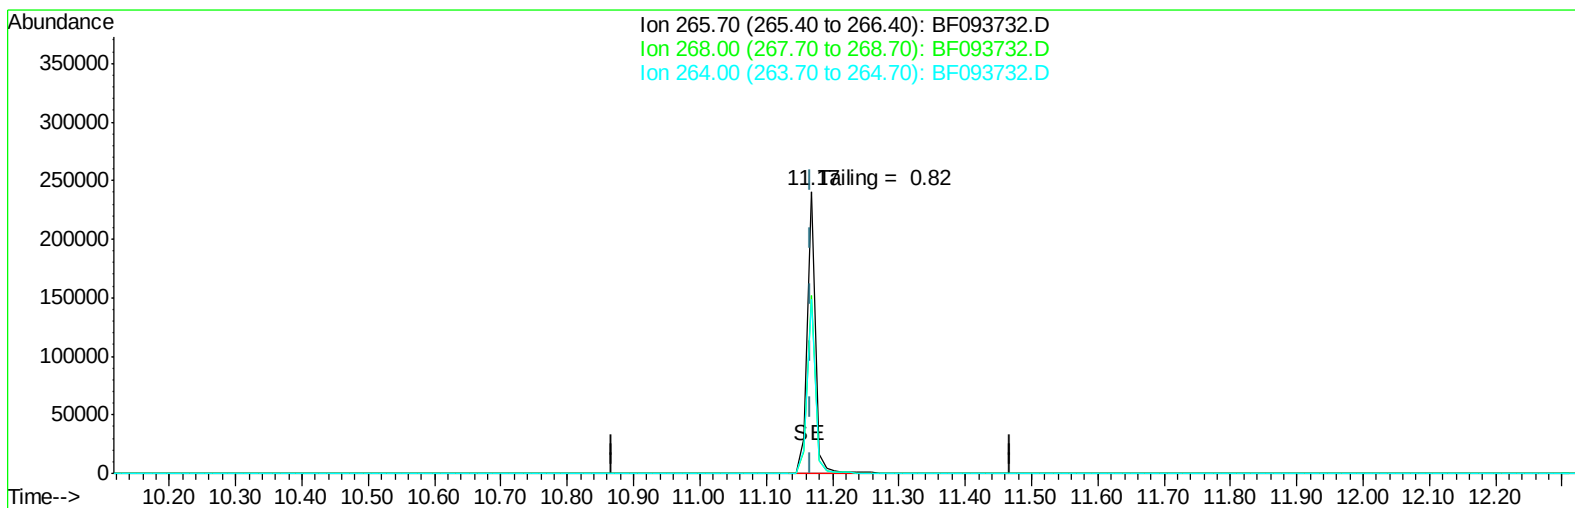

TIC: BF093732.D

(69) Pentachlorophenol (C)




11.168min (+0.000) 0.00ng

response 205479

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.24
264.00	64.60	61.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031817\
Data File : BF093732.D
Acq On : 18 Mar 2017 5:05
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 04:44:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 18 05:21:29 2017
Response via : Initial Calibration

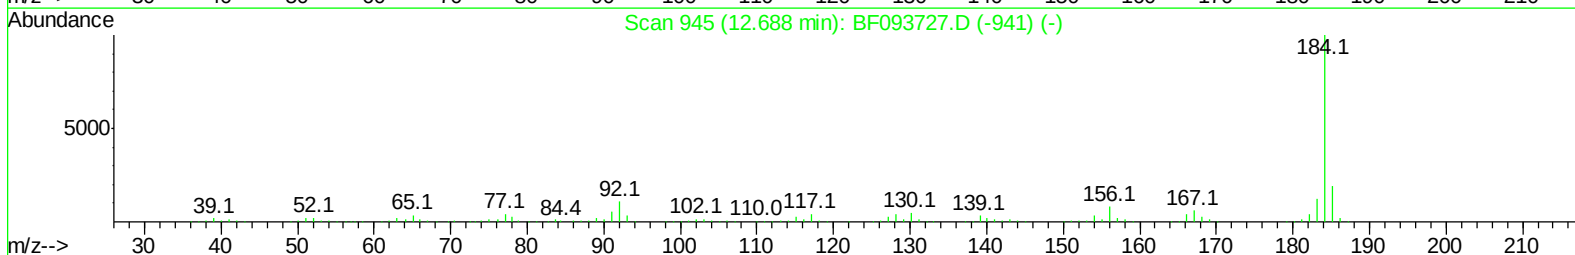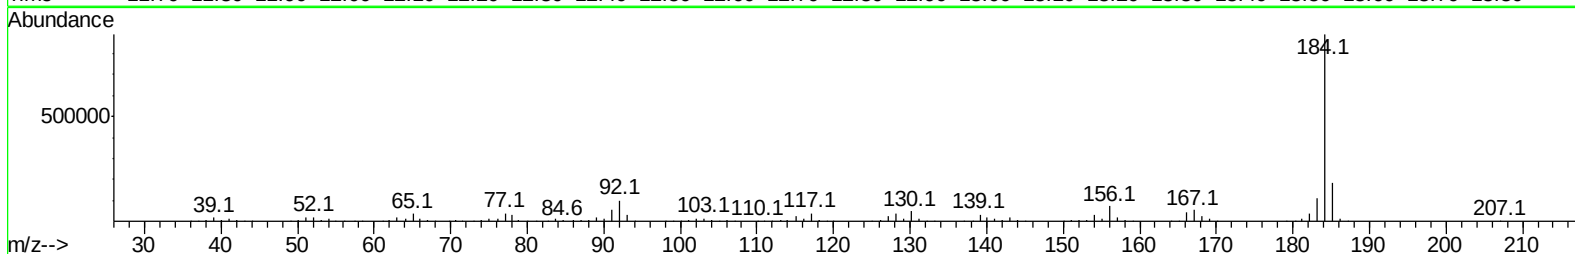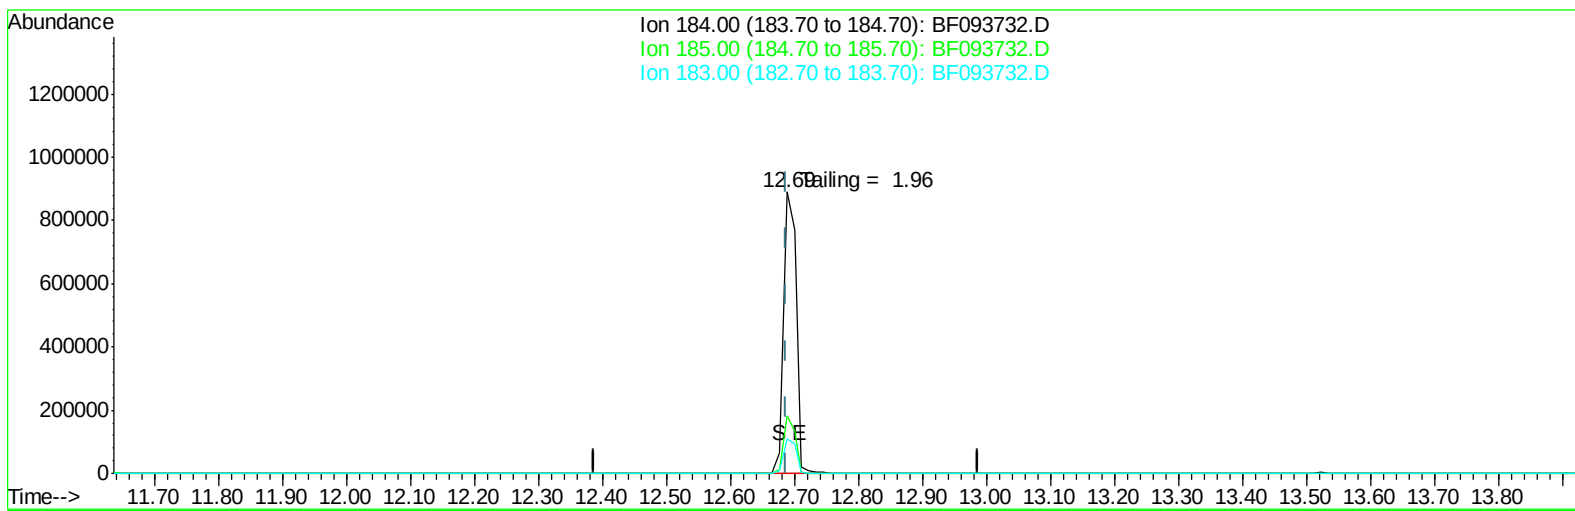

TIC: BF093732.D

(76) Benzidine

12.688min (+0.000) 0.00ng

response 1215961

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	20.26
183.00	12.20	12.21
0.00	0.00	0.00