

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031817\
 Data File : BF093745.D
 Acq On : 18 Mar 2017 11:16
 Operator : SJ/MA
 Sample : I2263-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-101D

Quant Time: Mar 20 01:32:12 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 18 05:21:29 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	203546	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	761110	20.00	ng	-0.01
38) Acenaphthene-d10	9.88	164	354906	20.00	ng	-0.01
63) Phenanthrene-d10	11.36	188	681581	20.00	ng	0.00
75) Chrysene-d12	13.99	240	592291	20.00	ng	-0.01
86) Perylene-d12	15.40	264	468905	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	743231	60.88	ng	0.00
7) Phenol-d6	6.47	99	644902	42.62	ng	-0.01
23) Nitrobenzene-d5	7.41	82	1119682	88.29	ng	0.00
41) 2,4,6-Tribromophenol	10.66	330	383883	165.27	ng	-0.01
44) 2-Fluorobiphenyl	9.21	172	2059054	109.48	ng	0.00
78) Terphenyl-d14	12.95	244	1631785	59.30	ng	0.00
Target Compounds						
2) 1,4-Dioxane	2.47	88	98236	15.58	ng	99
32) Benzoic acid	7.84	122	37777	8.59	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031817\
Data File : BF093745.D
Acq On : 18 Mar 2017 11:16
Operator : SJ/MA
Sample : I2263-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101D

Quant Time: Mar 20 01:32:12 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 18 05:21:29 2017
Response via : Initial Calibration

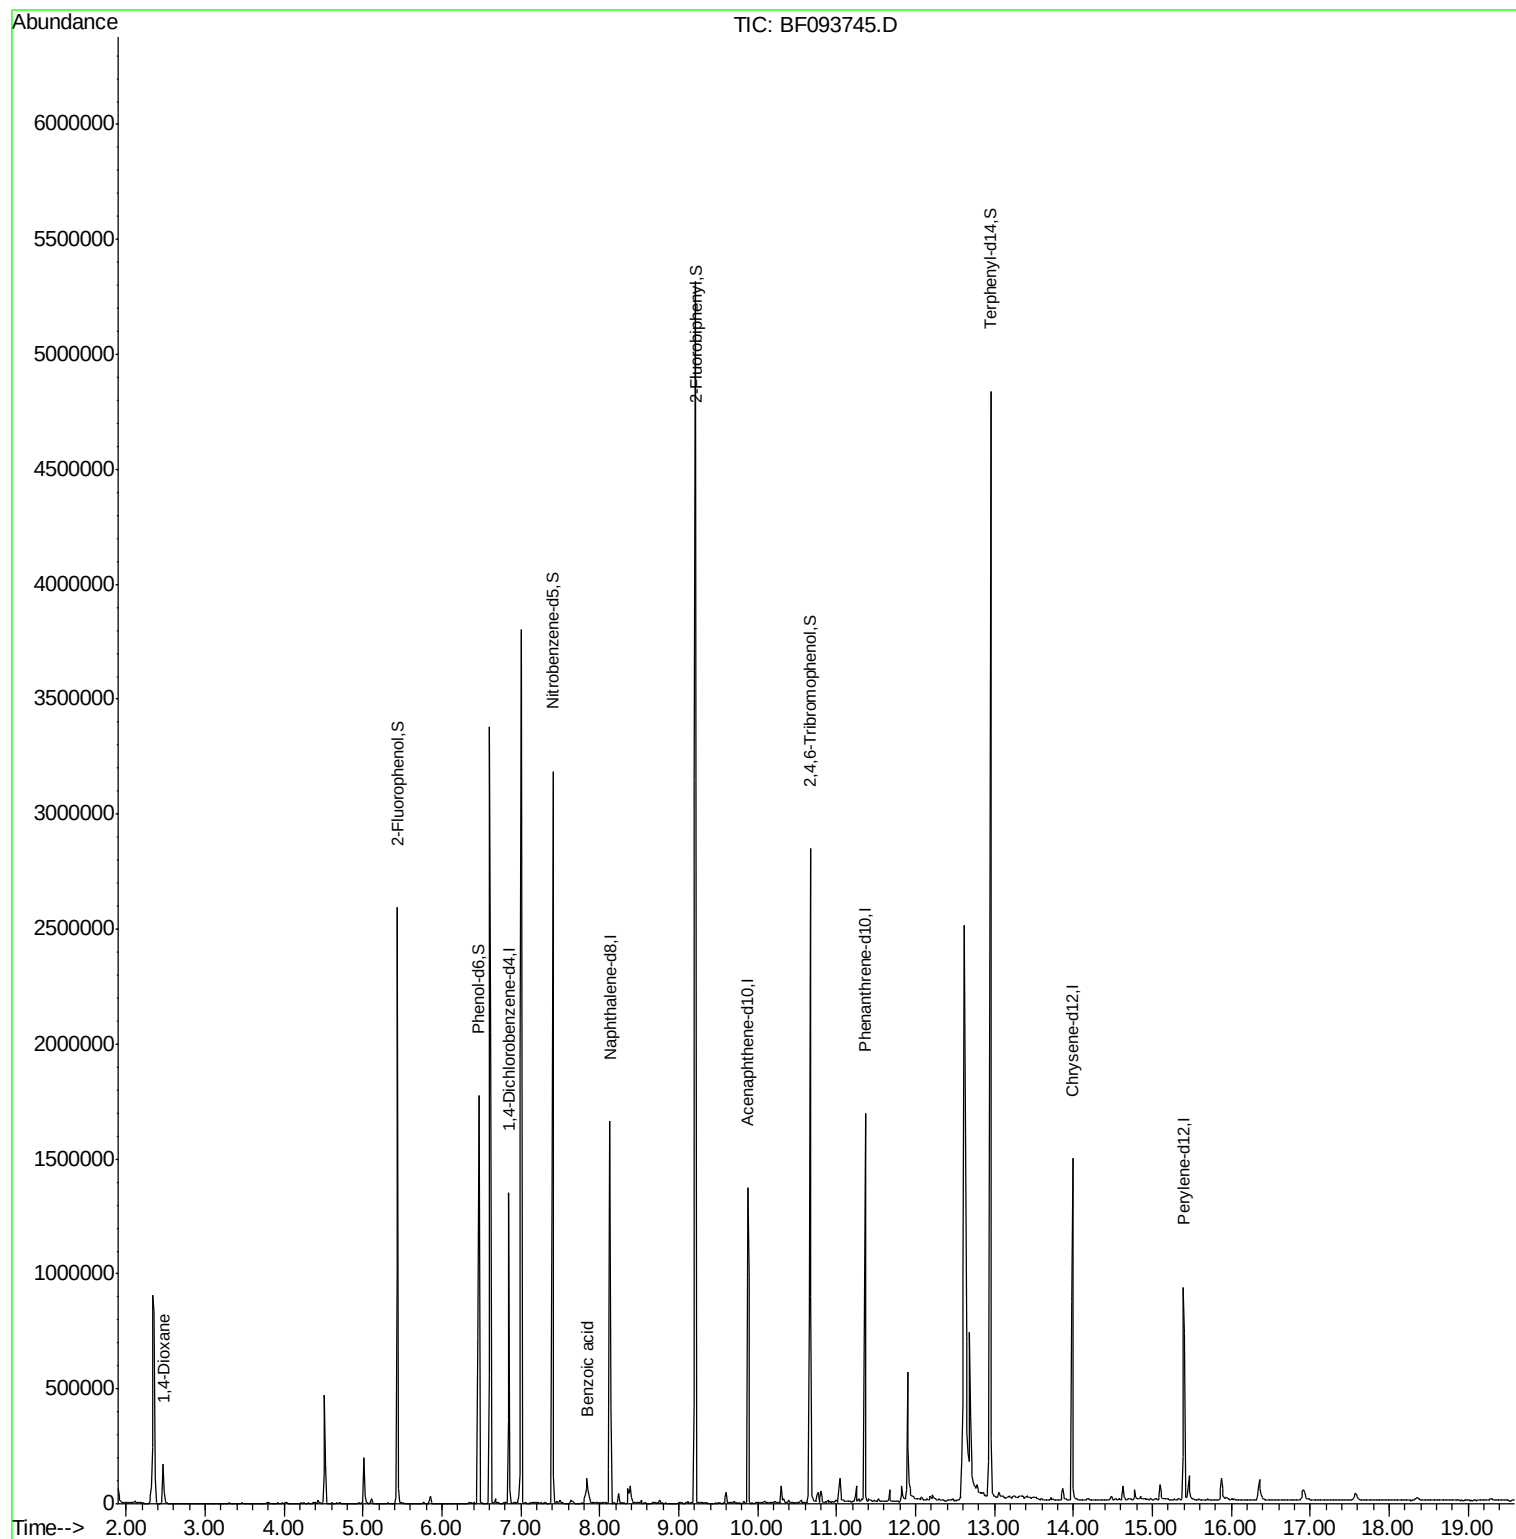

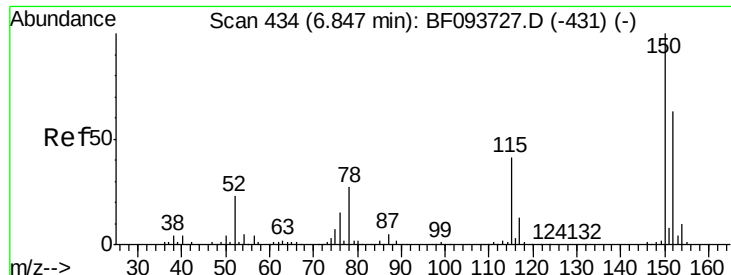

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.85 min Scan# 434

Delta R.T. -0.00 min

Lab File: BF093745.D

Acq: 18 Mar 2017 11:16

Instrument :

BNA_F

ClientSampleId :

MW-101D


Tgt Ion:152 Resp: 203546

Ion Ratio Lower Upper

152 100

150 156.5 126.2 189.2




115 58.6 52.2 78.2

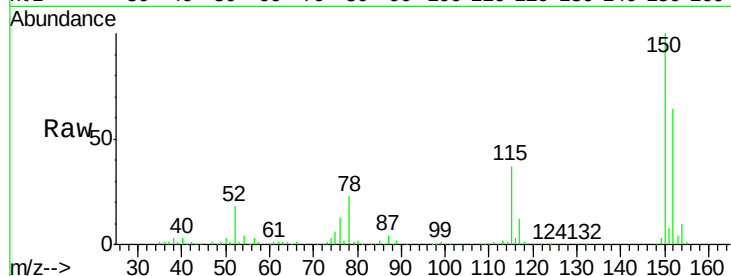

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

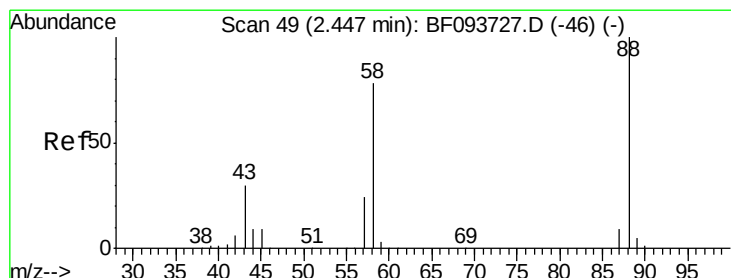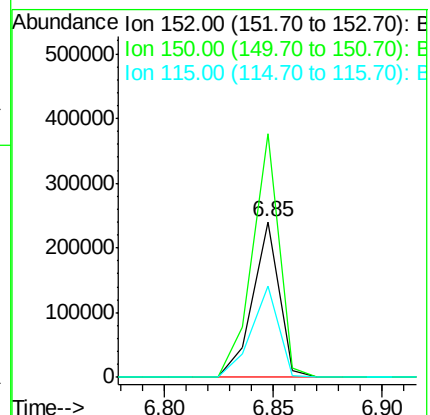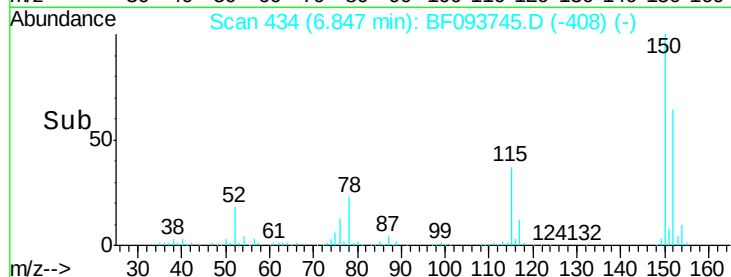

#2

1,4-Dioxane

Concen: 15.58 ng

RT: 2.47 min Scan# 51

Delta R.T. 0.02 min

Lab File: BF093745.D

Acq: 18 Mar 2017 11:16


Tgt Ion: 88 Resp: 98236

Ion Ratio Lower Upper

88 100

58 76.6 61.4 92.0



43 30.0 23.4 35.0

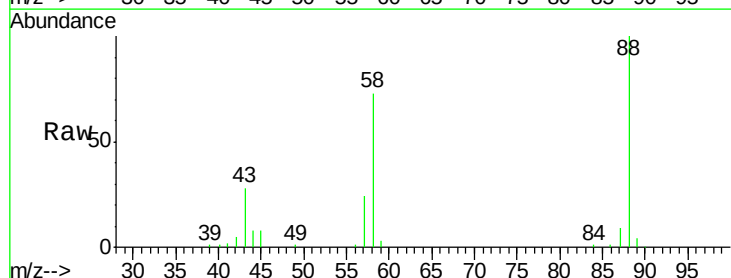


Abundance Ion 88.00 (87.70 to 88.70): BF0

Ion 58.00 (57.70 to 58.70): BF0

Ion 43.00 (42.70 to 43.70): BF0

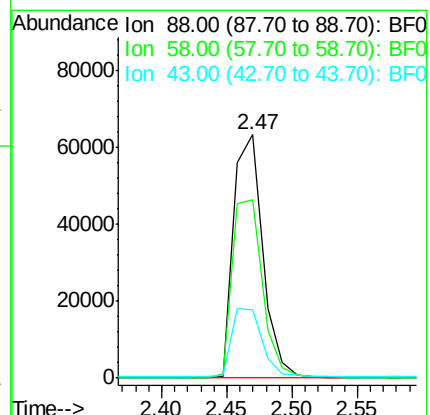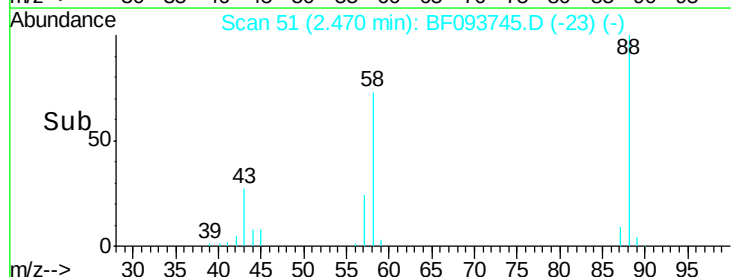

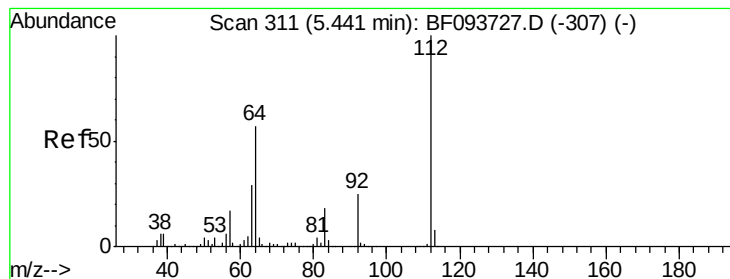

#5

2-Fluorophenol

Concen: 60.88 ng

RT: 5.44 min Scan# 311

Delta R.T. -0.00 min

Lab File: BF093745.D

Acq: 18 Mar 2017 11:16

Instrument :

BNA_F

ClientSampleId :

MW-101D


Tgt Ion: 112 Resp: 743231

Ion Ratio Lower Upper

112 100

64 56.4 46.0 69.0




63 28.1 23.4 35.0

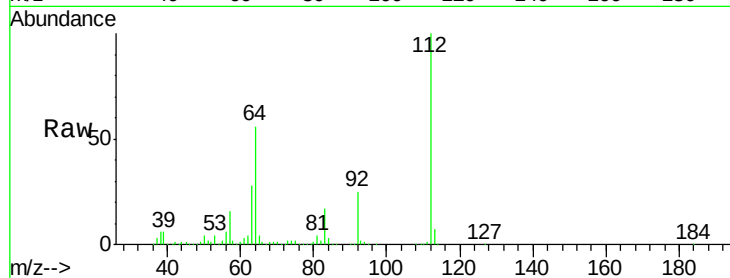

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

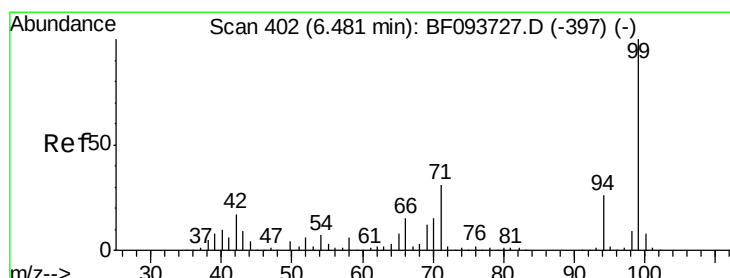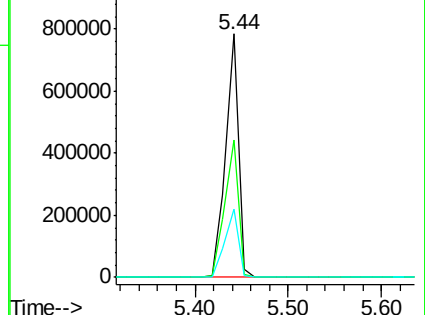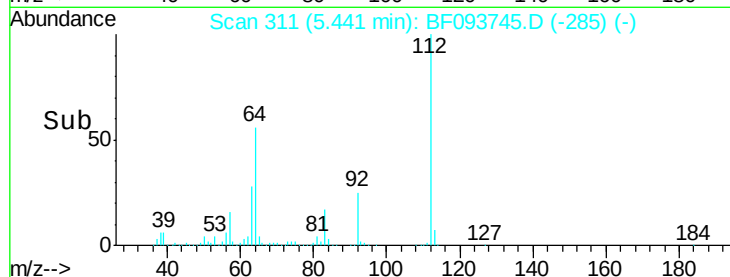

#7

Phenol-d6

Concen: 42.62 ng

RT: 6.47 min Scan# 401

Delta R.T. -0.01 min

Lab File: BF093745.D

Acq: 18 Mar 2017 11:16


Tgt Ion: 99 Resp: 644902

Ion Ratio Lower Upper

99 100

42 15.8 13.5 20.3



71 29.8 24.5 36.7

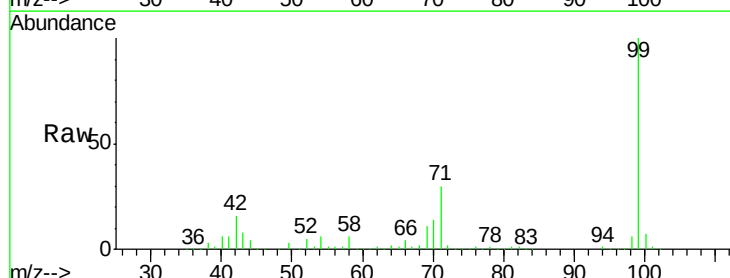


Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

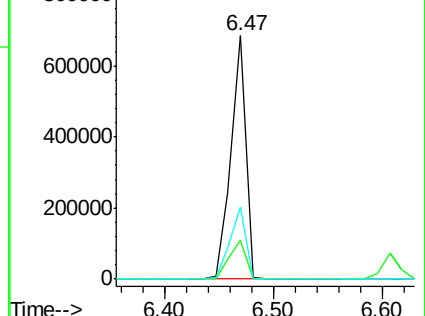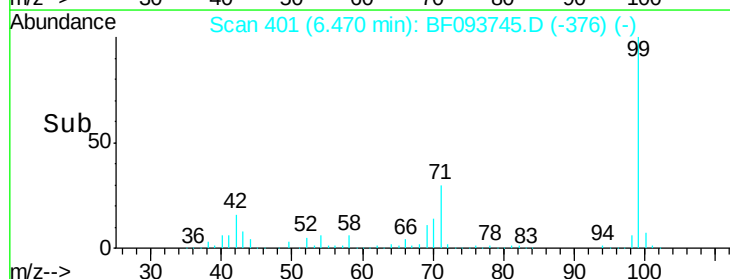

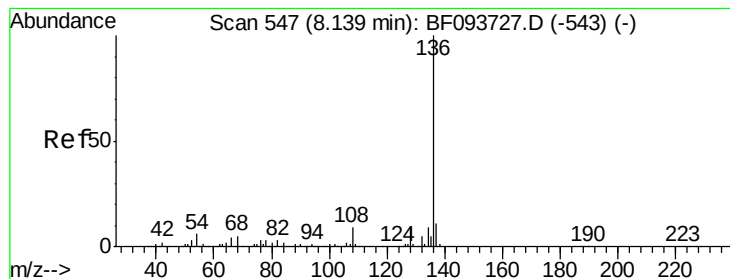

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.13 min Scan# 546

Delta R.T. -0.01 min

Lab File: BF093745.D

Acq: 18 Mar 2017 11:16

Instrument :

BNA_F

ClientSampleId :

MW-101D

Tgt Ion:136 Resp: 761110


Ion Ratio Lower Upper

136 100

137 11.2 8.5 12.7

54 9.2 4.9 7.3#

68 7.2 4.1 6.1#

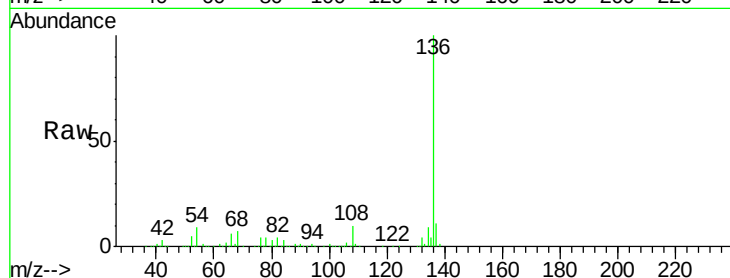


Abundance Ion 136.00 (135.70 to 136.70): E



Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

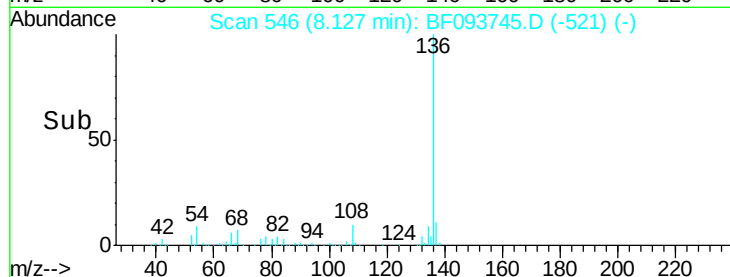

Time-->

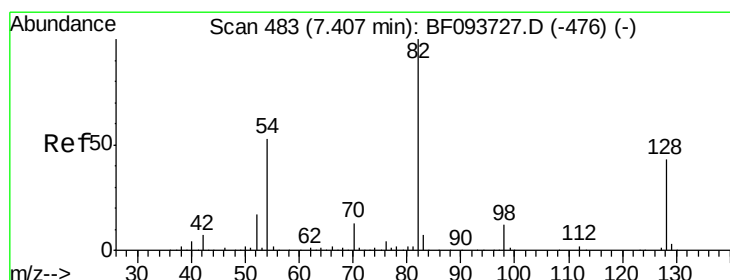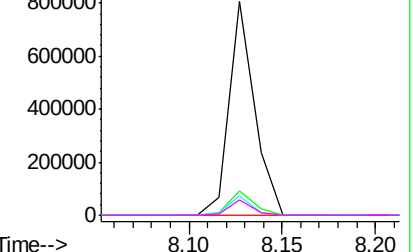

#23

Nitrobenzene-d5

Concen: 88.29 ng

RT: 7.41 min Scan# 483

Delta R.T. -0.00 min

Lab File: BF093745.D

Acq: 18 Mar 2017 11:16


Tgt Ion: 82 Resp: 1119682

Ion Ratio Lower Upper

82 100

128 45.0 34.0 51.0


54 51.4 42.2 63.2

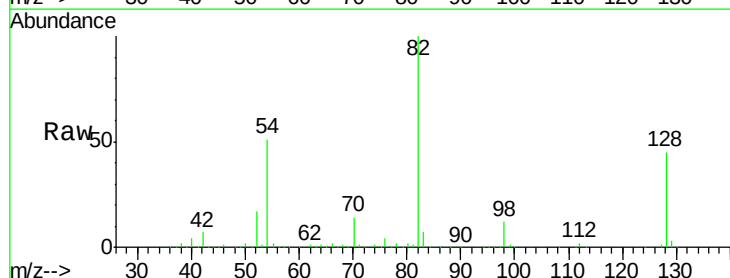


Abundance Ion 82.00 (81.70 to 82.70): BF0


Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

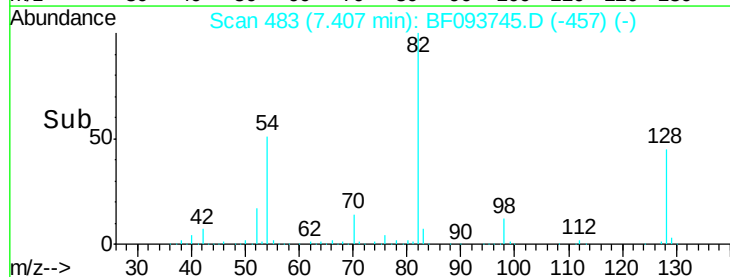

Time-->

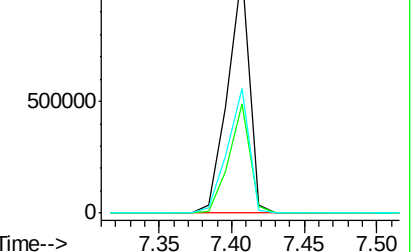

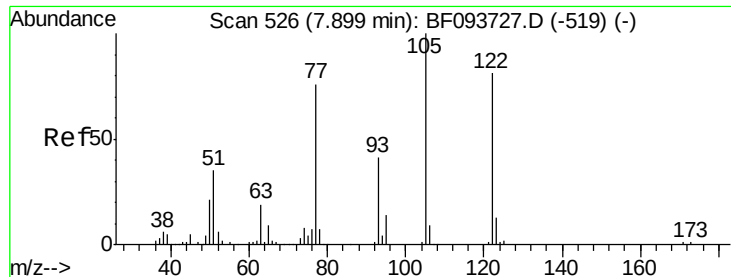

#32

Benzoic acid

Concen: 8.59 ng

RT: 7.84 min Scan# 521

Delta R.T. -0.06 min

Lab File: BF093745.D

Acq: 18 Mar 2017 11:16

Instrument :

BNA_F

ClientSampleId :

MW-101D


Tgt Ion:122 Resp: 37777

Ion Ratio Lower Upper

122 100

105 125.9 103.3 143.3




77 97.8 73.7 113.7

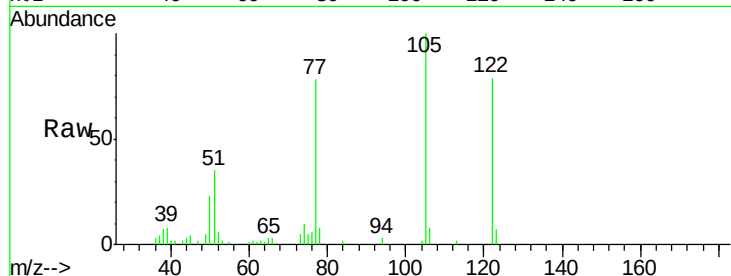

Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF0

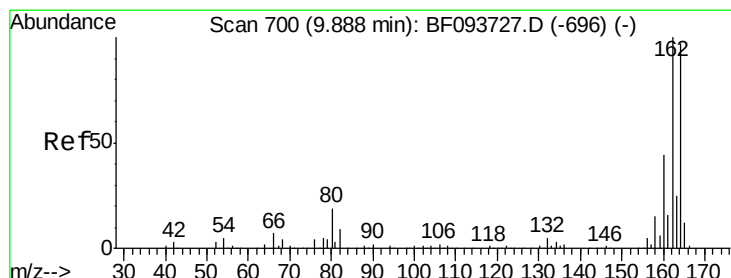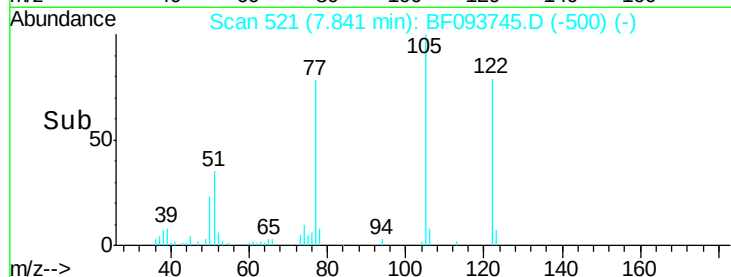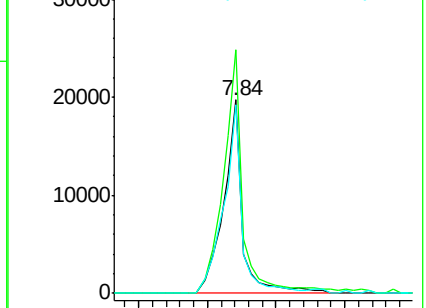

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.88 min Scan# 699

Delta R.T. -0.01 min

Lab File: BF093745.D

Acq: 18 Mar 2017 11:16


Tgt Ion:164 Resp: 354906

Ion Ratio Lower Upper

164 100

162 101.3 82.6 123.8



160 45.1 36.2 54.2

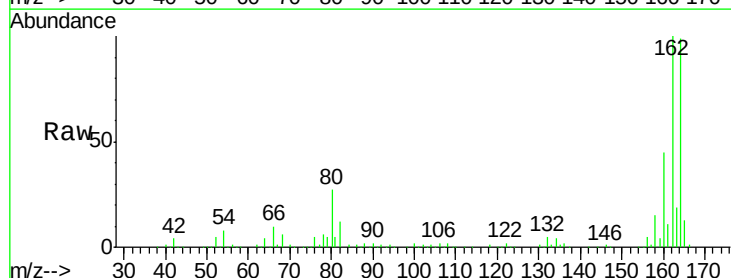


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

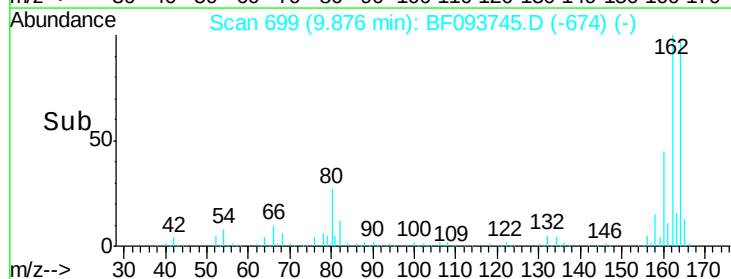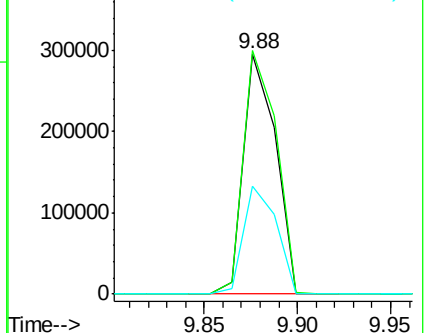


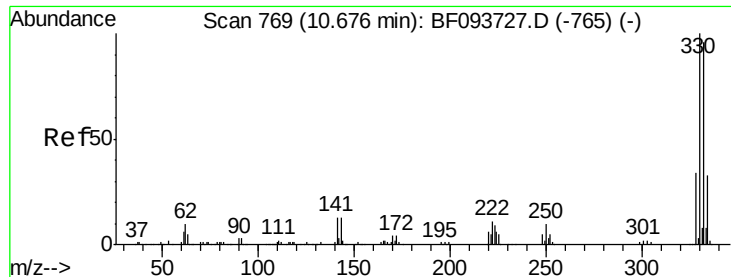




#41
 2,4,6-Tribromophenol
 Concen: 165.27 ng
 RT: 10.66 min Scan# 768
 Delta R.T. -0.01 min
 Lab File: BF093745.D
 Acq: 18 Mar 2017 11:16

Instrument :
 BNA_F
 ClientSampleId :
 MW-101D

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.6	76.6	115.0
141	37.5	31.4	47.2

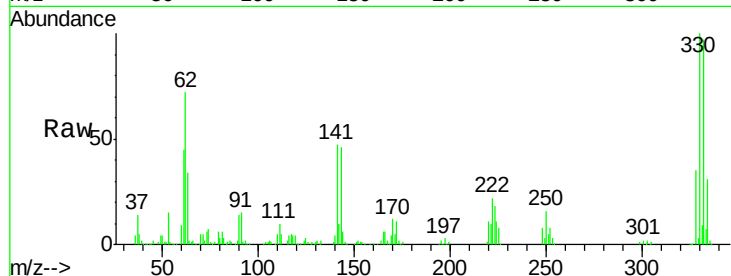


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

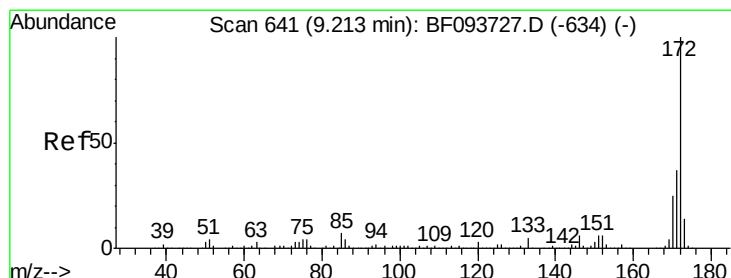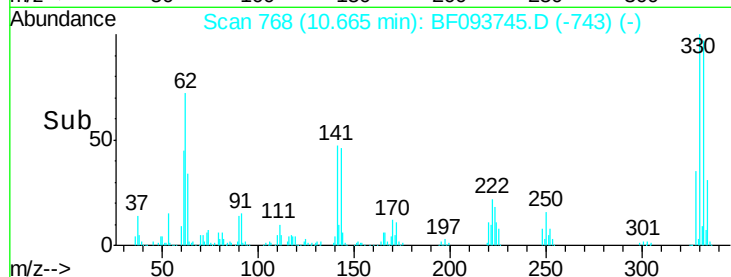
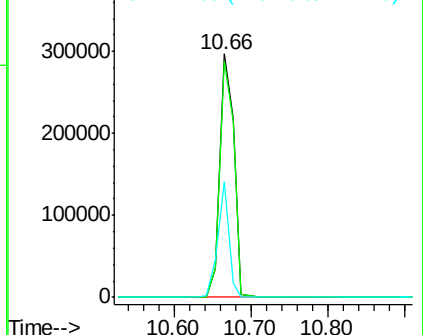



#44
 2-Fluorobiphenyl
 Concen: 109.48 ng
 RT: 9.21 min Scan# 641
 Delta R.T. 0.00 min
 Lab File: BF093745.D
 Acq: 18 Mar 2017 11:16

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.6	44.4
170	24.8	19.8	29.8

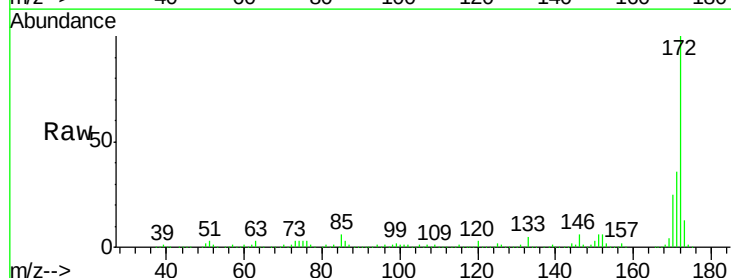

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



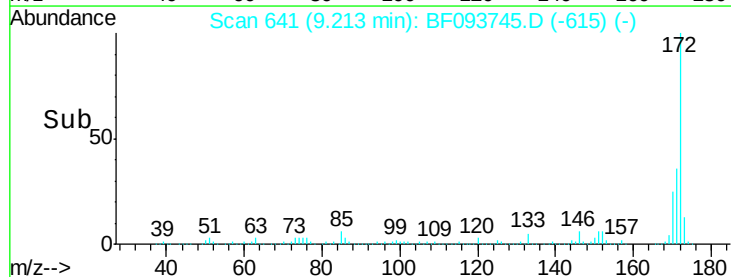
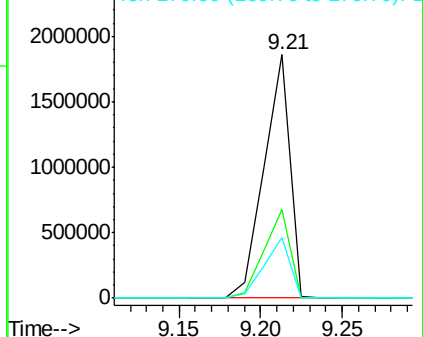


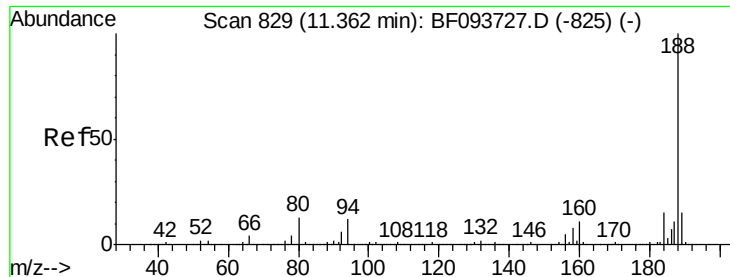

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.36 min Scan# 829
Delta R.T. -0.00 min
Lab File: BF093745.D
Acq: 18 Mar 2017 11:16




Instrument :
BNA_F
ClientSampleId :
MW-101D


Tgt Ion:188 Resp: 681581
Ion Ratio Lower Upper
188 100
94 7.9 9.4 14.2#
80 8.2 10.2 15.2#

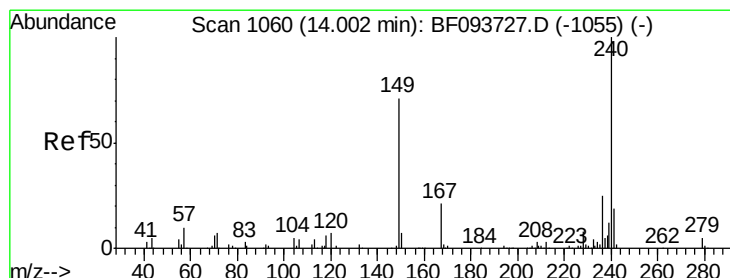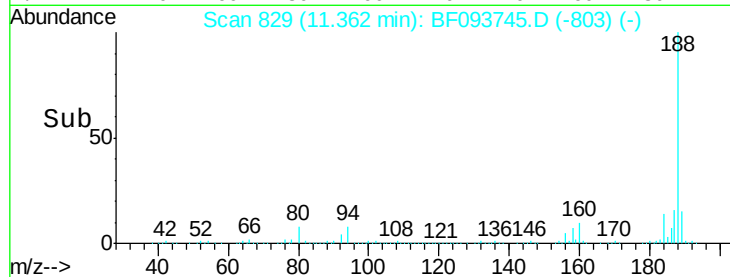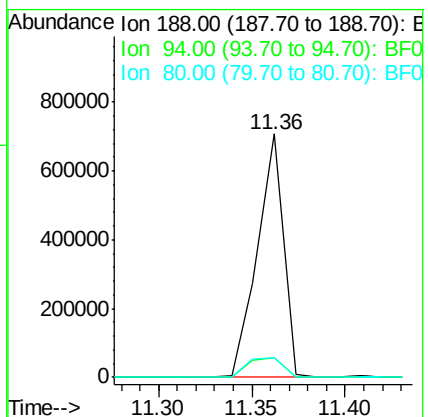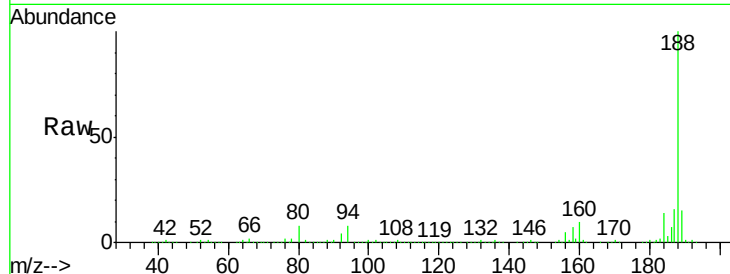

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.99 min Scan# 1059
Delta R.T. -0.01 min
Lab File: BF093745.D
Acq: 18 Mar 2017 11:16

Tgt Ion:240 Resp: 592291
Ion Ratio Lower Upper
240 100
120 10.7 5.8 8.8#
236 25.8 20.5 30.7

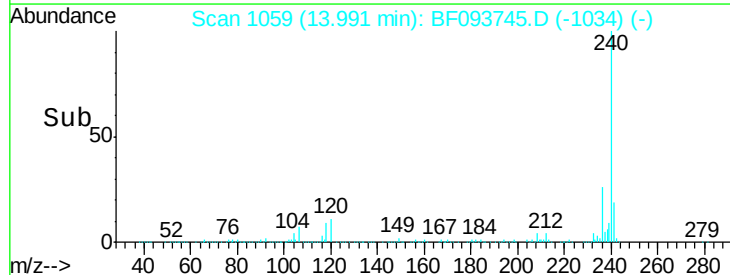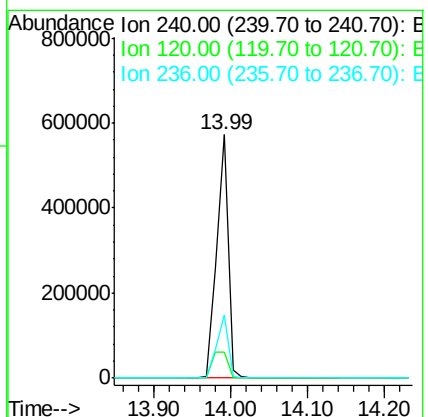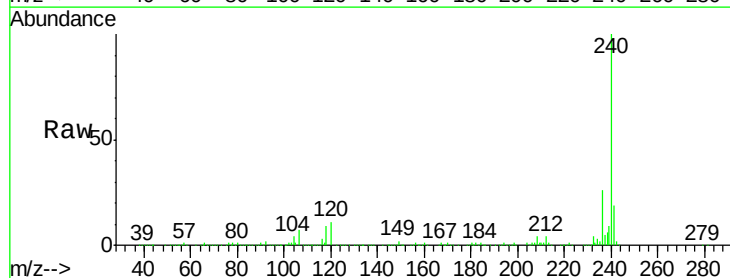

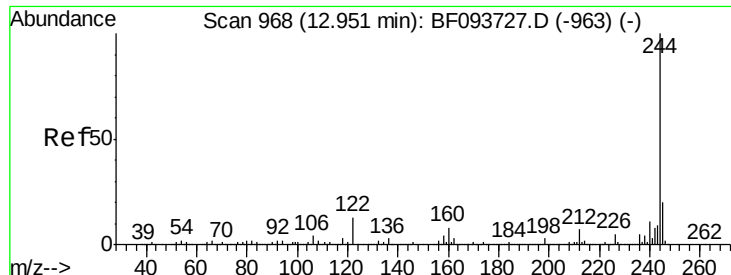

#78

Terphenyl-d14

Concen: 59.30 ng

RT: 12.95 min Scan# 968

Delta R.T. -0.00 min

Lab File: BF093745.D

Acq: 18 Mar 2017 11:16

Instrument :

BNA_F

ClientSampleId :

MW-101D





Tgt Ion:244 Resp: 1631785

Ion Ratio Lower Upper

244 100

212 7.6 6.0 9.0

122 13.2 10.3 15.5

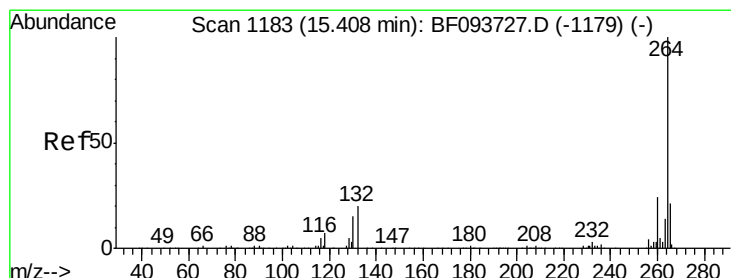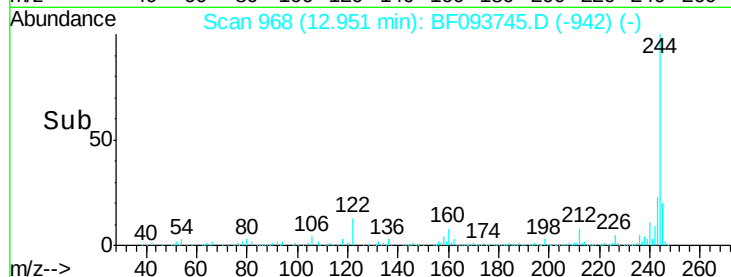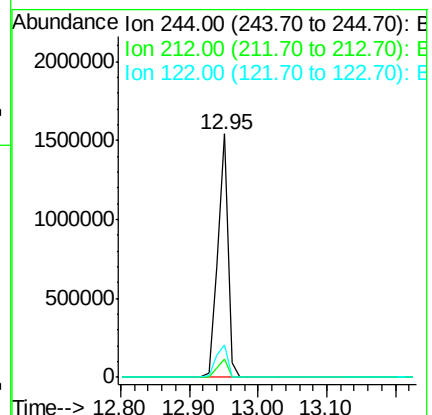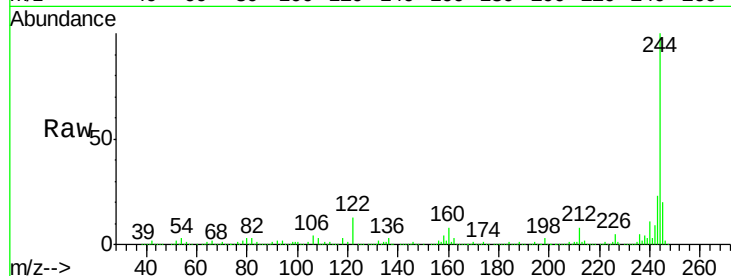

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.40 min Scan# 1182

Delta R.T. -0.01 min

Lab File: BF093745.D

Acq: 18 Mar 2017 11:16

Tgt Ion:264 Resp: 468905

Ion Ratio Lower Upper

264 100

260 23.9 19.5 29.3

265 21.1 17.2 25.8

