

Data Path : Z:\HPCHEM1\BNA_F\Data\BF031817\
 Data File : BF093744.D
 Acq On : 18 Mar 2017 10:49
 Operator : SJ/MA
 Sample : I2263-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-101I

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.355	36	41	44	rVB	136015	189773	3.21%	0.482%
2	2.470	50	51	57	rBV	47504	70759	1.20%	0.180%
3	4.516	227	230	233	rVB	433462	550918	9.33%	1.400%
4	5.018	272	274	277	rBV	254562	335329	5.68%	0.852%
5	5.441	308	311	313	rBV	2637993	2456140	41.61%	6.243%
6	6.470	398	401	403	rBV	1739615	1727358	29.26%	4.390%
7	6.607	410	413	416	rBV	3386159	4075279	69.03%	10.358%
8	6.847	431	434	436	rBV	1248919	1163527	19.71%	2.957%
9	7.007	445	448	450	rVB	3547013	3854052	65.29%	9.796%
10	7.407	480	483	485	rBV	3252788	3358558	56.89%	8.537%
11	8.127	544	546	548	rBV	1618152	1449593	24.56%	3.684%
12	9.213	637	641	643	rBV	4970718	5903387	100.00%	15.005%
13	9.876	697	699	702	rBV	1276553	1598104	27.07%	4.062%
14	10.665	765	768	771	rBV	2771366	3055895	51.77%	7.767%
15	11.362	826	829	831	rBV	1604553	1636996	27.73%	4.161%
16	12.951	965	968	970	rBV	4682458	5186892	87.86%	13.184%
17	13.991	1056	1059	1061	rBV	1241443	1505086	25.50%	3.826%
18	15.397	1179	1182	1185	rBV	877632	1225726	20.76%	3.115%


Sum of corrected areas: 39343372

Data Path : Z:\HPCHEM1\BNA_F\Data\BF031817\
Data File : BF093744.D
Acq On : 18 Mar 2017 10:49
Operator : SJ/MA
Sample : I2263-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

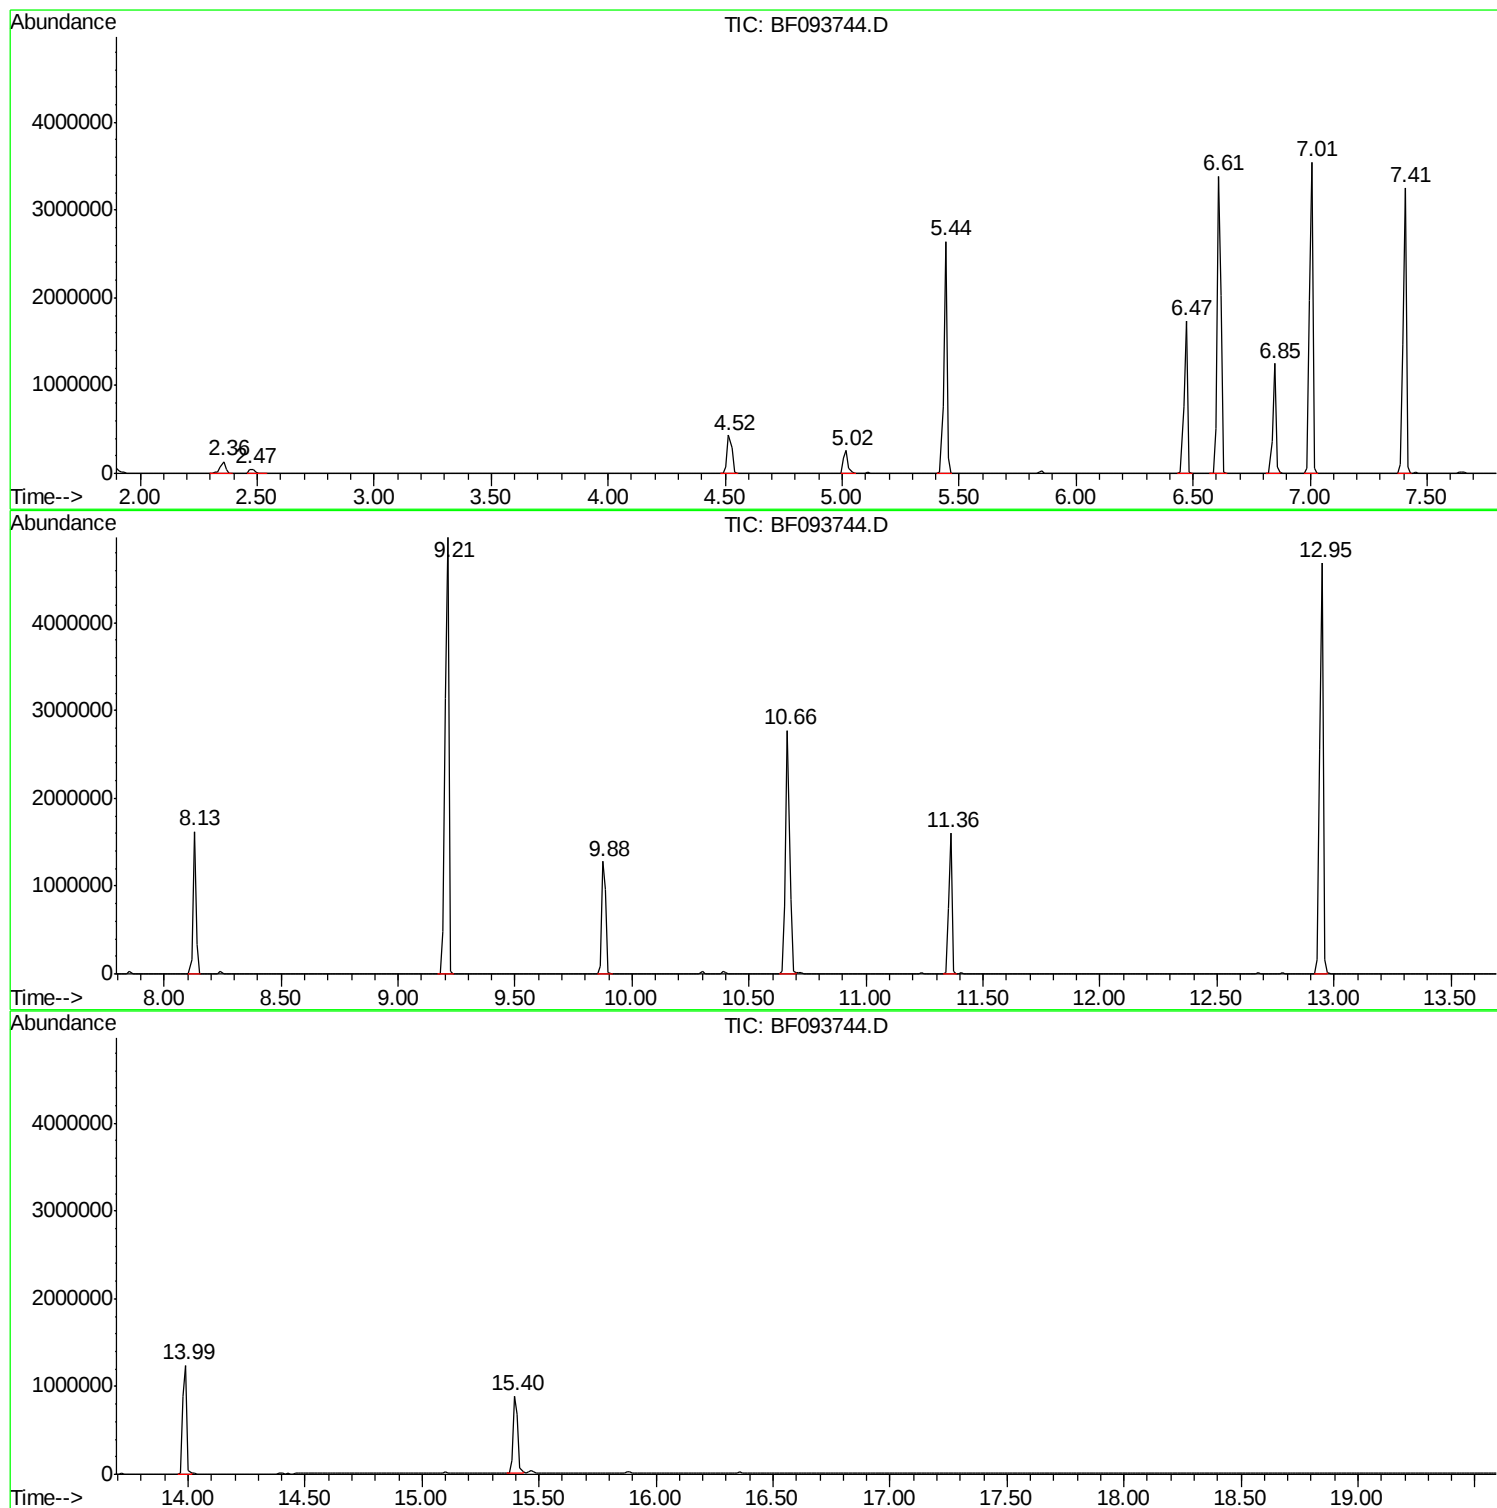

Data Path : Z:\HPCHEM1\BNA_F\Data\BF031817\
Data File : BF093744.D
Acq On : 18 Mar 2017 10:49
Operator : SJ/MA
Sample : I2263-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I









Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.02	5.76 ng	335329	1,4-Dichlorobenzene-d4	6.85

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16
3		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4		Butane	58	C4H10	000106-97-8	9
5		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

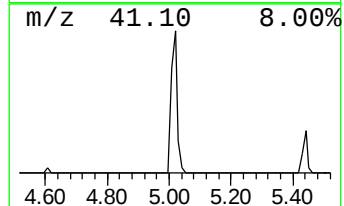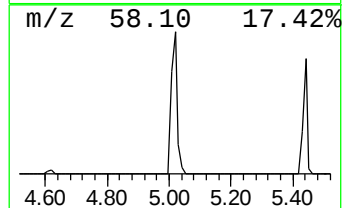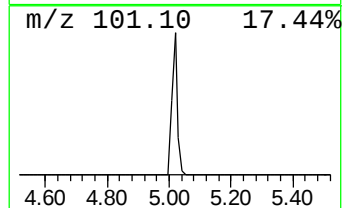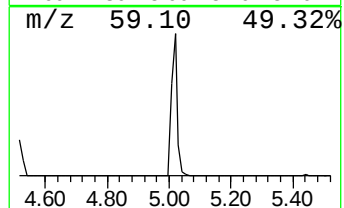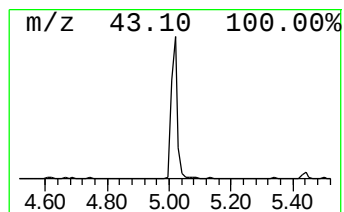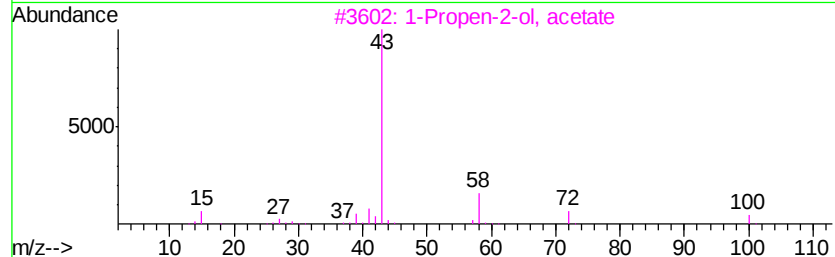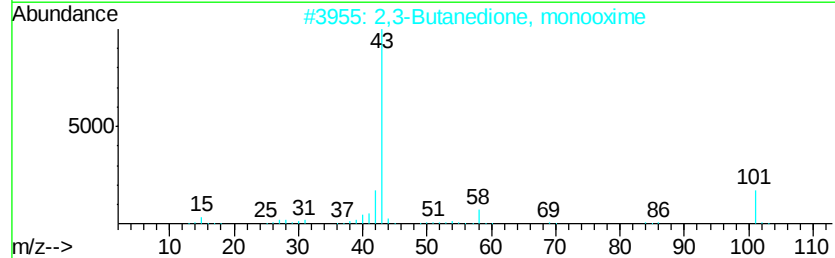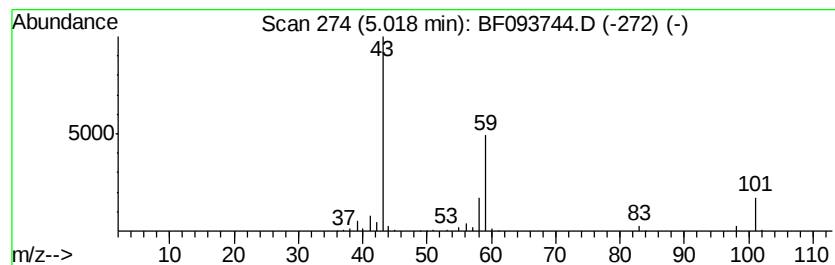

Data Path : Z:\HPCHEM1\BNA_F\Data\BF031817\
Data File : BF093744.D
Acq On : 18 Mar 2017 10:49
Operator : SJ/MA
Sample : I2263-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.61 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.61	70.05 ng	4075280	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9

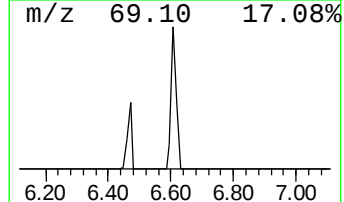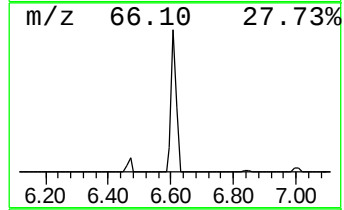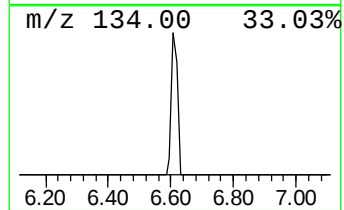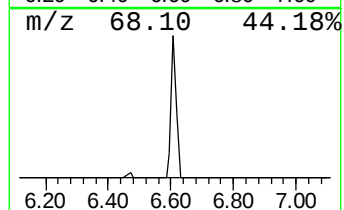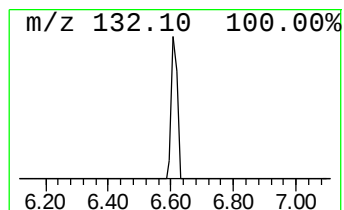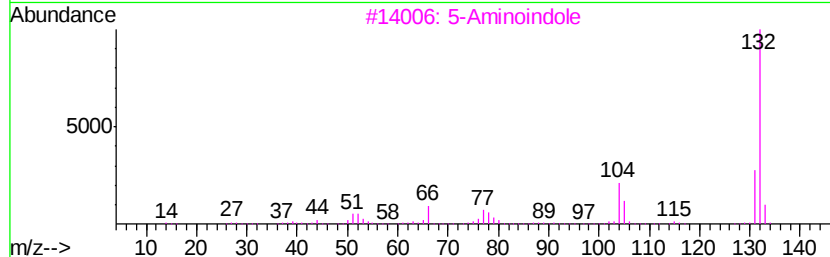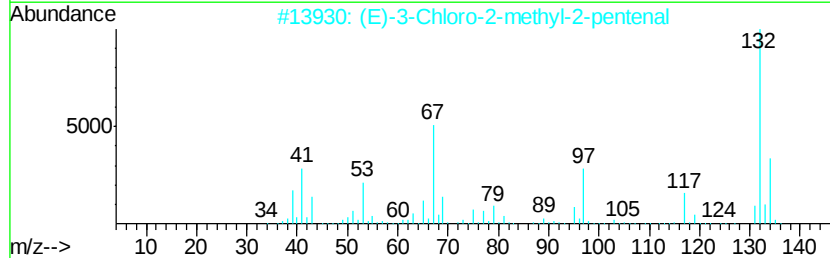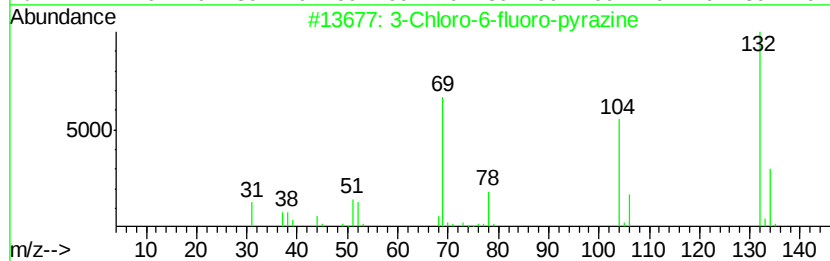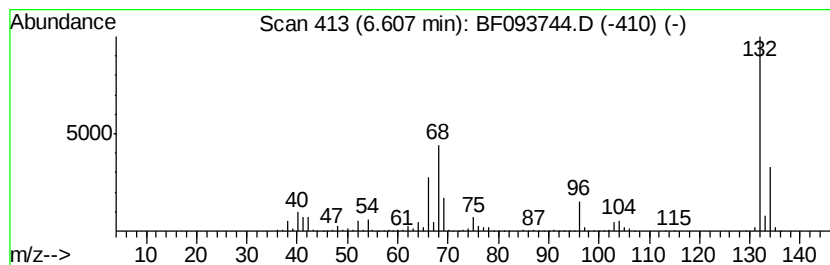

Data Path : Z:\HPCHEM1\BNA_F\Data\BF031817\
Data File : BF093744.D
Acq On : 18 Mar 2017 10:49
Operator : SJ/MA
Sample : I2263-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.02	5.8	ng	335329	1	6.85	1163530	20.0
unknown6.61	6.61	70.0	ng	4075280	1	6.85	1163530	20.0