


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031817\
 Data File : BF093723.D
 Acq On : 18 Mar 2017 00:09
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 18 05:21:29 2017

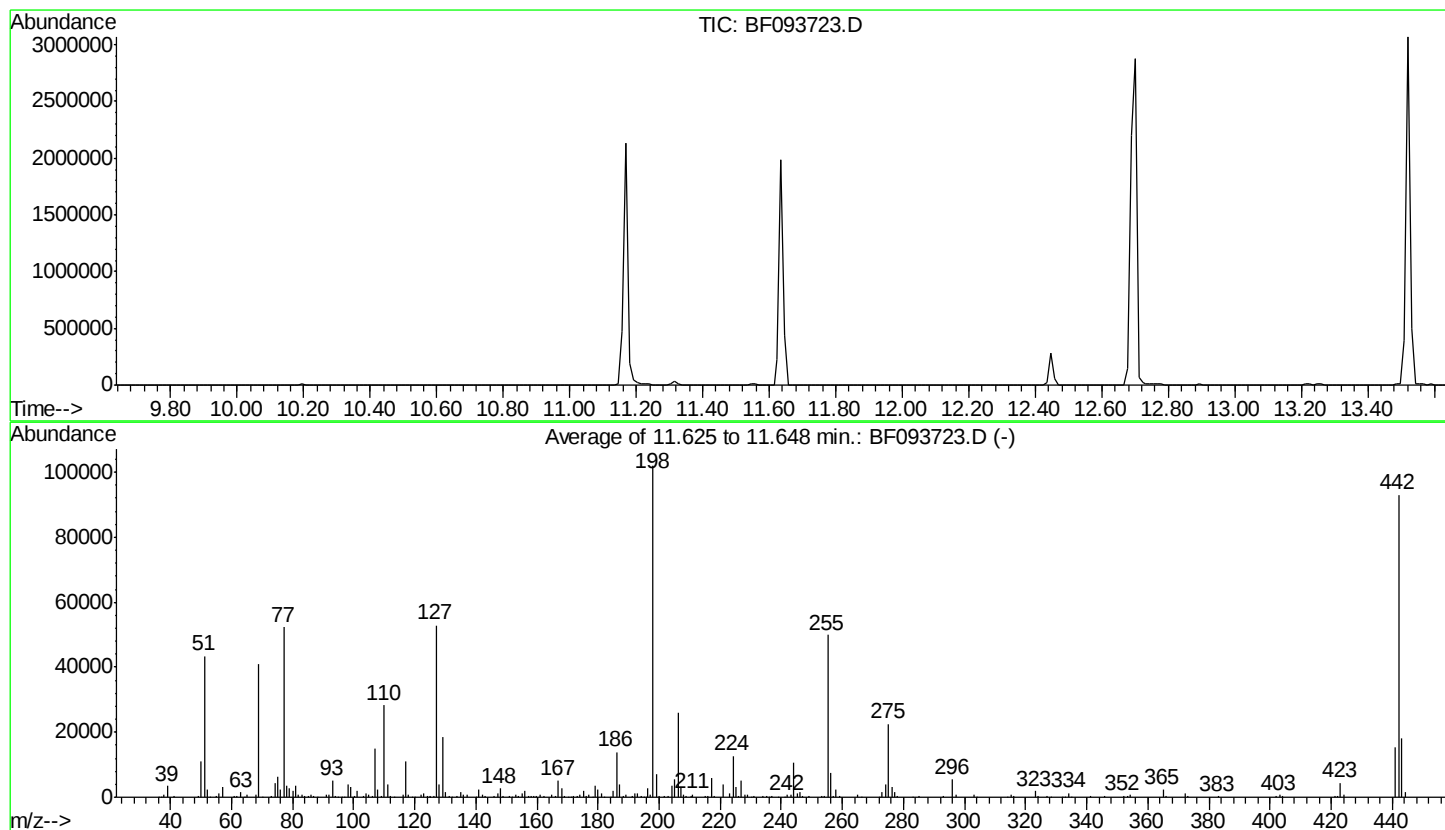

AutoFind: Scans 852, 853, 854; Background Corrected with Scan 849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	43519	PASS
68	69	0.00	2	1.7	693	PASS
69	198	0.00	100	40.2	41054	PASS
70	69	0.00	2	0.4	179	PASS
127	198	10	80	51.9	52918	PASS
197	198	0.00	2	0.9	888	PASS
198	198	100	100	100.0	102010	PASS
199	198	5	9	6.9	7044	PASS
275	198	10	60	22.1	22516	PASS
365	198	1	100	2.3	2317	PASS
441	442	0.01	24	16.5	15332	PASS
442	198	50	100	91.2	93027	PASS
443	442	15	24	19.7	18290	PASS