
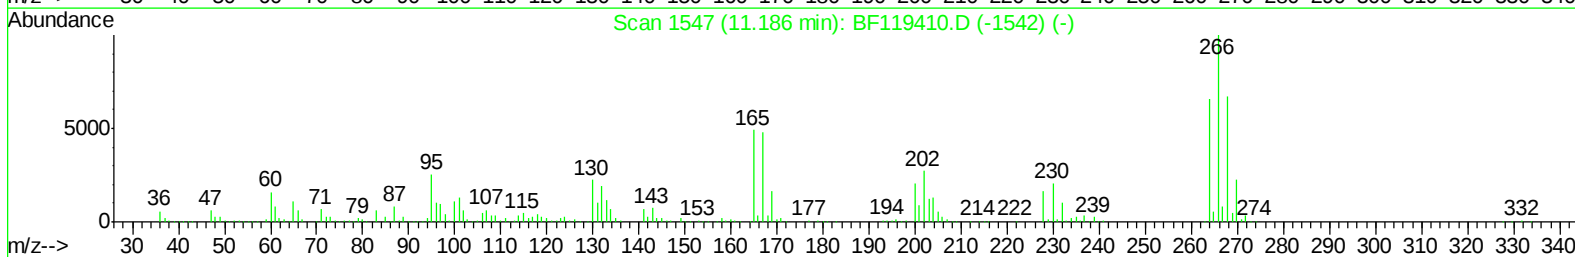
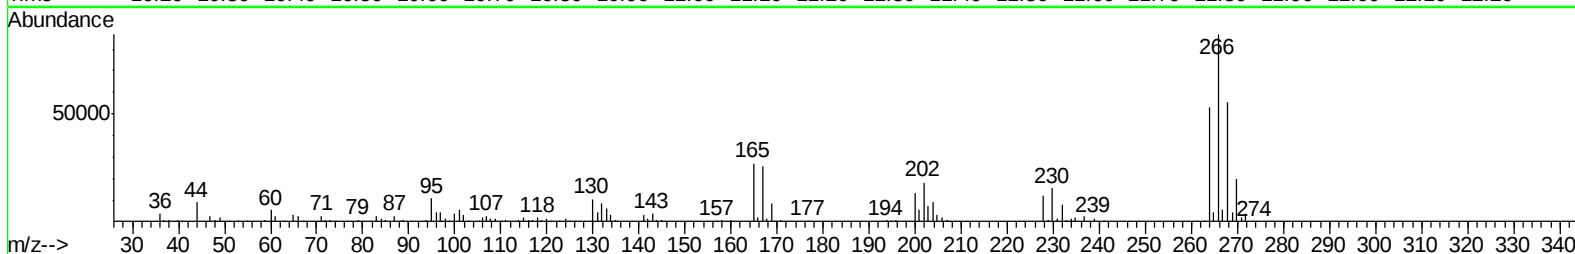


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF031820\  
Data File : BF119416.D  
Acq On : 18 Mar 2020 15:31  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 05:34:00 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF031820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 18 15:11:18 2020  
Response via : Initial Calibration

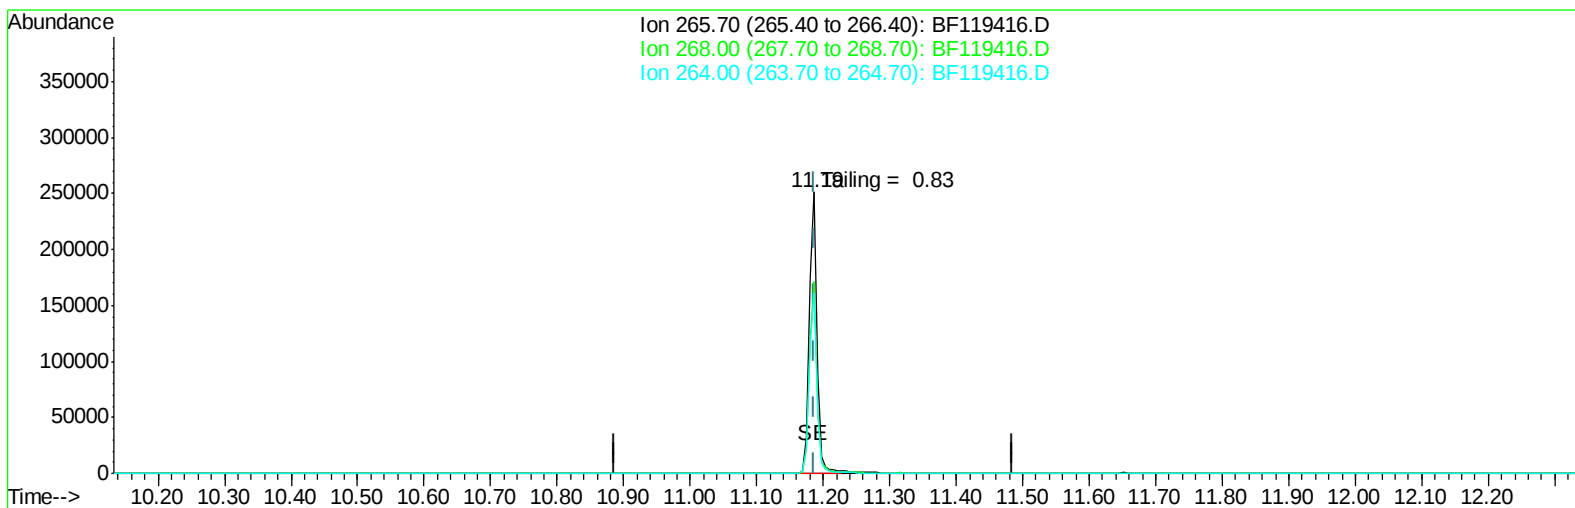

TIC: BF119416.D

(70) Pentachlorophenol (C)




11.186min (+0.000) 50245.44ng

response 208792

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 67.10 | 68.40 |
| 264.00 | 65.60 | 63.92 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF031820\  
 Data File : BF119416.D  
 Acq On : 18 Mar 2020 15:31  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 05:34:00 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF031820.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Mar 18 15:11:18 2020  
 Response via : Initial Calibration

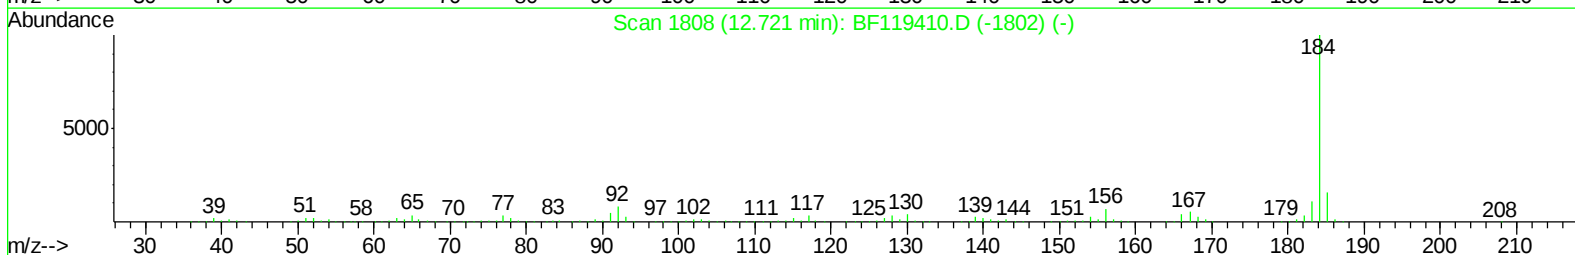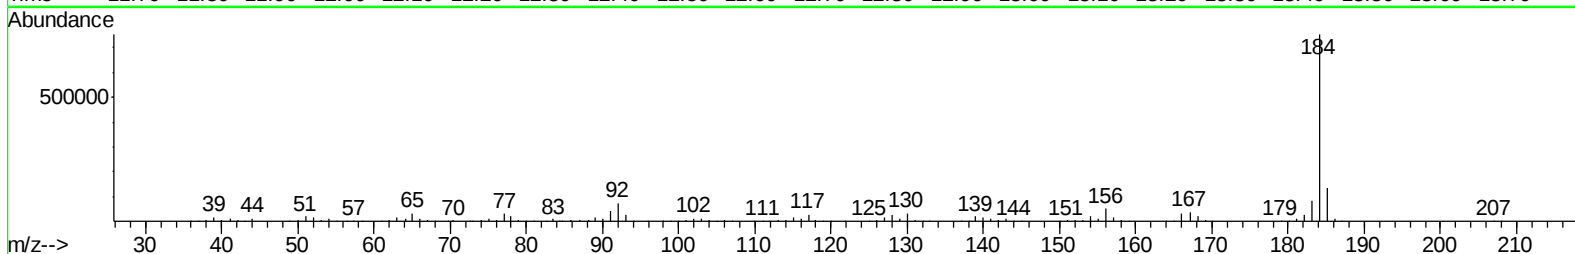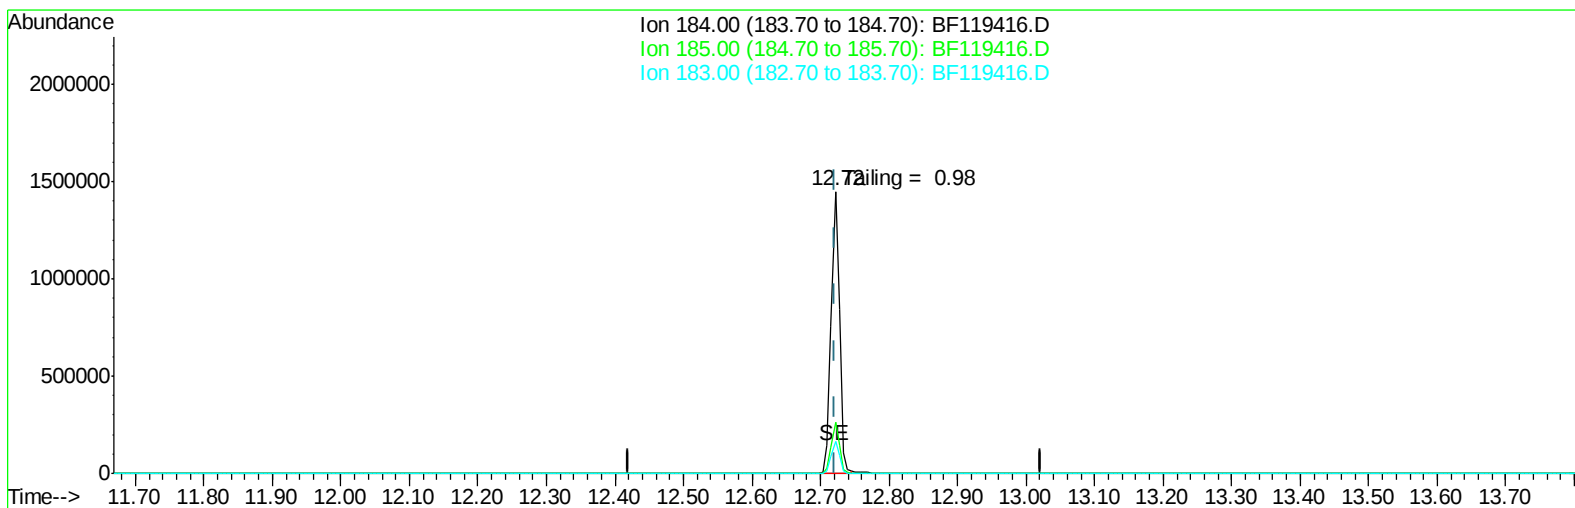

TIC: BF119416.D

(77) Benzidine

12.722min (+0.000) 0.00ng

response 1188857

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.10 | 18.10 |
| 183.00 | 11.20 | 11.21 |
| 0.00   | 0.00  | 0.00  |