


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031820\
 Data File : BF119407.D
 Acq On : 18 Mar 2020 10:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 18 15:11:18 2020

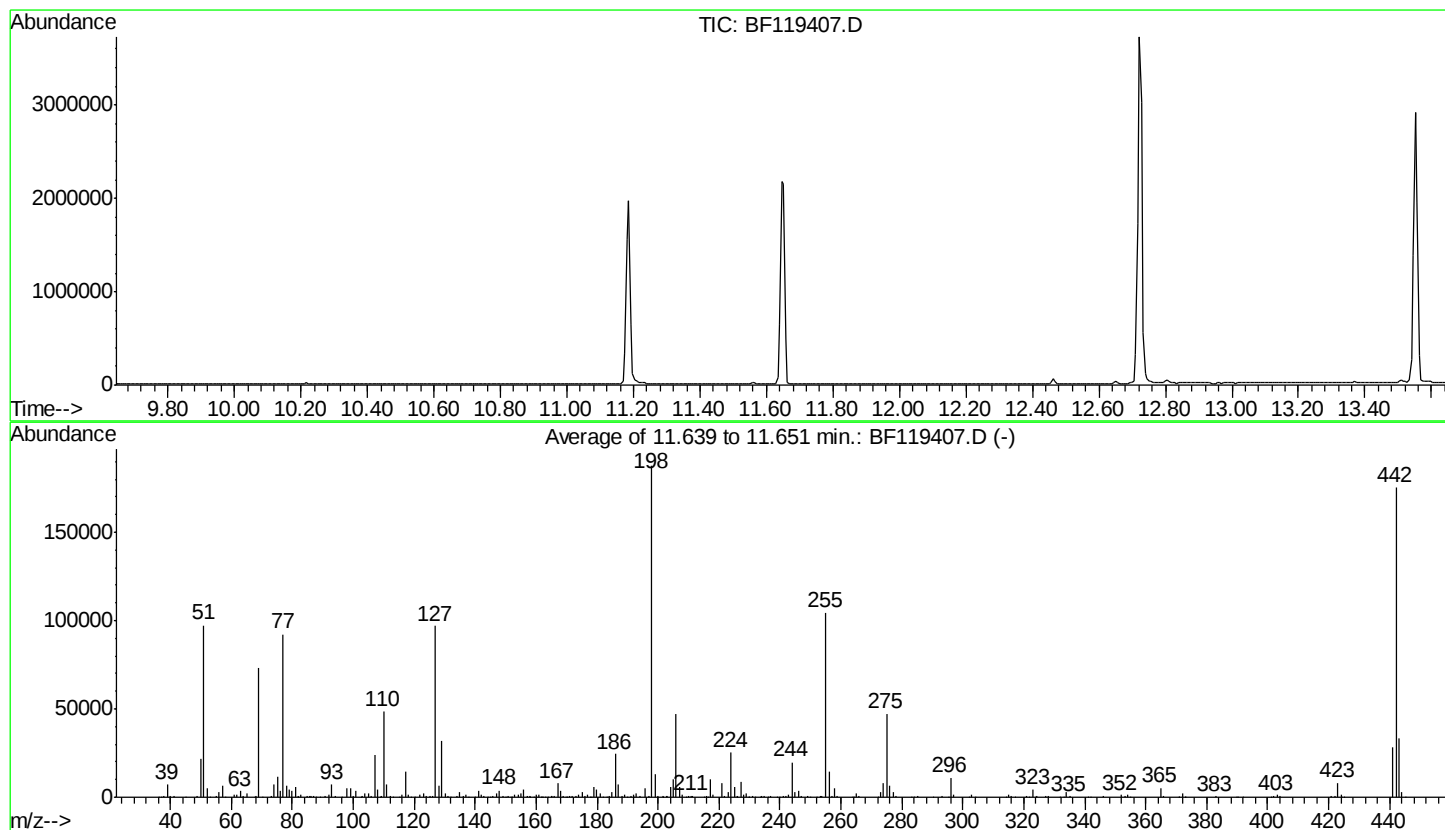

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.9	97494	PASS
68	69	0.00	2	1.5	1070	PASS
69	198	0.00	100	39.1	73322	PASS
70	69	0.00	2	0.3	206	PASS
127	198	10	80	51.6	96853	PASS
197	198	0.00	2	0.6	1092	PASS
198	198	100	100	100.0	187746	PASS
199	198	5	9	6.9	12939	PASS
275	198	10	60	25.2	47283	PASS
365	198	1	100	2.8	5180	PASS
441	198	0.01	100	15.2	28495	PASS
442	198	50	100	93.4	175314	PASS
443	442	15	24	19.0	33235	PASS