
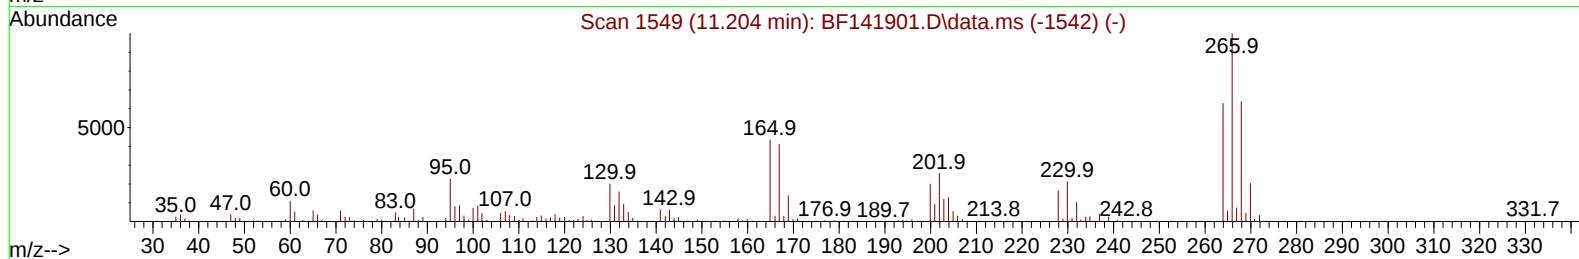
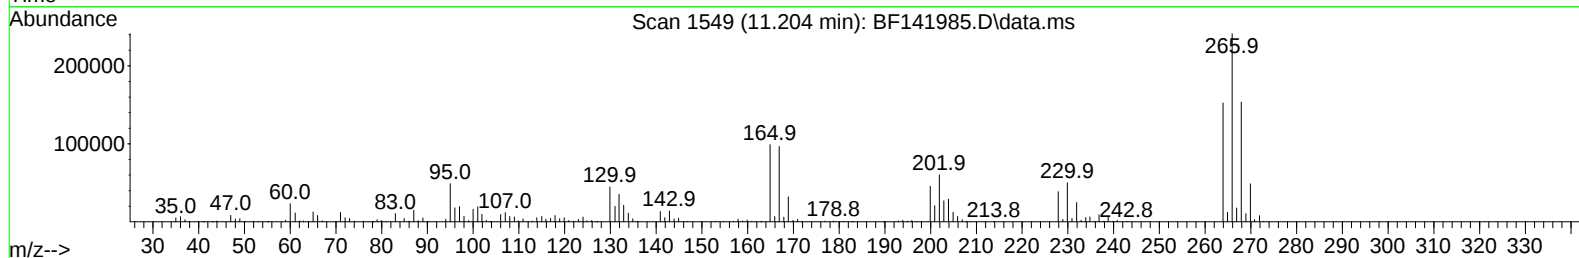


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031825\
Data File : BF141985.D
Acq On : 18 Mar 2025 09:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 11:21:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

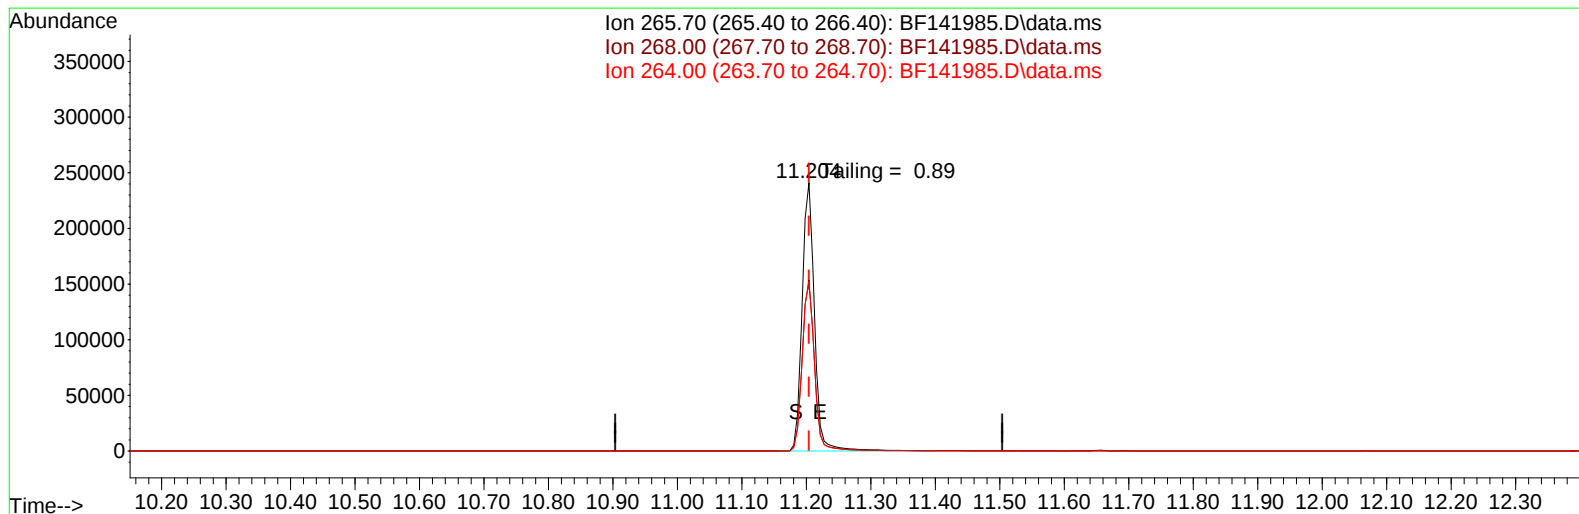

TIC: BF141985.D\data.ms

(70) Pentachlorophenol (C)




11.204min (+ 0.000) 55437.20 ng

response 323218

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.67
264.00	62.70	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031825\
Data File : BF141985.D
Acq On : 18 Mar 2025 09:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 11:21:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

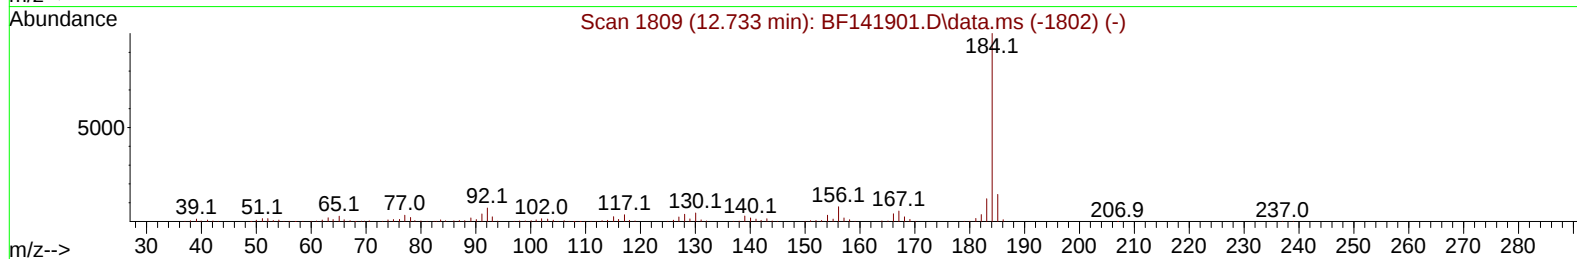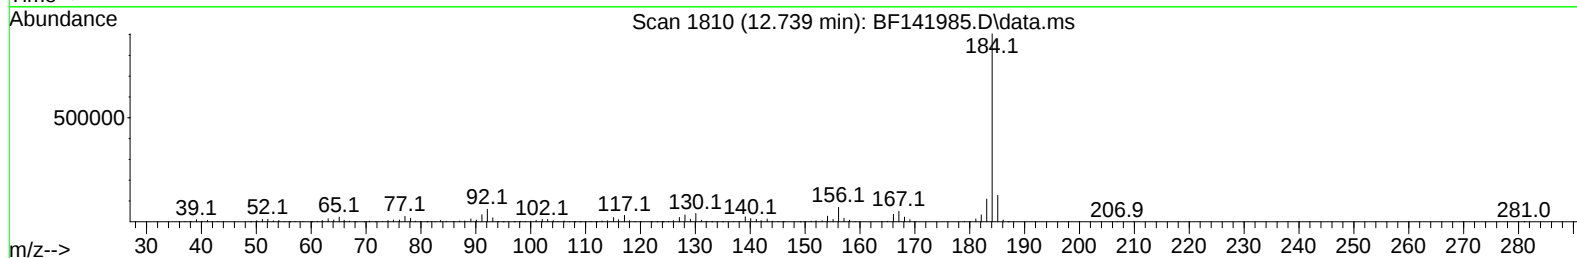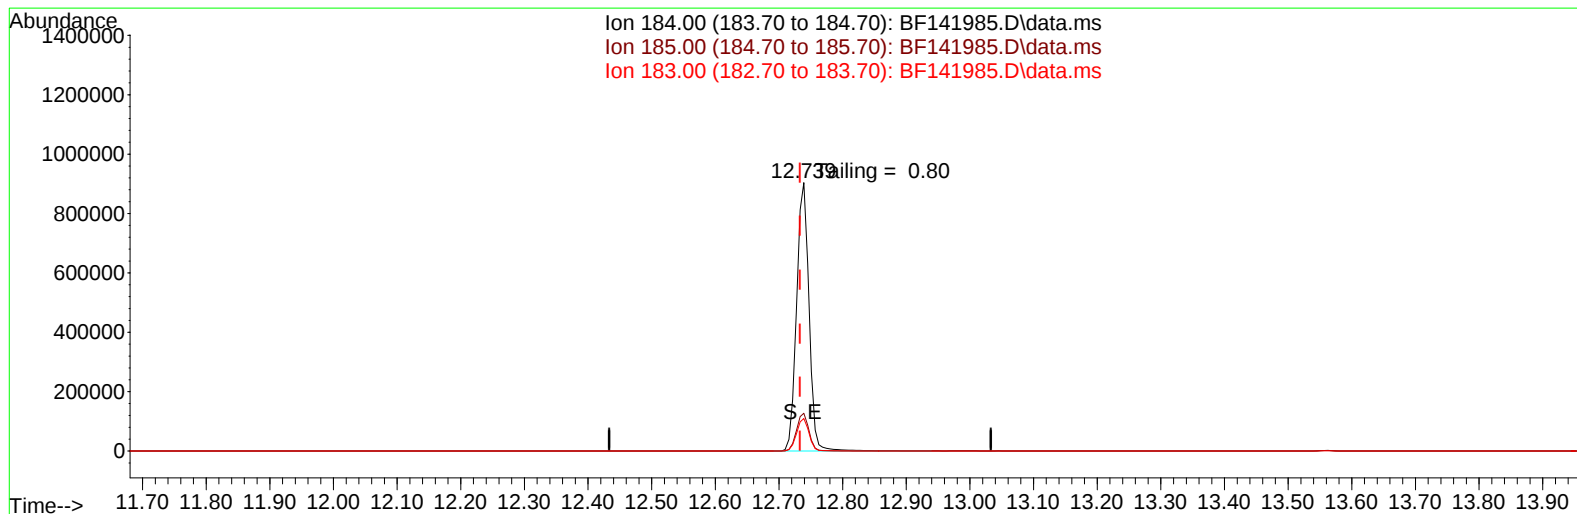

TIC: BF141985.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 128113.33 ng

response 1226172

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.06
183.00	12.10	12.12
0.00	0.00	0.00