


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031915\
 Data File : BF077829.D
 Acq On : 19 Mar 2015 13:30
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 02:09:19 2015

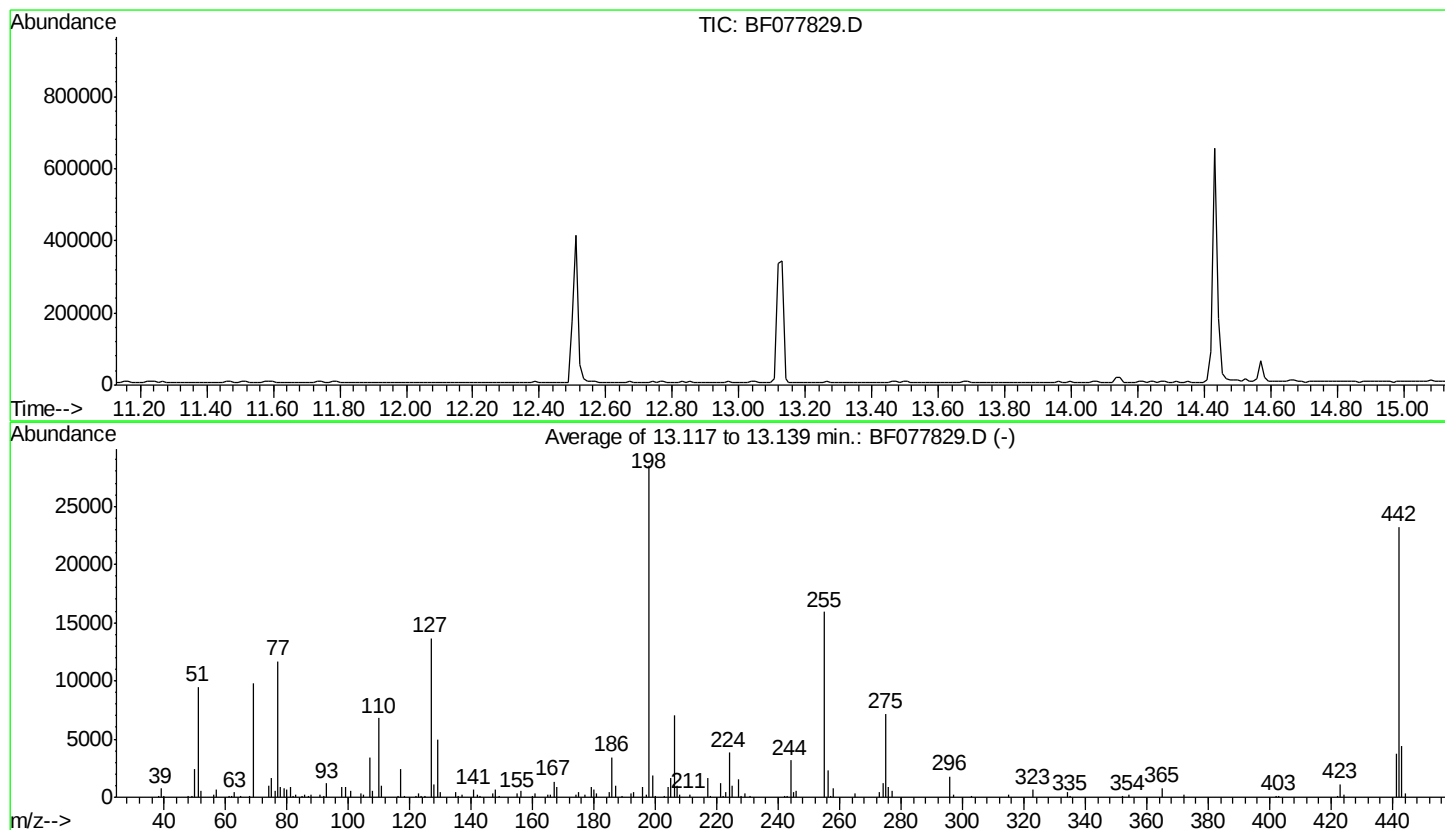

AutoFind: Scans 1070, 1071, 1072; Background Corrected with Scan 1066

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	9470	PASS
68	69	0.00	2	1.1	105	PASS
69	198	0.00	100	34.4	9788	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	13688	PASS
197	198	0.00	2	0.8	231	PASS
198	198	100	100	100.0	28490	PASS
199	198	5	9	6.7	1897	PASS
275	198	10	60	25.3	7203	PASS
365	198	1	100	2.7	773	PASS
441	442	0.01	24	16.3	3793	PASS
442	198	50	100	81.5	23210	PASS
443	442	15	24	19.1	4433	PASS