


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031915\
 Data File : BF077848.D
 Acq On : 20 Mar 2015 00:31
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 20 01:13:23 2015

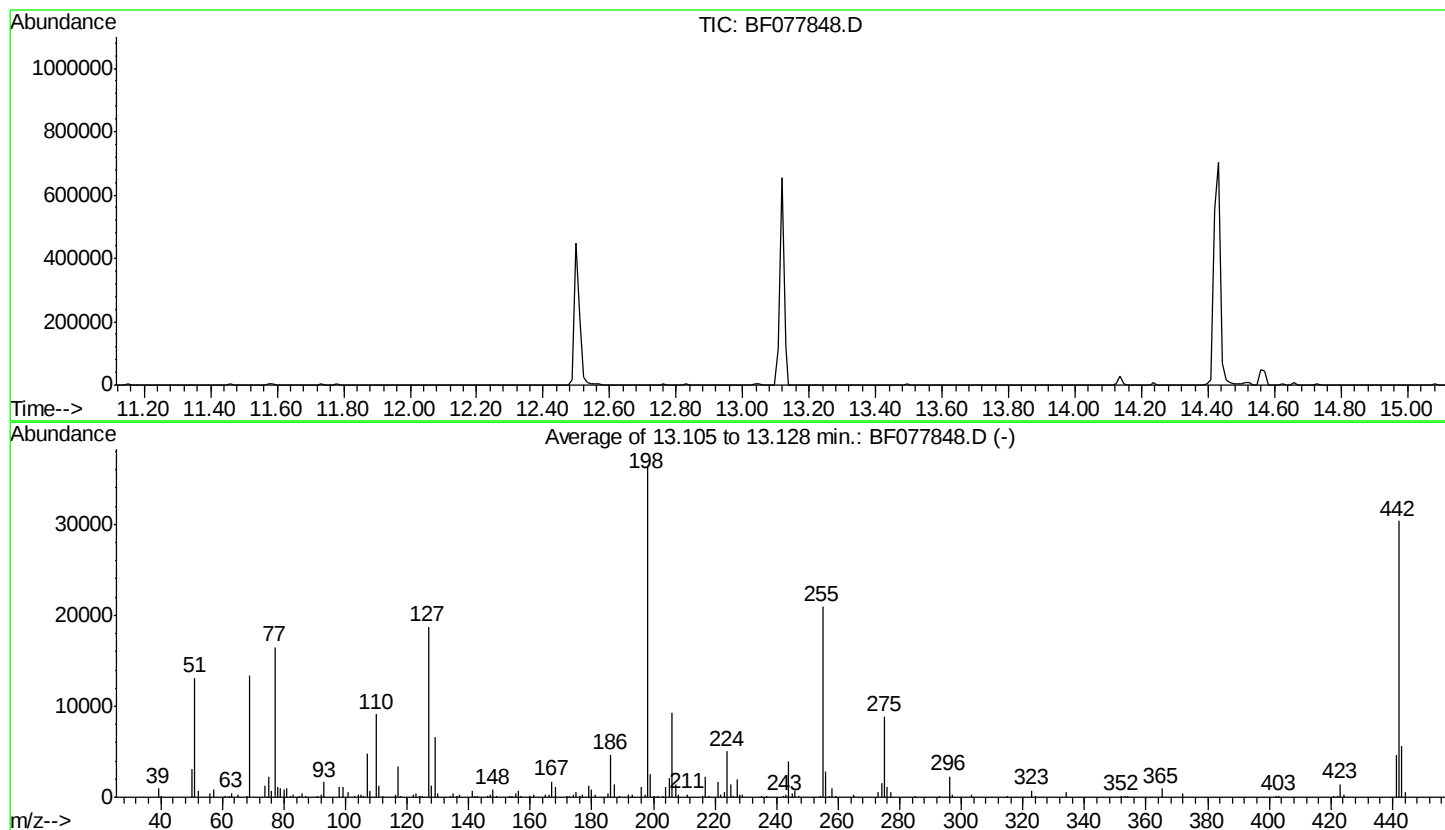

AutoFind: Scans 1069, 1070, 1071; Background Corrected with Scan 1066

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	13126	PASS
68	69	0.00	2	1.0	139	PASS
69	198	0.00	100	36.7	13355	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.4	18727	PASS
197	198	0.00	2	0.7	254	PASS
198	198	100	100	100.0	36438	PASS
199	198	5	9	6.8	2467	PASS
275	198	10	60	24.2	8834	PASS
365	198	1	100	2.6	956	PASS
441	442	0.01	24	15.1	4577	PASS
442	198	50	100	83.3	30353	PASS
443	442	15	24	18.4	5589	PASS