

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031918\
 Data File : BF103795.D
 Acq On : 20 Mar 2018 9:55
 Operator : JU/SJ
 Sample : J1954-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Mar 20 10:51:17 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 18:31:53 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	153846	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	604611	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	266348	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	420748	20.00	ng	0.00
75) Chrysene-d12	14.16	240	302135	20.00	ng	0.00
86) Perylene-d12	15.70	264	257786	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	412328	40.76	ng	0.00
7) Phenol-d6	6.58	99	307558	24.85	ng	0.00
23) Nitrobenzene-d5	7.53	82	998079	115.12	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	239381	104.53	ng	0.00
44) 2-Fluorobiphenyl	9.33	172	1587893	95.10	ng	0.00
78) Terphenyl-d14	13.10	244	1258551	96.69	ng	0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.53	70	132417	16.697	ng	# 73
25) Isophorone	7.53	82	998059	49.728	ng	# 64
47) 2-Nitroaniline	9.33	65	2418	7.264	ng	# 1
50) 2,6-Dinitrotoluene	10.01	165	34341	11.995	ng	# 25
56) 2,4-Dinitrotoluene	10.01	165	34341	12.217	ng	# 23
64) 4,6-Dinitro-2-methylphenol	10.80	198	438	8.428	ng	# 1
66) 4-Bromophenyl-phenylether	10.80	248	14447	3.344	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031918\
Data File : BF103795.D
Acq On : 20 Mar 2018 9:55
Operator : JU/SJ
Sample : J1954-06
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 20 10:51:17 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

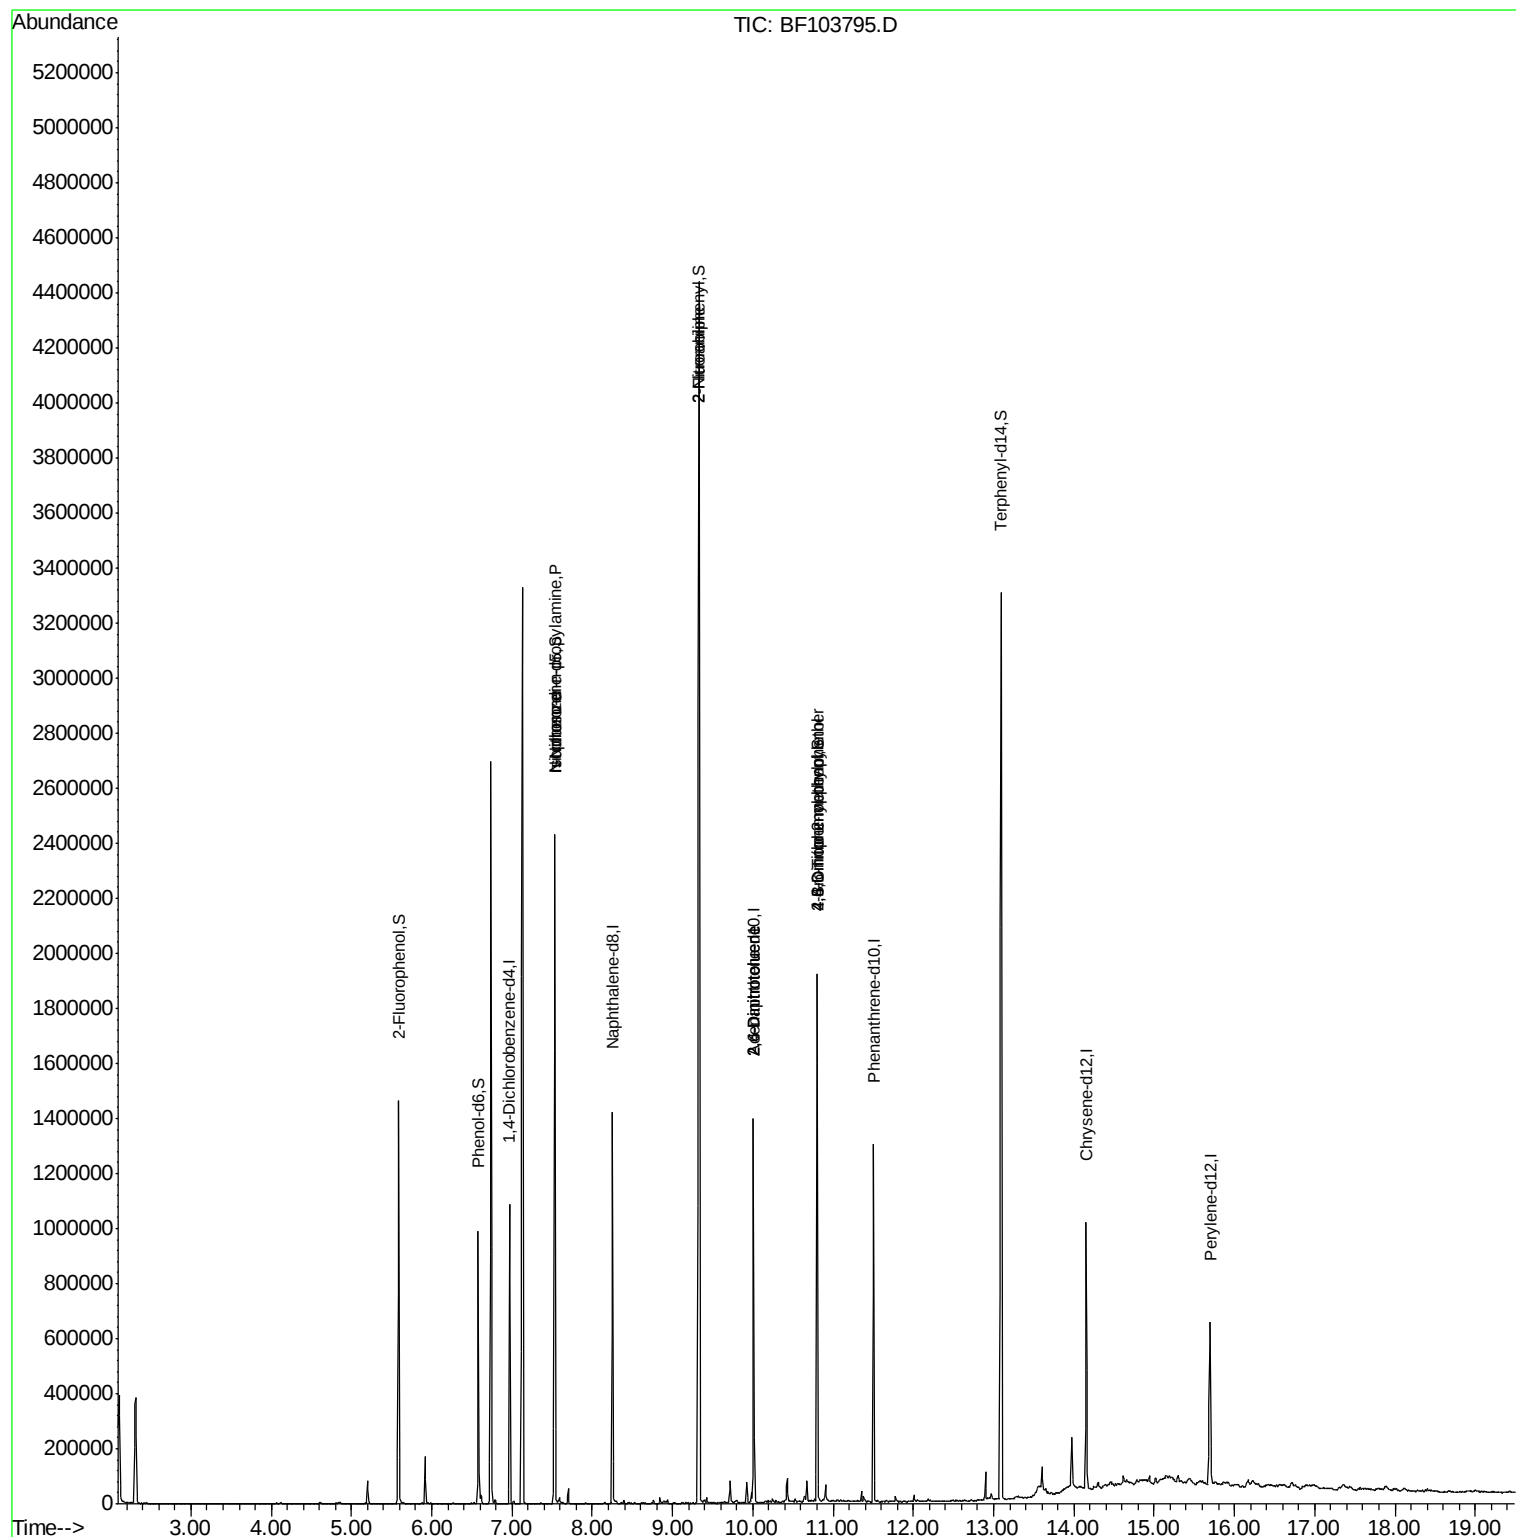




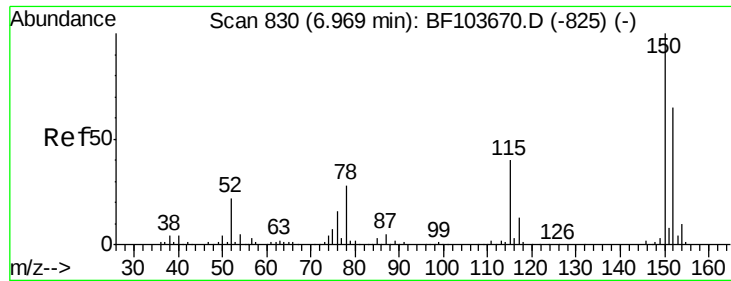


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 830
Delta R.T. -0.00 min
Lab File: BF103795.D
Acq: 20 Mar 2018 9:55

Instrument :
BNA_F
ClientSampleId :




Tot Ion	Ratio	Lower	Upper
152	100		
150	160.4	124.6	186.8
115	65.0	50.1	75.1

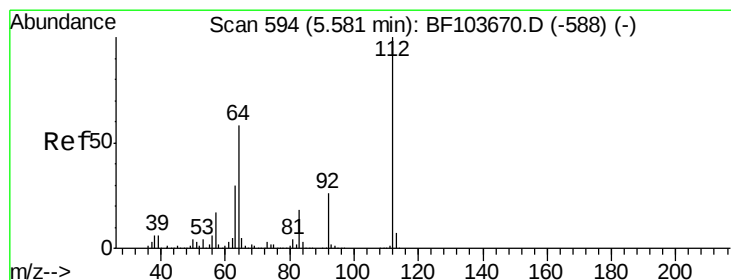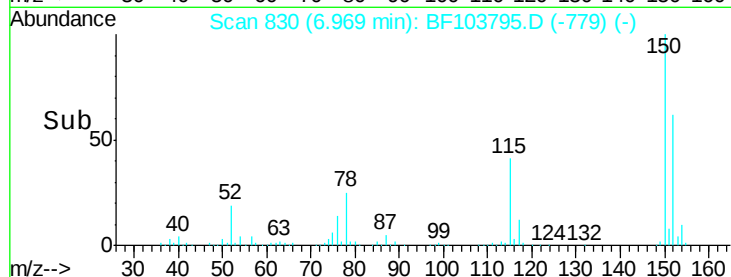
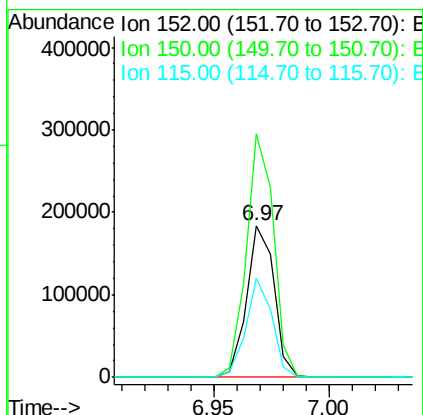
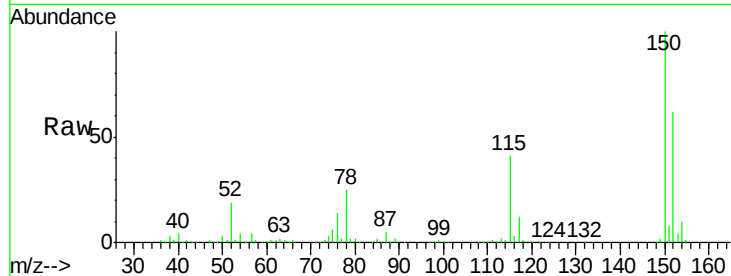


#5

2-Fluorophenol
Concen: 40.765 ng
RT: 5.59 min Scan# 595
Delta R.T. 0.01 min
Lab File: BF103795.D
Acq: 20 Mar 2018 9:55

Tgt Ion	Ratio	Lower	Upper
112	100		
64	55.7	47.9	71.9
63	28.0	23.7	35.5

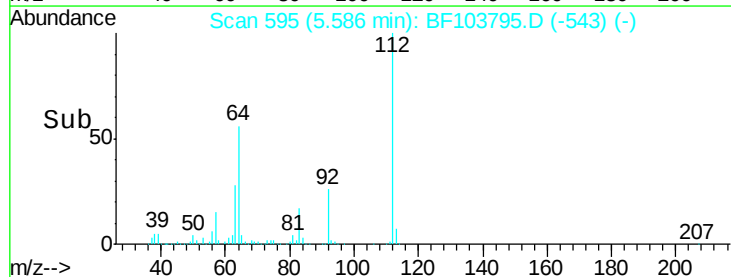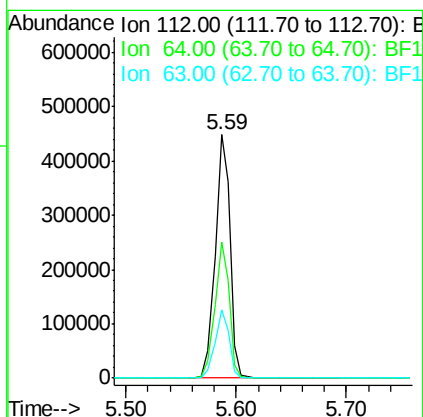

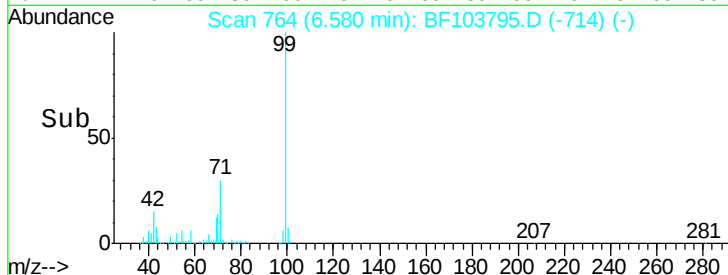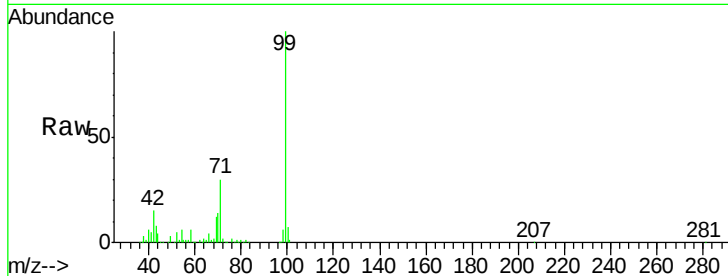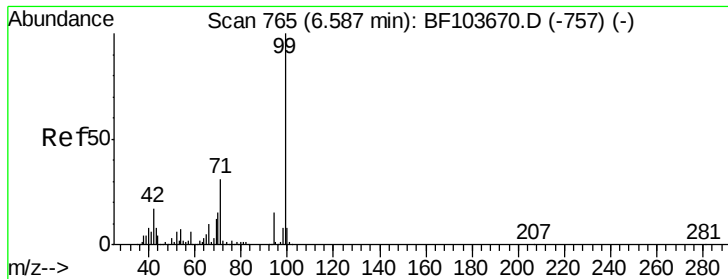

#7

Phenol-d6

Concen: 24.854 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.01 min

Lab File: BF103795.D

Acq: 20 Mar 2018 9:55

Instrument :

BNA_F

ClientSampled :





Tot Ion: 99 Resp: 307558

Ion Ratio Lower Upper

99 100

42 15.3 14.5 21.7

71 30.5 25.4 38.0

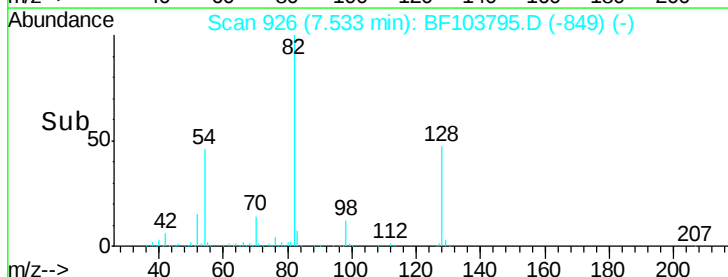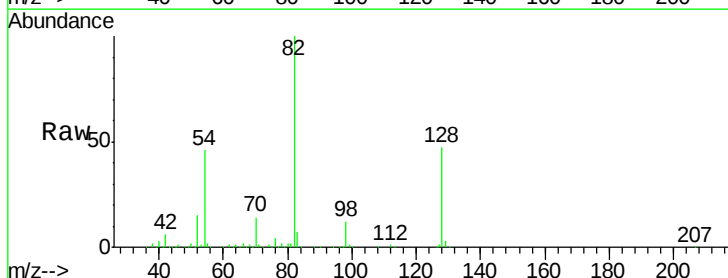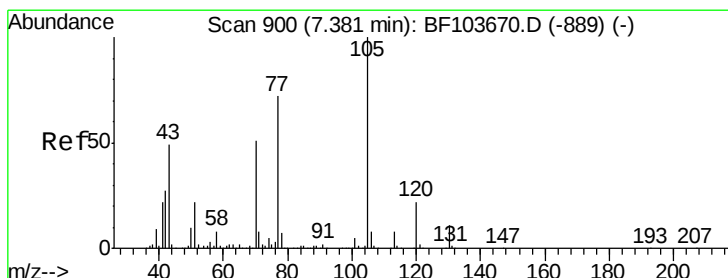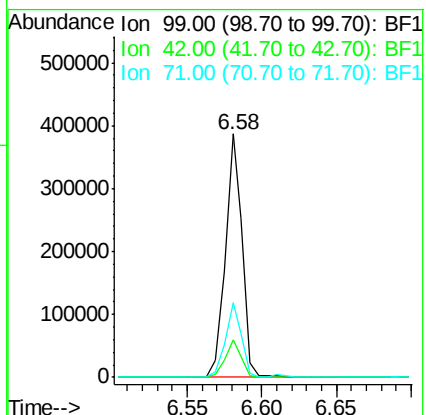

#19

n-Nitroso-di-n-propylamine

Concen: 16.697 ng

RT: 7.53 min Scan# 926

Delta R.T. 0.15 min

Lab File: BF103795.D

Acq: 20 Mar 2018 9:55

Tgt Ion: 70 Resp: 132417


Ion Ratio Lower Upper


70 100

42 41.7 47.5 71.3#

101 0.0 7.4 11.2#

130 2.4 16.6 25.0#

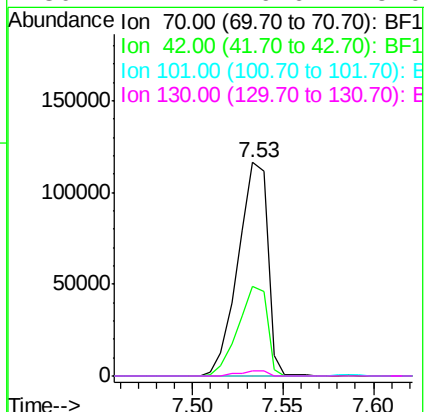

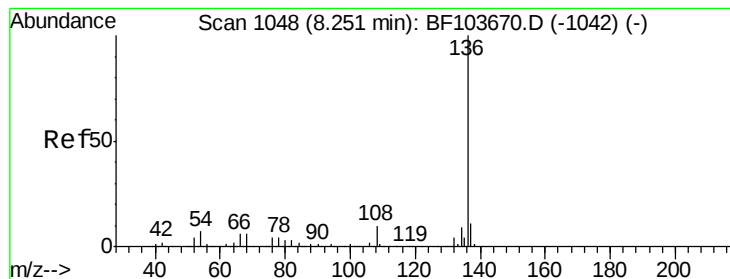

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1048

Delta R.T. -0.00 min

Lab File: BF103795.D

Acq: 20 Mar 2018 9:55

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 604611


Ion Ratio Lower Upper

136 100

137 11.3 8.9 13.3

54 7.3 6.6 9.8

68 6.5 5.0 7.4



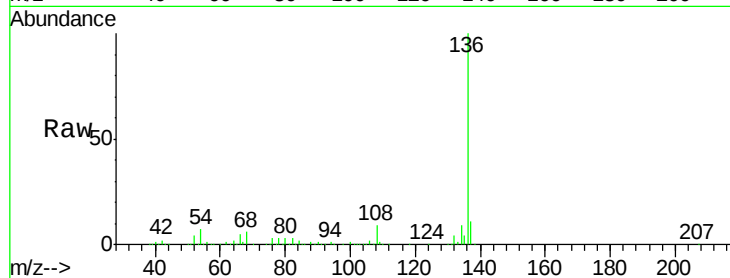


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

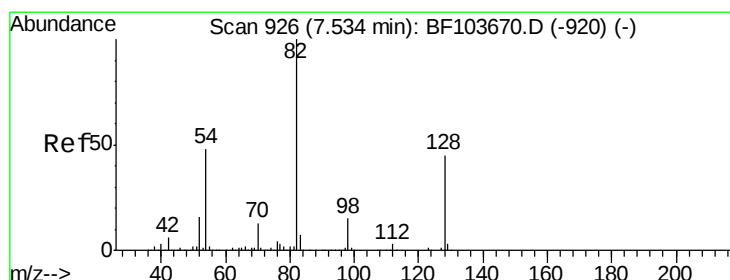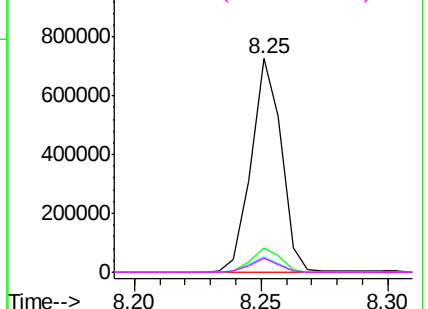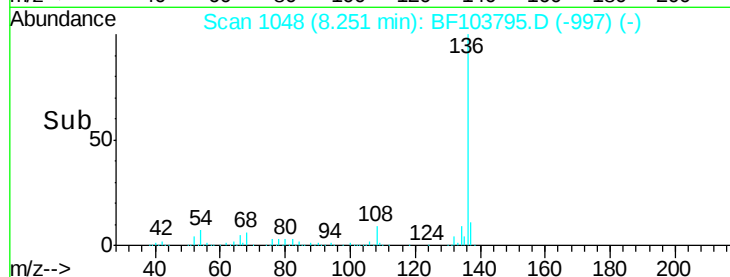

#23

Nitrobenzene-d5

Concen: 115.119 ng

RT: 7.53 min Scan# 926

Delta R.T. -0.00 min

Lab File: BF103795.D

Acq: 20 Mar 2018 9:55


Tgt Ion: 82 Resp: 998079

Ion Ratio Lower Upper

82 100

128 46.7 36.1 54.1



54 45.5 41.4 62.2

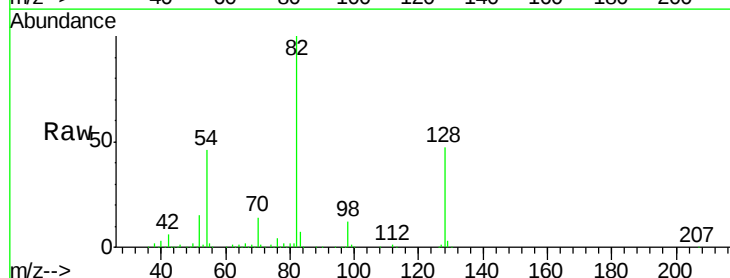


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

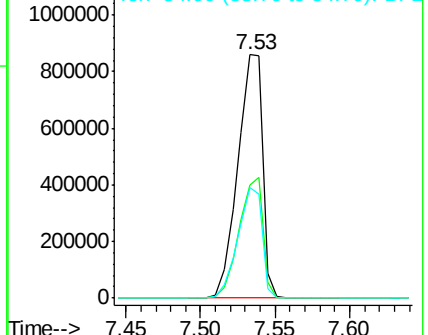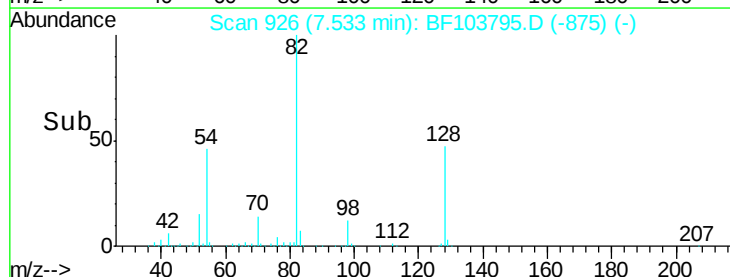

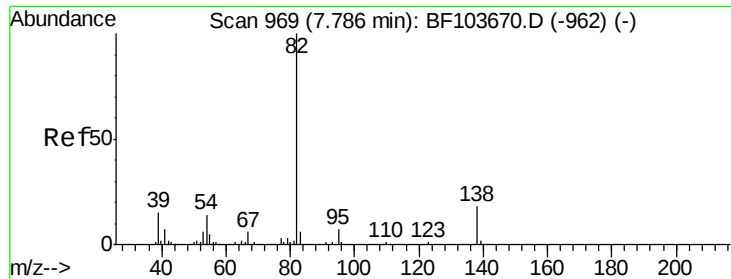

#25

Isophorone

Concen: 49.728 ng

RT: 7.53 min Scan# 926

Delta R.T. -0.25 min

Lab File: BF103795.D

Acq: 20 Mar 2018 9:55

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 998059

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

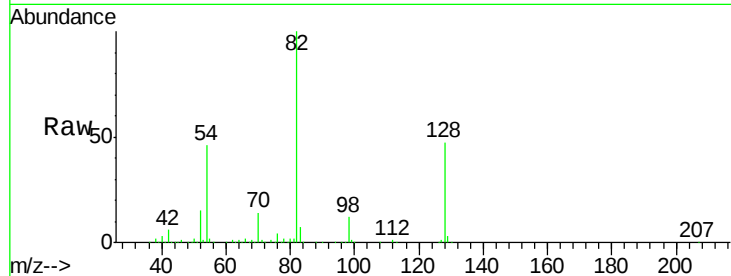

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

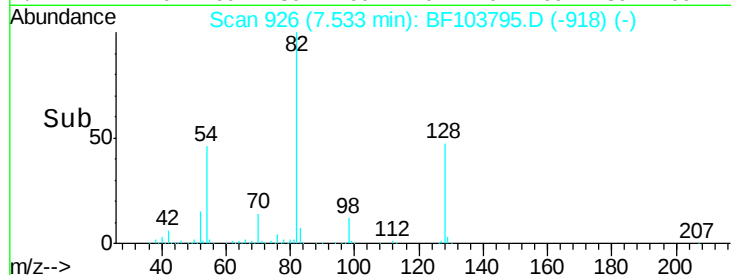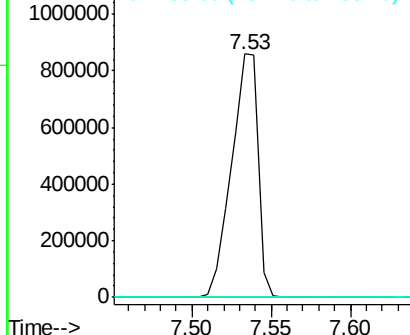

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.01 min Scan# 1347

Delta R.T. -0.00 min

Lab File: BF103795.D

Acq: 20 Mar 2018 9:55


Tgt Ion:164 Resp: 266348

Ion Ratio Lower Upper



164 100


162 103.9 86.1 129.1

160 46.1 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

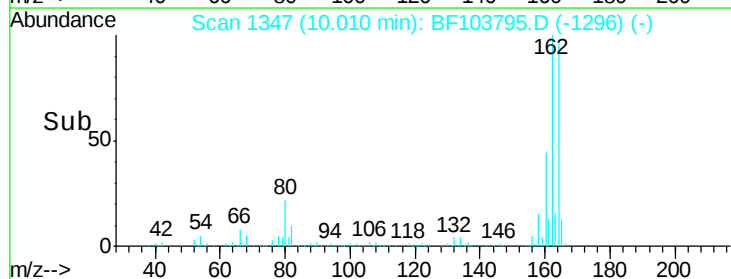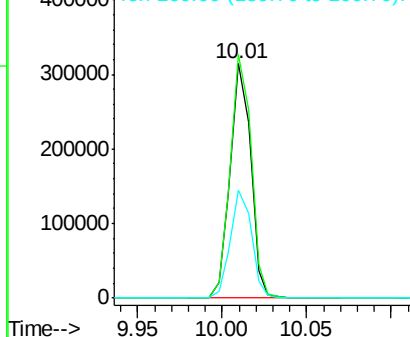


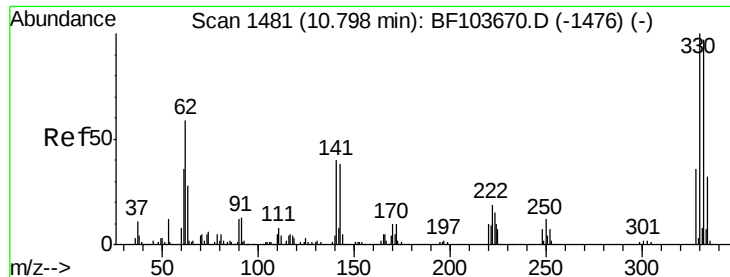




#41
 2,4,6-Tribromophenol
 Concen: 104.530 ng
 RT: 10.80 min Scan# 1482
 Delta R.T. 0.01 min
 Lab File: BF103795.D
 Acq: 20 Mar 2018 9:55

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 239381
 Ion Ratio Lower Upper
 330 100
 332 95.4 77.0 115.6
 141 32.9 29.9 44.9

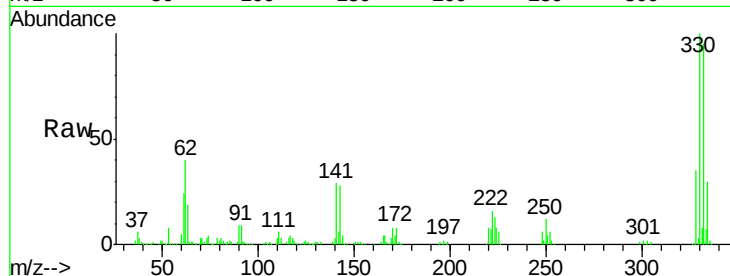


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

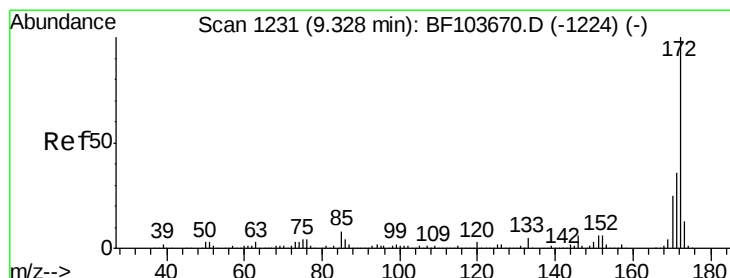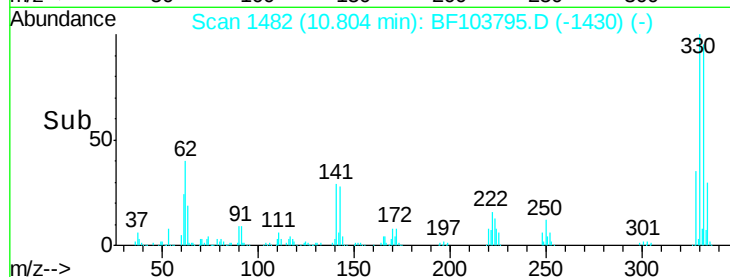
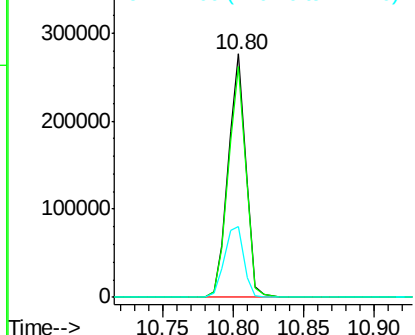



#44
 2-Fluorobiphenyl
 Concen: 95.098 ng
 RT: 9.33 min Scan# 1231
 Delta R.T. 0.00 min
 Lab File: BF103795.D
 Acq: 20 Mar 2018 9:55

Tgt Ion:172 Resp: 1587893
 Ion Ratio Lower Upper
 172 100
 171 36.9 29.7 44.5
 170 23.9 19.6 29.4

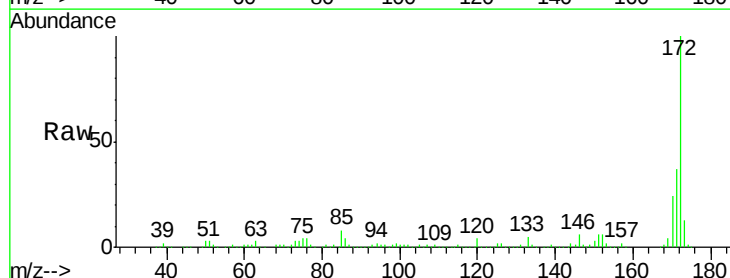

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



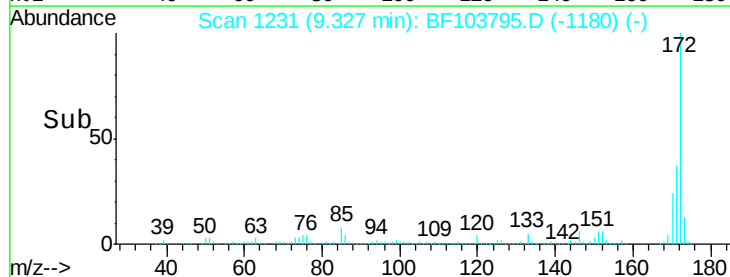
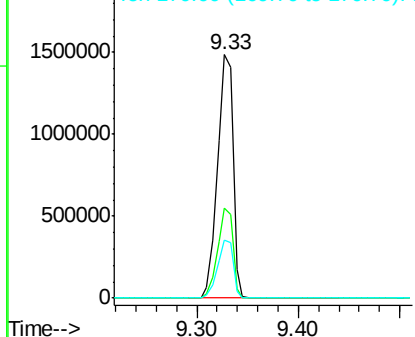


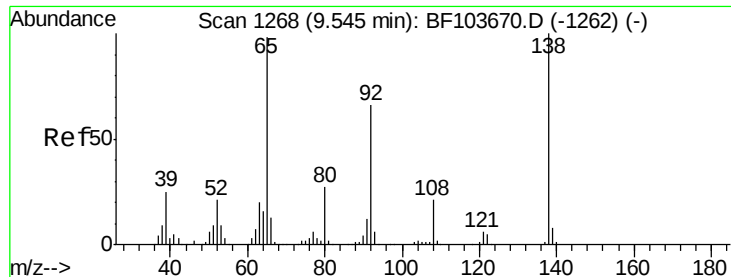

#47
2-Nitroaniline
Concen: 7.264 ng
RT: 9.33 min Scan# 1231
Delta R.T. -0.22 min
Lab File: BF103795.D
Acq: 20 Mar 2018 9:55




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 65 Resp: 2418
Ion Ratio Lower Upper
65 100
92 217.2 55.8 83.6#
138 44.7 91.2 136.8#

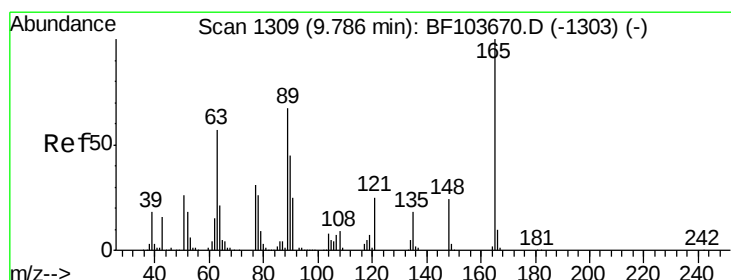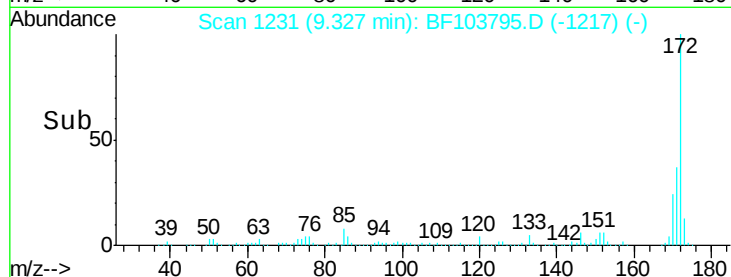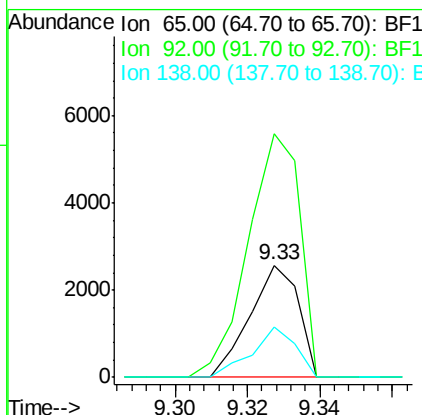

#50
2,6-Dinitrotoluene
Concen: 11.995 ng
RT: 10.01 min Scan# 1347
Delta R.T. 0.22 min
Lab File: BF103795.D
Acq: 20 Mar 2018 9:55

Tgt Ion:165 Resp: 34341
Ion Ratio Lower Upper
165 100
63 1.4 44.7 67.1#
89 1.3 44.0 66.0#

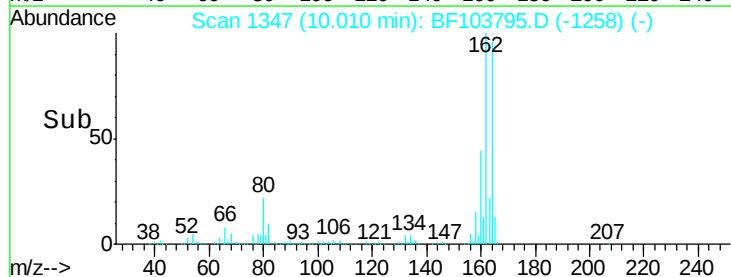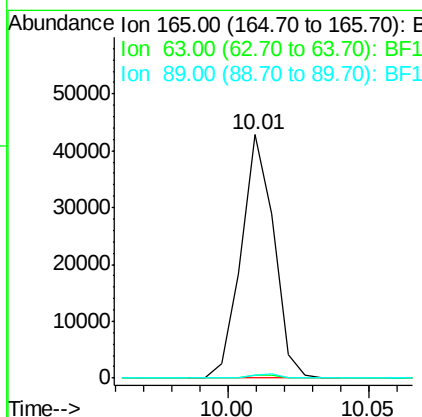


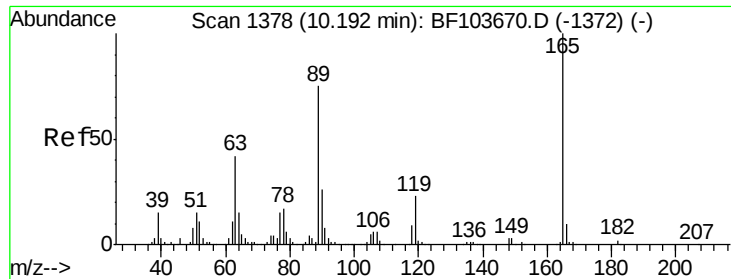




#56
2,4-Dinitrotoluene
Concen: 12.217 ng
RT: 10.01 min Scan# 1347
Delta R.T. -0.18 min
Lab File: BF103795.D
Acq: 20 Mar 2018 9:55

Instrument :
BNA_F
ClientSampleId :

Tot Ion:165 Resp: 34341
Ion Ratio Lower Upper
165 100
63 1.4 36.4 54.6#
89 1.3 57.8 86.6#
182 0.0 1.6 2.4#




Abundance Ion 165.00 (164.70 to 165.70): E

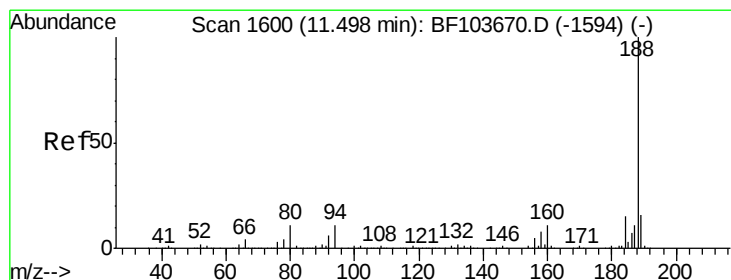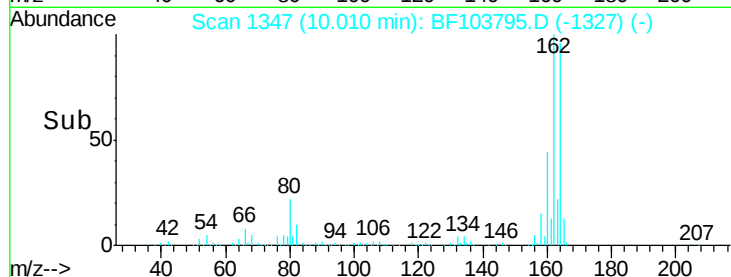
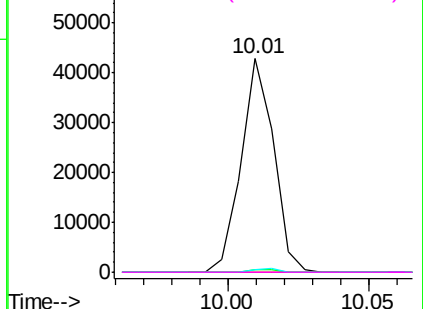



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.50 min Scan# 1601
Delta R.T. 0.01 min
Lab File: BF103795.D
Acq: 20 Mar 2018 9:55

Tgt Ion:188 Resp: 420748
Ion Ratio Lower Upper
188 100
94 10.8 8.5 12.7
80 11.3 9.2 13.8



Abundance Ion 188.00 (187.70 to 188.70): E

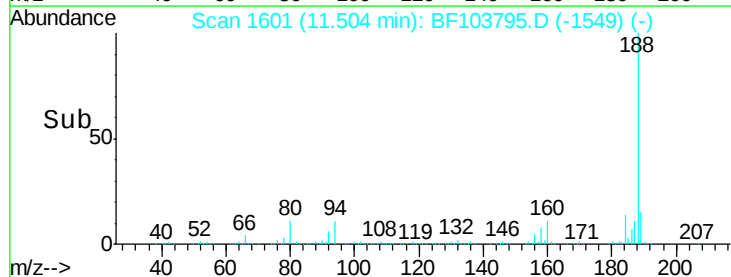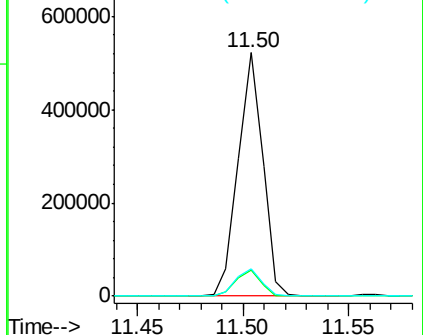


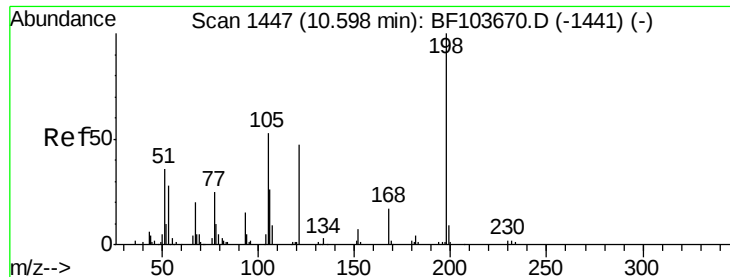




#64
4,6-Dinitro-2-methylphenol
Concen: 8.428 ng
RT: 10.80 min Scan# 1482
Delta R.T. 0.21 min
Lab File: BF103795.D
Acq: 20 Mar 2018 9:55

Instrument :
BNA_F
ClientSampled :

Tot Ion:198 Resp: 438
Ion Ratio Lower Upper
198 100
51 140.2 37.7 77.7#
105 193.6 36.3 76.3#

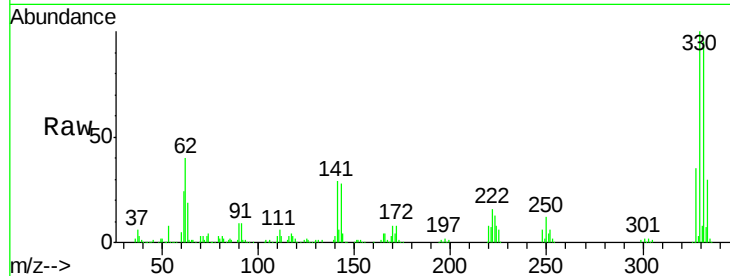


Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BF1
Ion 105.00 (104.70 to 105.70): E

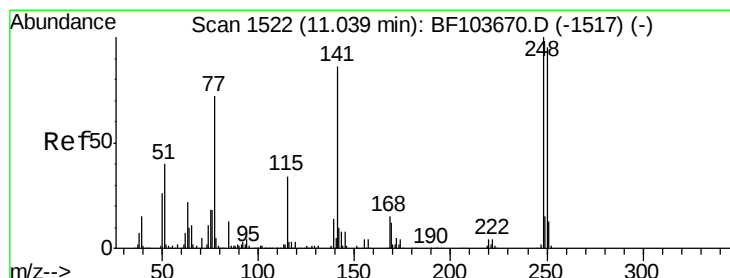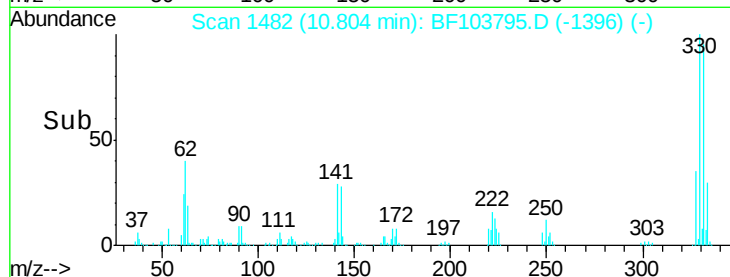
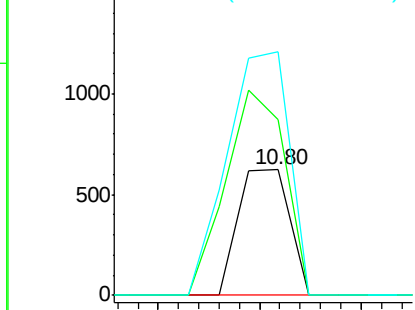



#66
4-Bromophenyl-phenylether
Concen: 3.344 ng
RT: 10.80 min Scan# 1482
Delta R.T. -0.24 min
Lab File: BF103795.D
Acq: 20 Mar 2018 9:55

Tgt Ion:248 Resp: 14447
Ion Ratio Lower Upper
248 100
250 189.4 76.9 115.3#
141 480.7 74.4 111.6#

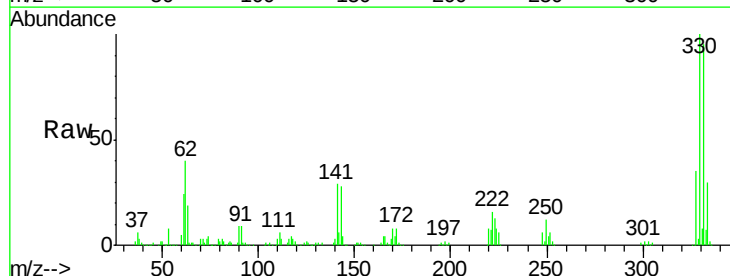

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

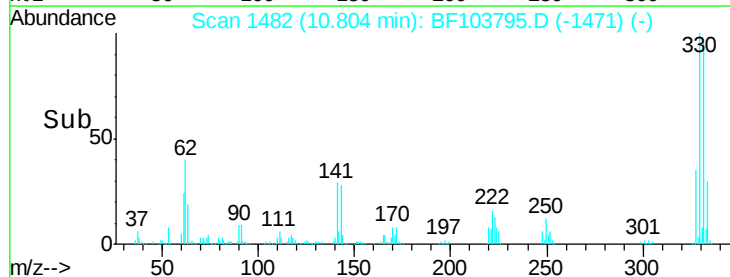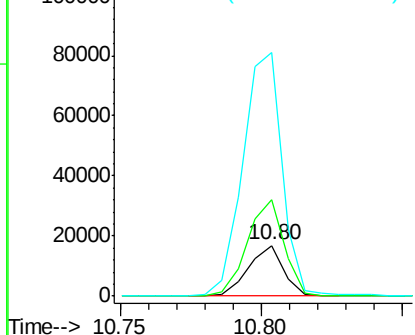

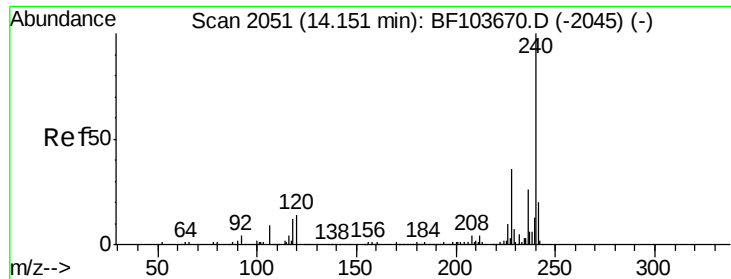

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.16 min Scan# 2052

Delta R.T. 0.01 min

Lab File: BF103795.D

Acq: 20 Mar 2018 9:55

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 302135

Ion Ratio Lower Upper

240 100

120 12.6 9.5 14.3




236 25.7 20.7 31.1

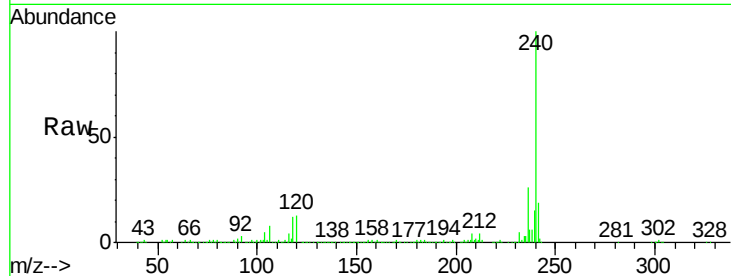

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

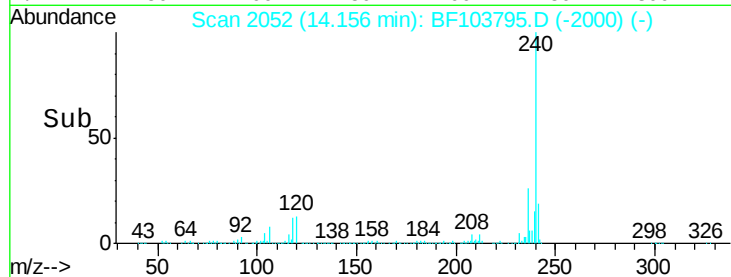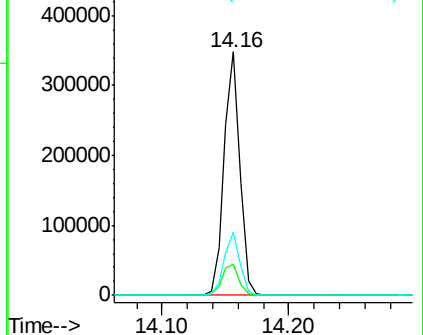

#78

Terphenyl-d14

Concen: 96.688 ng

RT: 13.10 min Scan# 1872

Delta R.T. 0.01 min

Lab File: BF103795.D

Acq: 20 Mar 2018 9:55


Tgt Ion:244 Resp: 1258551

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0



122 11.4 11.0 16.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

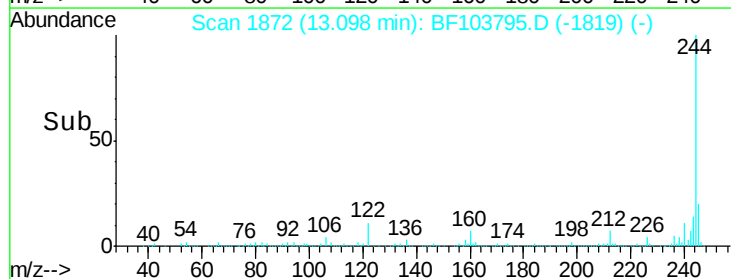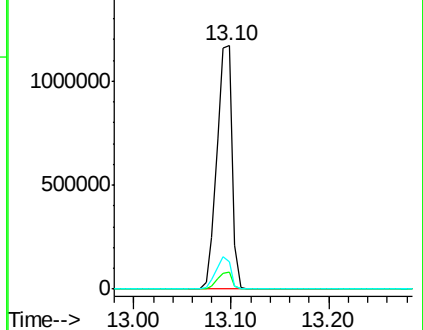


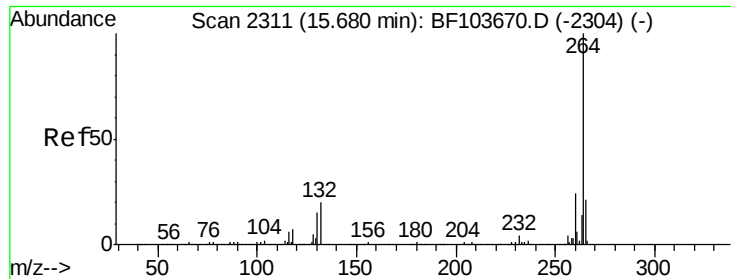

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.70 min Scan# 2314
Delta R.T. 0.02 min
Lab File: BF103795.D
Acq: 20 Mar 2018 9:55

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 264 Resp: 257786
Ion Ratio Lower Upper
264 100
260 23.9 19.2 28.8
265 21.4 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

