
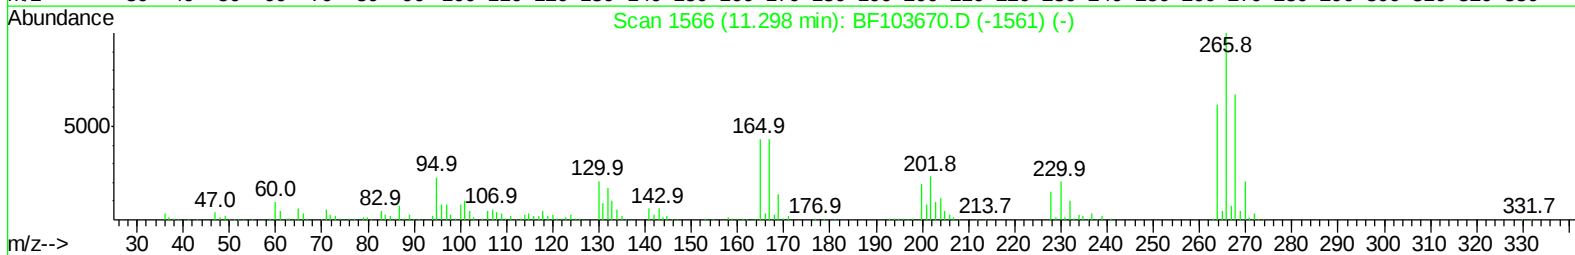
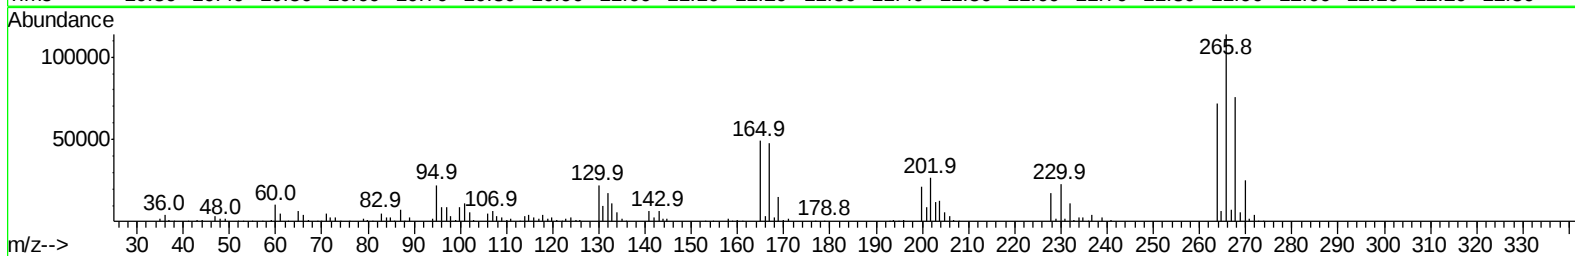


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF031918\
Data File : BF103758.D
Acq On : 19 Mar 2018 15:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 06:11:06 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

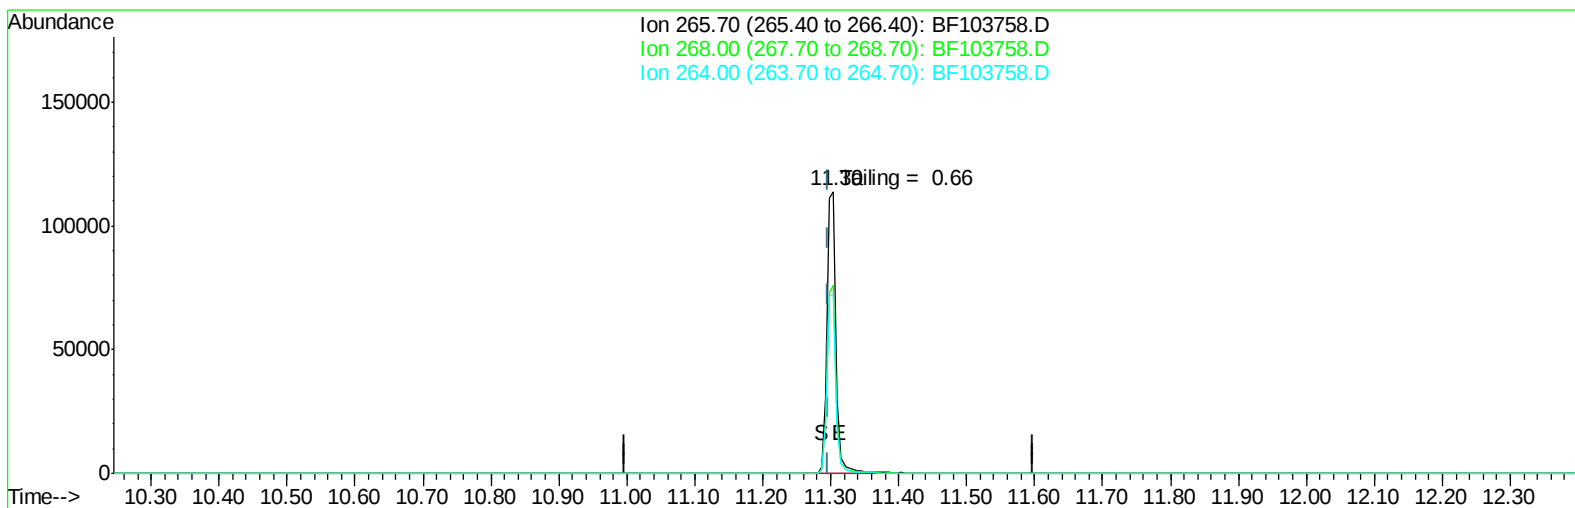

TIC: BF103758.D

(69) Pentachlorophenol (C)




11.304min (+0.006) 43413.26ng

response 107926

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.81
264.00	61.90	63.29
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF031918\
 Data File : BF103758.D
 Acq On : 19 Mar 2018 15:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 06:11:06 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 18:31:53 2018
 Response via : Initial Calibration

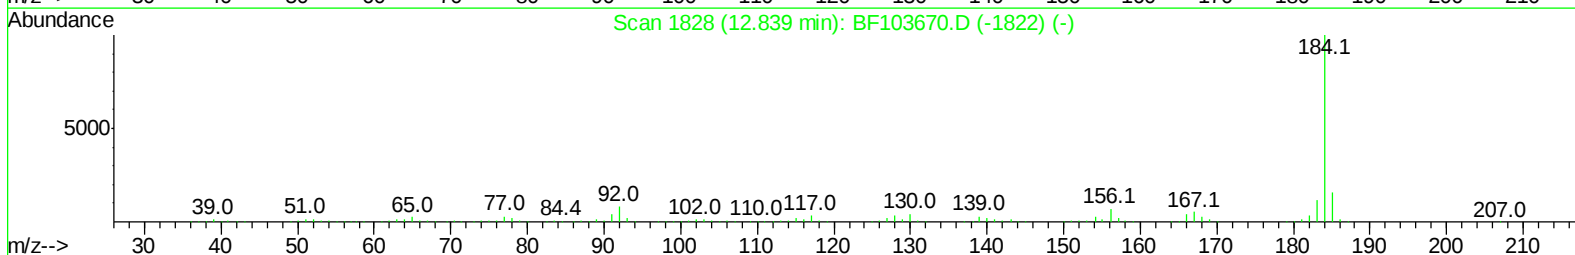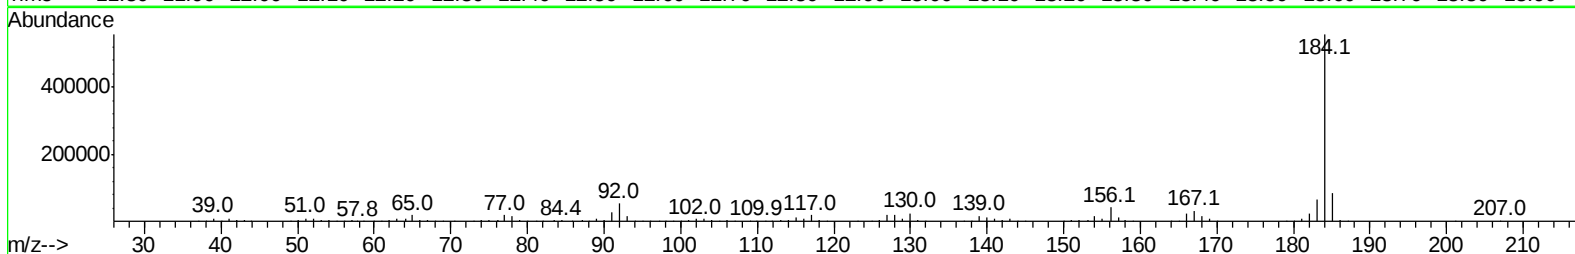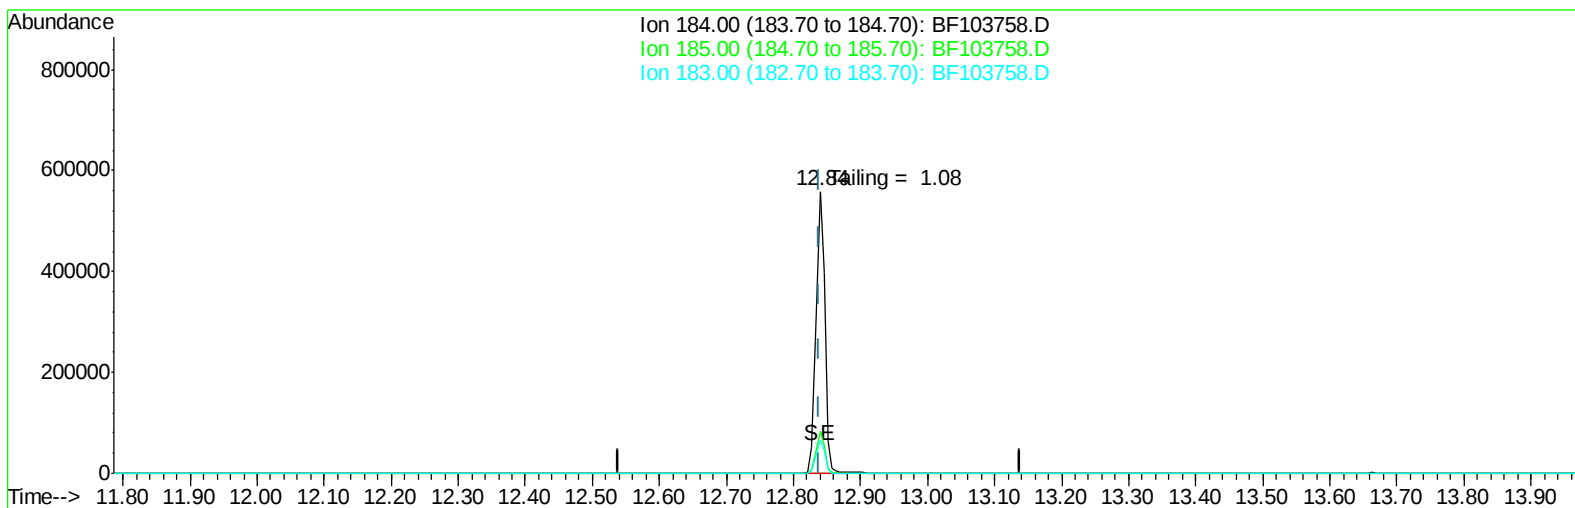

TIC: BF103758.D

(76) Benzidine

12.839min (+0.000) 0.00ng

response 484022

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.95
183.00	11.60	11.91
0.00	0.00	0.00