
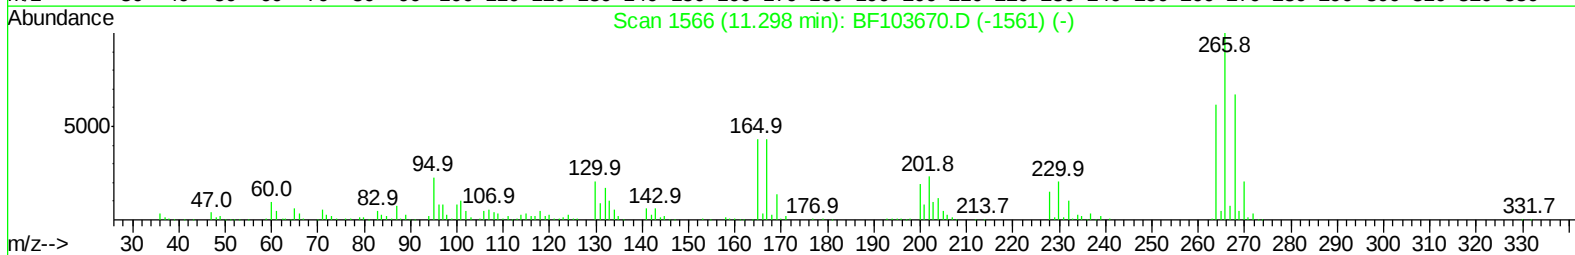
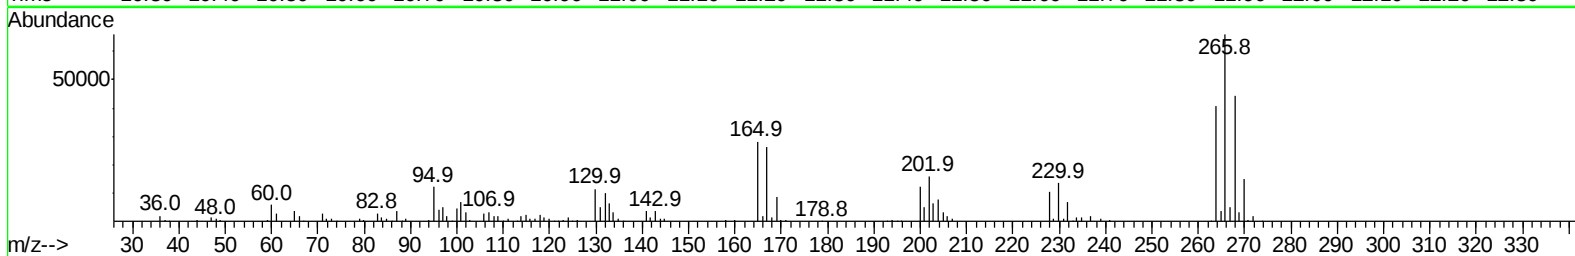


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF031918\
Data File : BF103784.D
Acq On : 20 Mar 2018 4:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 07:28:52 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

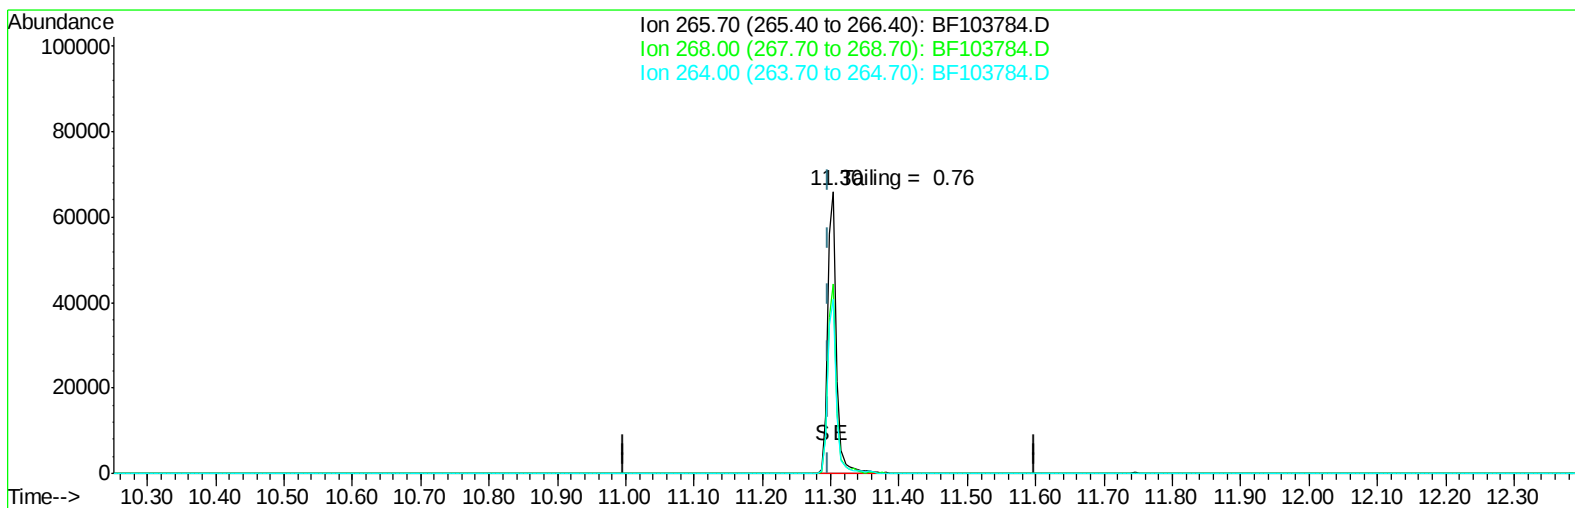

TIC: BF103784.D

(69) Pentachlorophenol (C)




11.304min (+0.006) 30407.59ng

response 60434

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.08
264.00	61.90	61.76
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF031918\
Data File : BF103784.D
Acq On : 20 Mar 2018 4:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 07:28:52 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

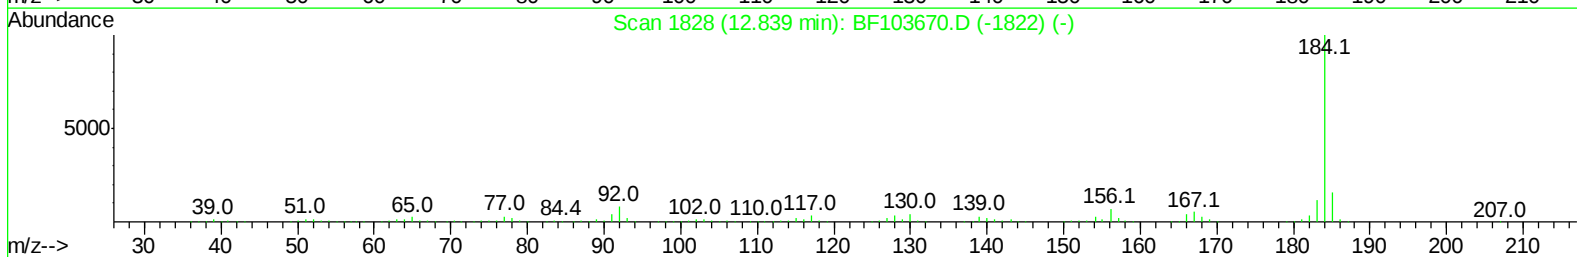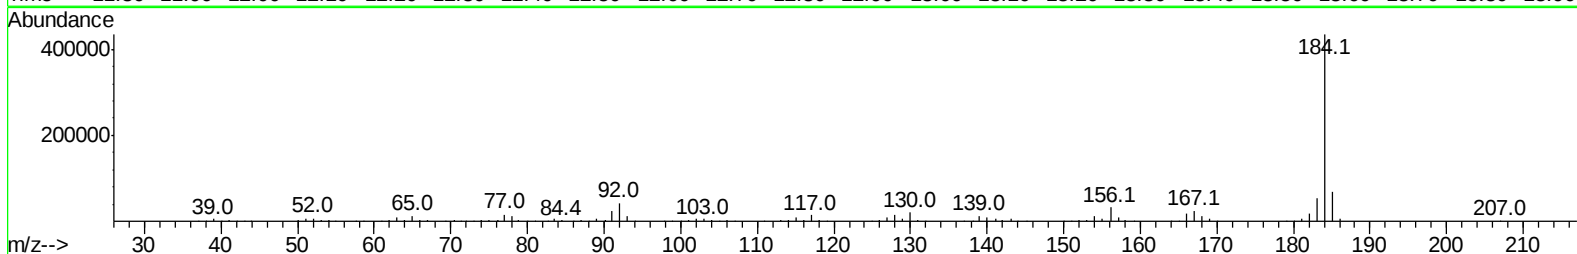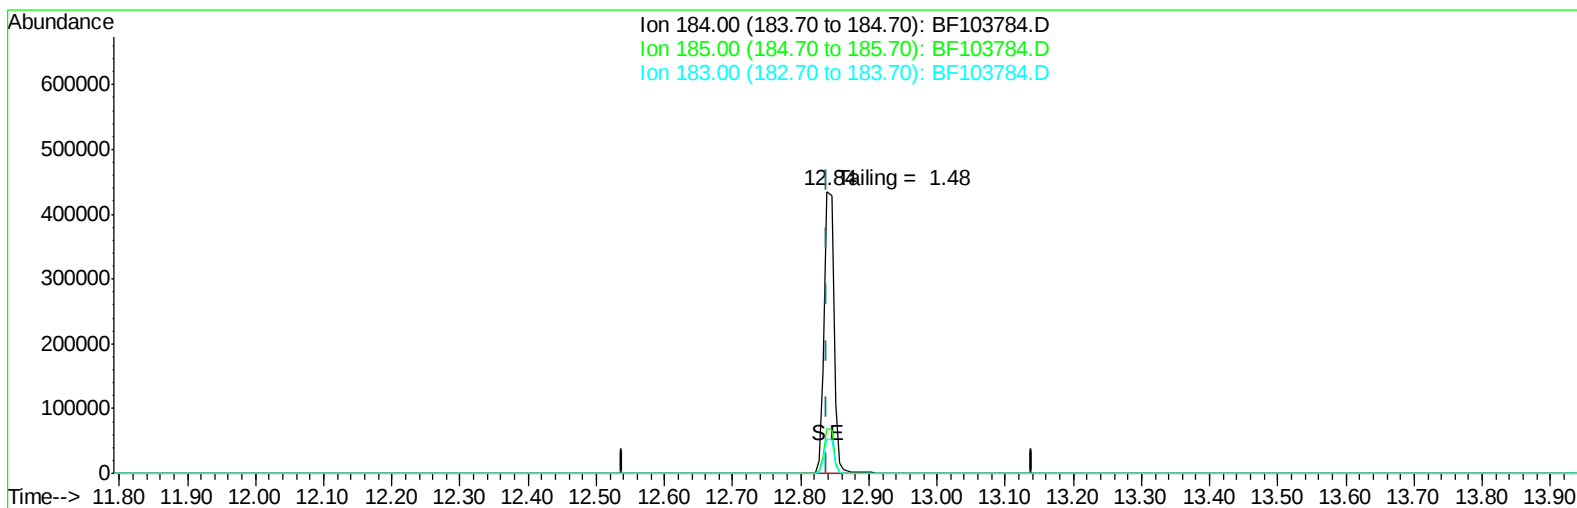

TIC: BF103784.D

(76) Benzidine

12.839min (-0.000) 0.00ng

response 419626

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.86
183.00	11.60	12.33
0.00	0.00	0.00