


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031918\
 Data File : BF103758.D
 Acq On : 19 Mar 2018 15:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 15 18:31:53 2018

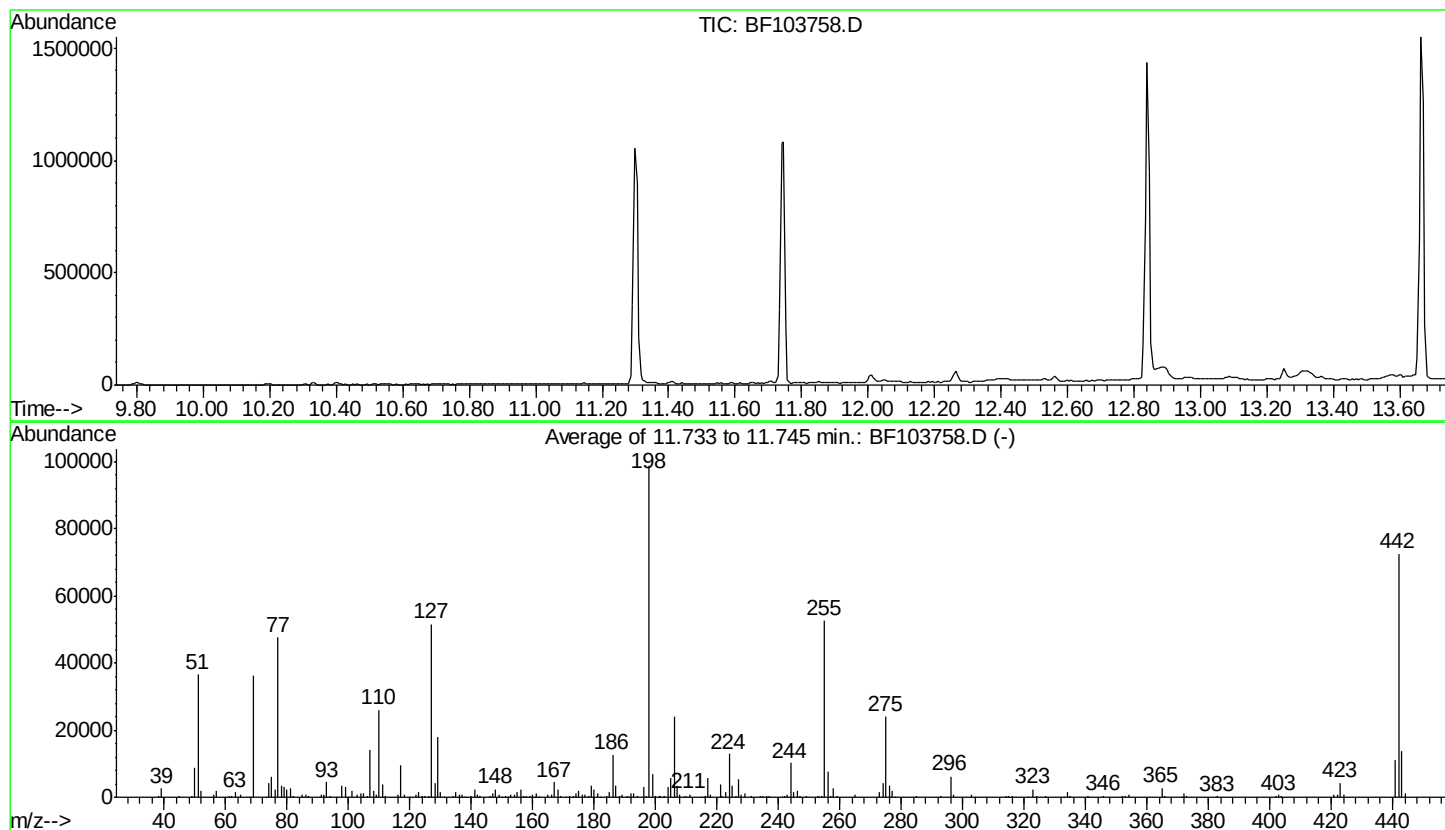

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	36541	PASS
68	69	0.00	2	0.4	159	PASS
69	198	0.00	100	36.5	36092	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	51557	PASS
197	198	0.00	2	0.6	574	PASS
198	198	100	100	100.0	98754	PASS
199	198	5	9	6.9	6790	PASS
275	198	10	60	24.2	23877	PASS
365	198	1	100	2.9	2840	PASS
441	443	0.01	100	80.7	10987	PASS
442	198	50	100	73.4	72457	PASS
443	442	15	24	18.8	13611	PASS