
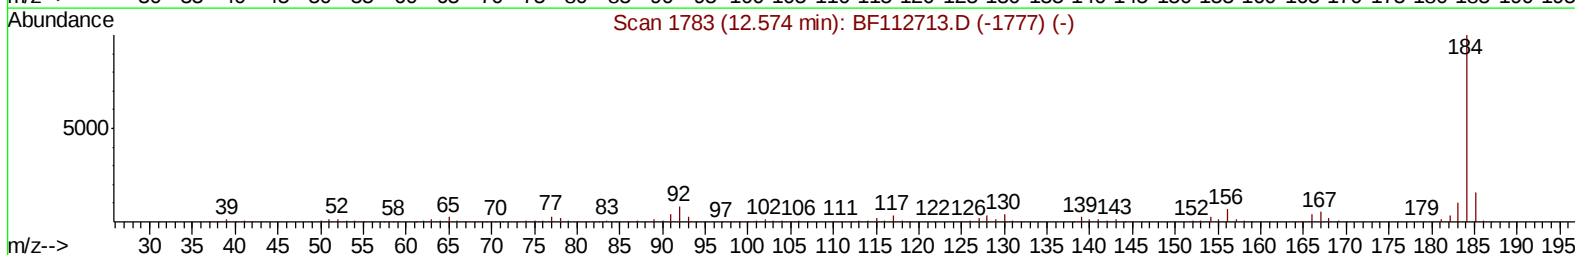
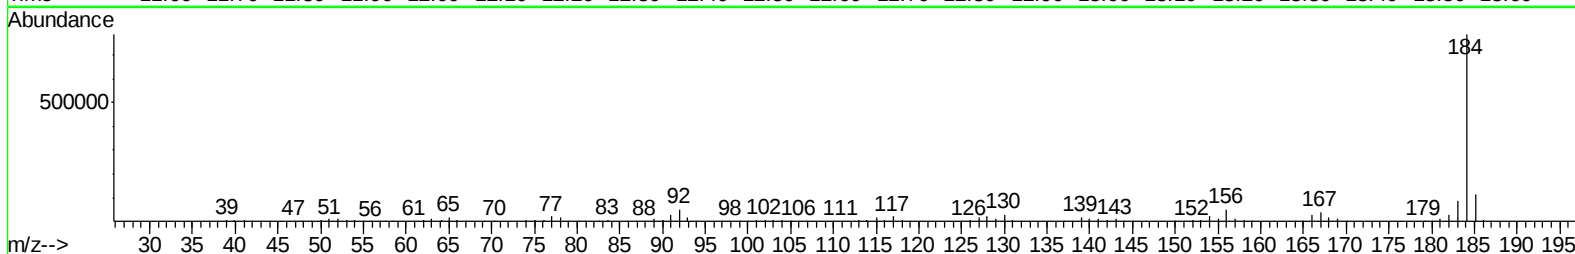


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
 Data File : BF113122.D
 Acq On : 19 Mar 2019 10:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 04:02:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 13 03:42:55 2019
 Response via : Initial Calibration

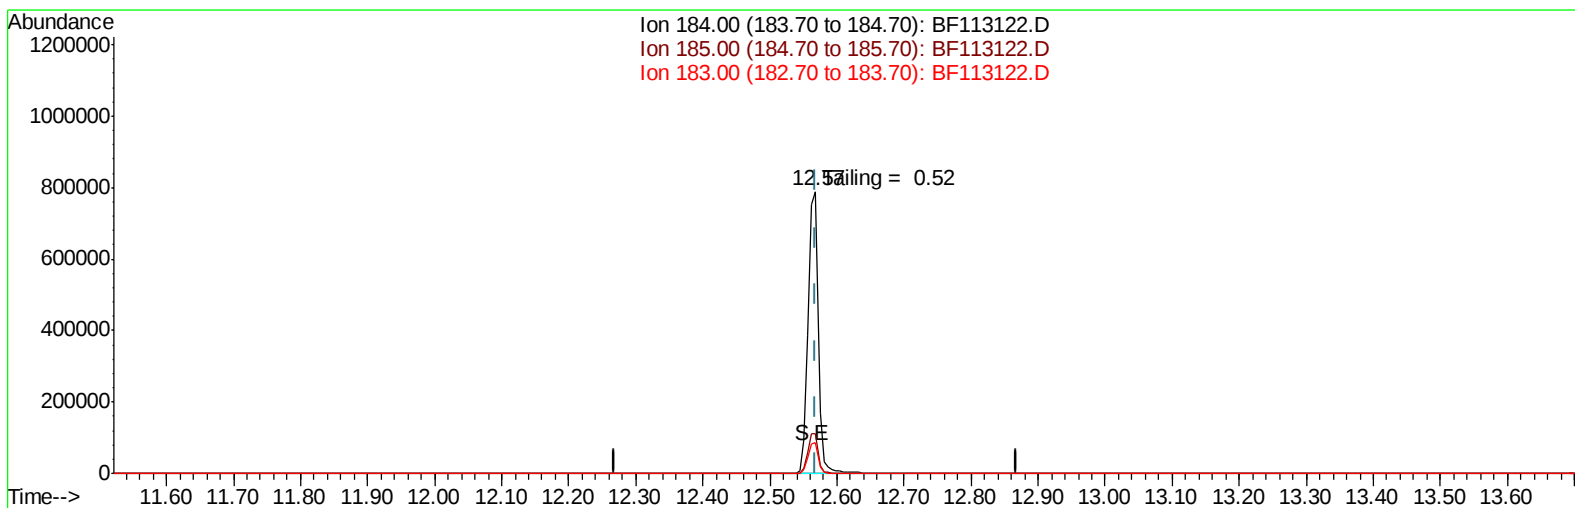

TIC: BF113122.D

(77) Benzidine




12.568min (-0.000) 14231.74ng

response 812204

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.21
183.00	10.70	10.72
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
Data File : BF113122.D
Acq On : 19 Mar 2019 10:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 04:02:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 13 03:42:55 2019
Response via : Initial Calibration

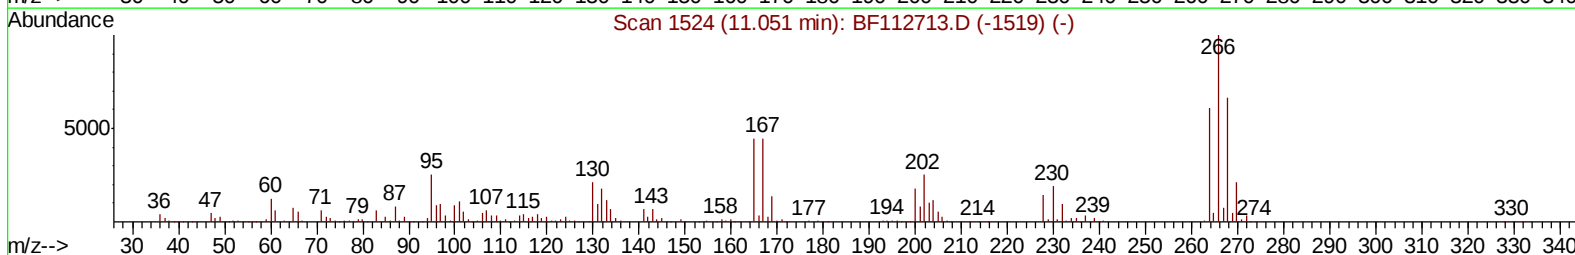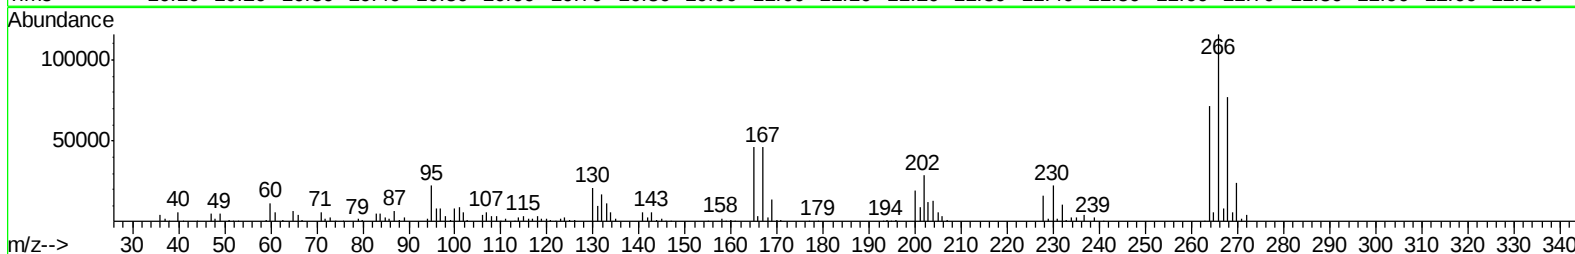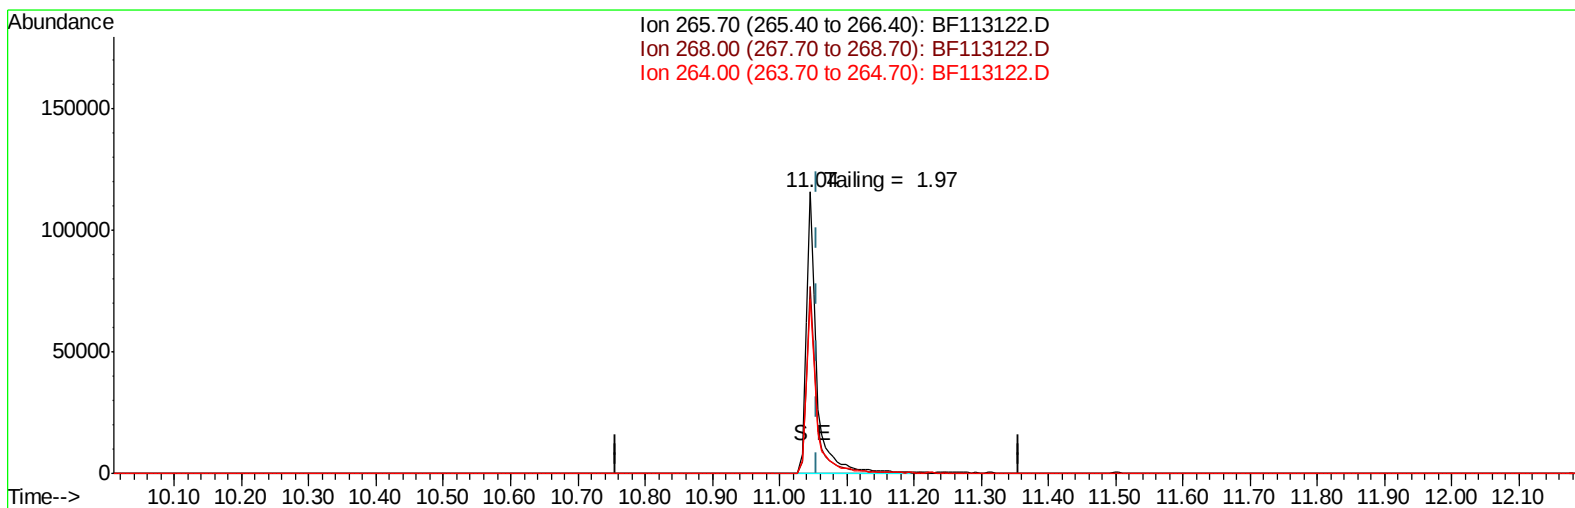

TIC: BF113122.D

(70) Pentachlorophenol (C)

11.045min (-0.012) 33225.98ng

response 126779

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.36
264.00	61.10	61.87
0.00	0.00	0.00