

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
 Data File : BF113140.D
 Acq On : 19 Mar 2019 22:05
 Operator : JU/SJ
 Sample : K1971-02 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-8(14-15)-031519

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.334	548	552	566	rVB	279319	291178	28.43%	3.482%
2	6.363	723	727	736	rBV	291441	316762	30.93%	3.788%
3	6.492	745	749	760	rBV	348638	309856	30.26%	3.705%
4	6.722	784	788	796	rBV	909122	761553	74.36%	9.107%
5	6.875	811	814	819	rBV	255412	223134	21.79%	2.668%
6	7.281	879	883	890	rBV	156423	159114	15.54%	1.903%
7	7.533	924	926	930	rVB2	21223	19740	1.93%	0.236%
8	8.004	1001	1006	1014	rBV	1109740	972659	94.98%	11.632%
9	8.080	1017	1019	1022	rVB	26236	21066	2.06%	0.252%
10	8.439	1076	1080	1082	rBV	30295	33184	3.24%	0.397%
11	8.604	1104	1108	1113	rBV5	14257	26896	2.63%	0.322%
12	8.698	1122	1124	1128	rVB3	22299	25802	2.52%	0.309%
13	8.922	1159	1162	1167	rVB2	15708	18732	1.83%	0.224%
14	9.039	1179	1182	1184	rBV2	20748	17434	1.70%	0.208%
15	9.080	1185	1189	1197	rVB	320921	311745	30.44%	3.728%
16	9.333	1227	1232	1234	rBV5	10600	16098	1.57%	0.193%
17	9.492	1253	1259	1261	rBV2	55684	67407	6.58%	0.806%
18	9.757	1299	1304	1311	rBV	1080960	1024084	100.00%	12.247%
19	9.922	1329	1332	1336	rBV3	10717	14652	1.43%	0.175%
20	10.027	1347	1350	1356	rVB4	20303	22630	2.21%	0.271%
21	10.416	1410	1416	1420	rBV	25111	31240	3.05%	0.374%
22	10.539	1433	1437	1442	rBV	167039	165602	16.17%	1.980%
23	10.680	1456	1461	1468	rBV2	25407	39550	3.86%	0.473%
24	11.145	1536	1540	1543	rVB2	23022	30831	3.01%	0.369%
25	11.192	1546	1548	1551	rVV4	14595	17202	1.68%	0.206%
26	11.233	1551	1555	1570	rVB	981224	928700	90.69%	11.106%
27	11.492	1596	1599	1603	rBV5	21256	30866	3.01%	0.369%
28	11.627	1620	1622	1626	rVB4	20089	18230	1.78%	0.218%
29	11.768	1643	1646	1649	rBV5	29136	45471	4.44%	0.544%
30	11.980	1680	1682	1684	rBV3	25716	25573	2.50%	0.306%
31	12.016	1685	1688	1693	rVB3	70842	83197	8.12%	0.995%
32	12.092	1699	1701	1705	rVB3	42750	35088	3.43%	0.420%
33	12.180	1713	1716	1719	rBV	79952	68355	6.67%	0.817%
34	12.445	1758	1761	1763	rBV3	36340	44264	4.32%	0.529%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
Data File : BF113140.D
Acq On : 19 Mar 2019 22:05
Operator : JU/SJ
Sample : K1971-02 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-8(14-15)-031519

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.810	1820	1823	1828	rBV	256314	257492	25.14%	3.079%
36	13.633	1961	1963	1966	rBV	71804	48407	4.73%	0.579%
37	13.668	1968	1969	1971	rBV2	77225	57378	5.60%	0.686%
38	13.827	1992	1996	1999	rBV5	147983	322066	31.45%	3.851%
39	13.862	1999	2002	2005	rVV	954313	935778	91.38%	11.191%
40	15.274	2239	2242	2246	rBV	476807	523189	51.09%	6.257%


Sum of corrected areas: 8362205

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
Data File : BF113140.D
Acq On : 19 Mar 2019 22:05
Operator : JU/SJ
Sample : K1971-02 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-8(14-15)-031519

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

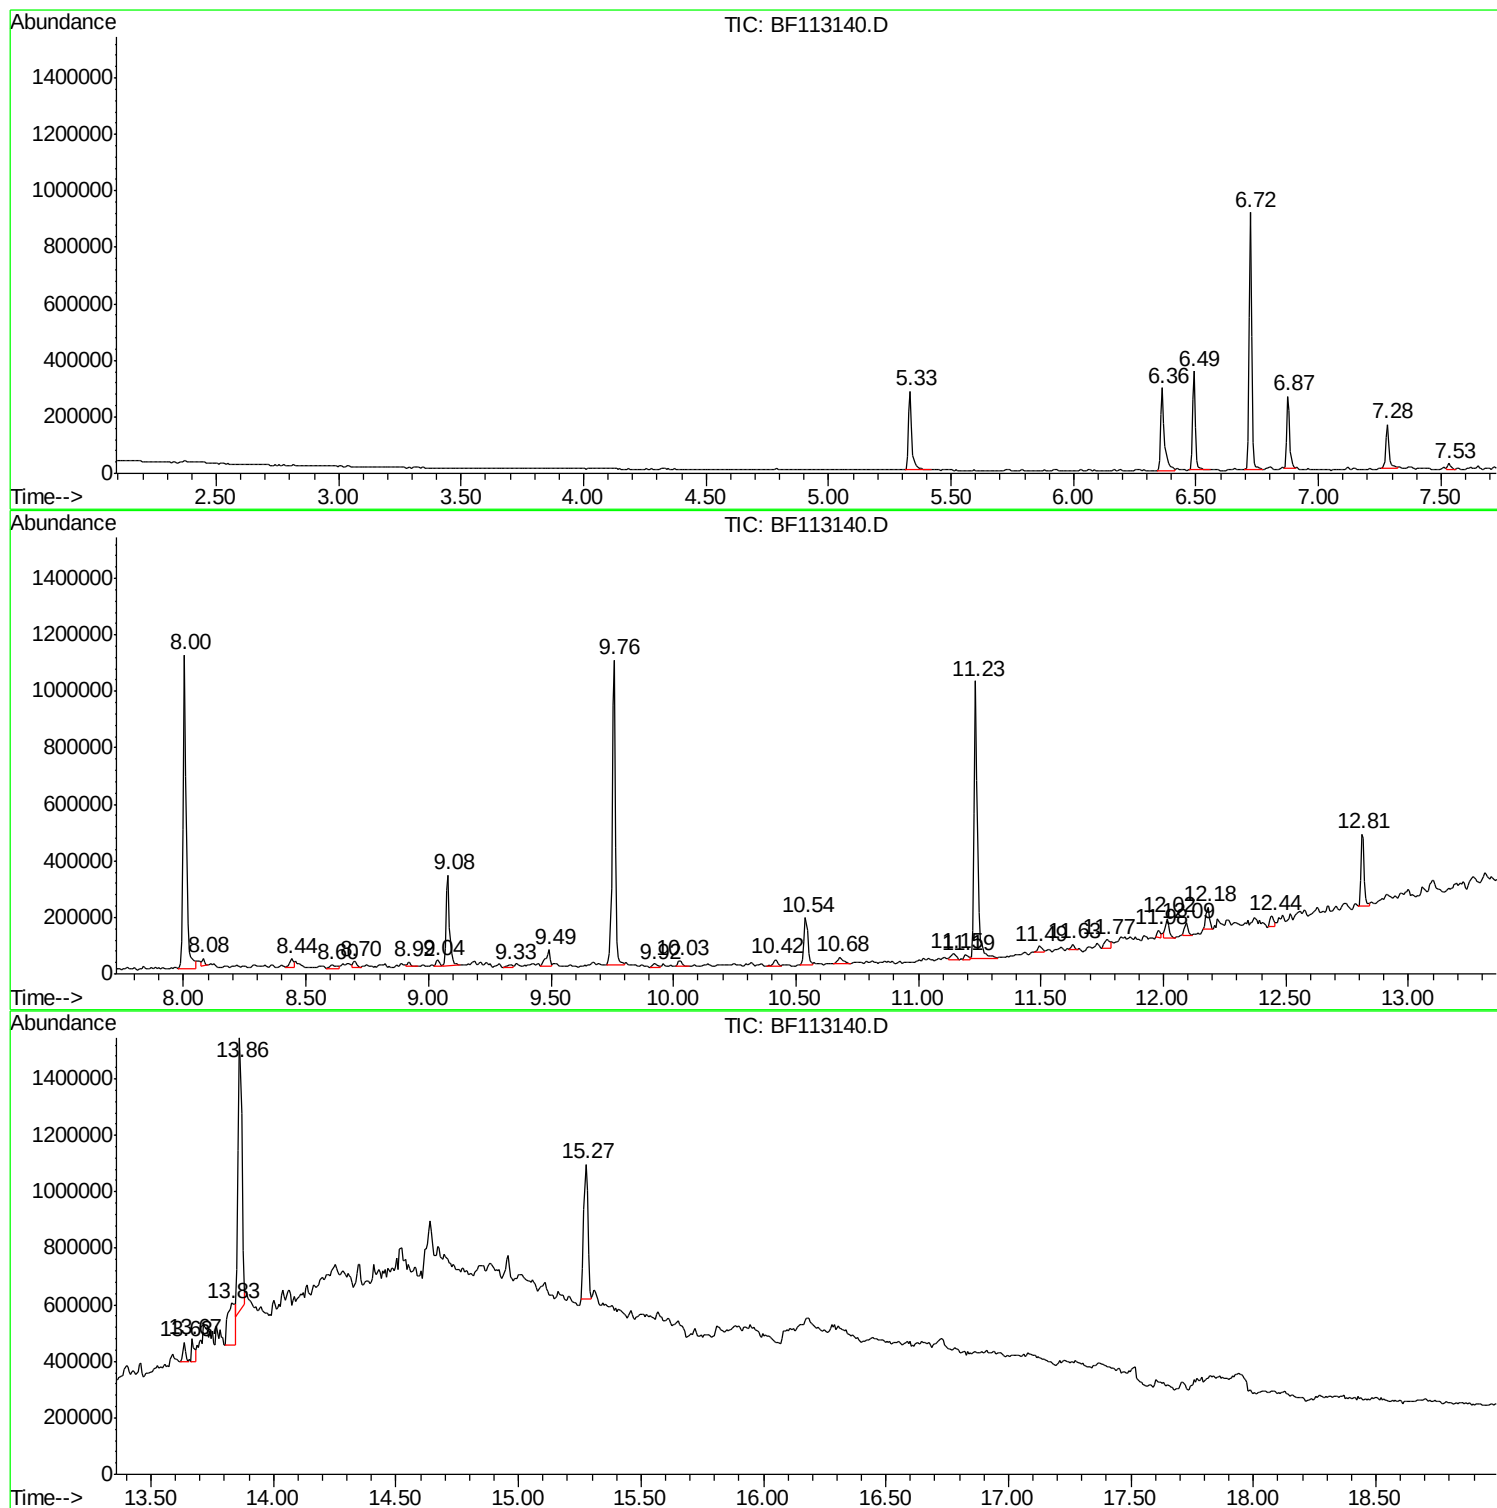

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
Data File : BF113140.D
Acq On : 19 Mar 2019 22:05
Operator : JU/SJ
Sample : K1971-02 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
SB-8(14-15)-031519

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.49 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
6.49	8.14 ng	309856	1,4-Dichlorobenzene-d4	6.72	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2	Tranlylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3	1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
4	Xenon	132	Xe	007440-63-3	9
5	2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

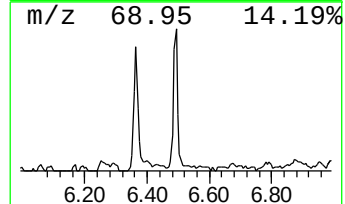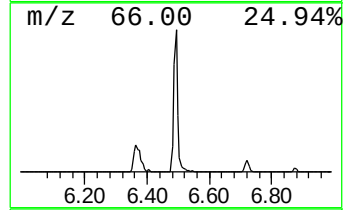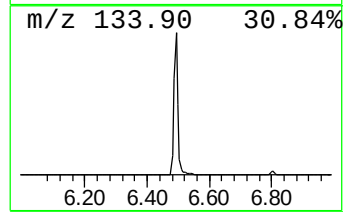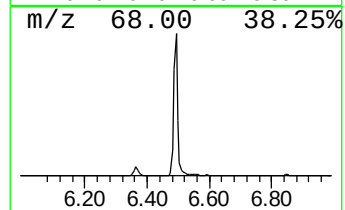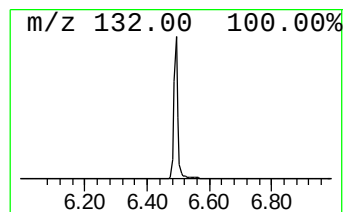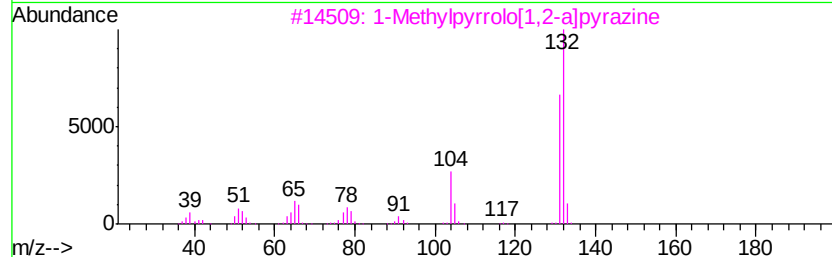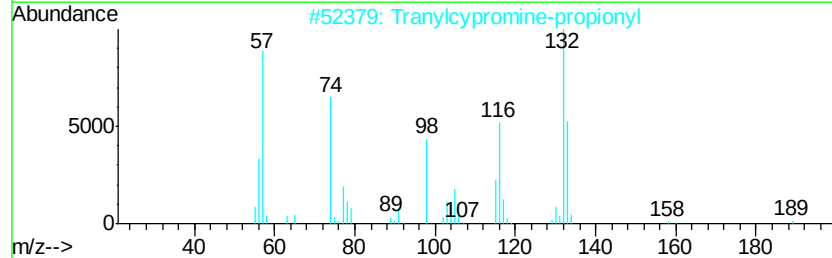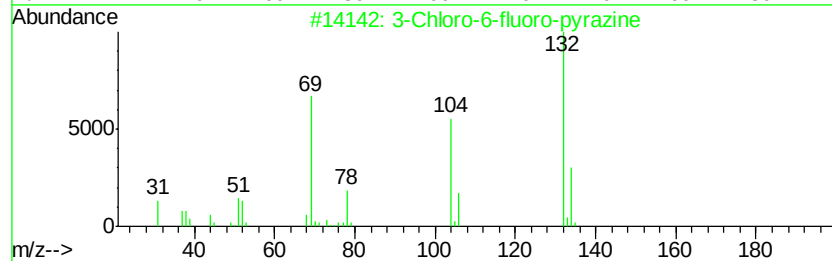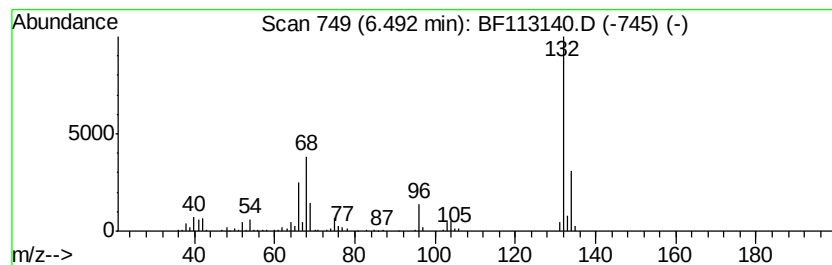

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
Data File : BF113140.D
Acq On : 19 Mar 2019 22:05
Operator : JU/SJ
Sample : K1971-02 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-8(14-15)-031519

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.49	6.49	8.1	ng	309856	1	6.72	761553	20.0