

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
 Data File : BF113141.D
 Acq On : 19 Mar 2019 22:34
 Operator : JU/SJ
 Sample : K1971-03 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-9(1-2)-031519

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.316	375	379	384	rVB3	8153	11434	1.16%	0.167%
2	5.334	548	552	564	rVB	199524	222410	22.61%	3.251%
3	5.634	598	603	611	rVB6	12338	19743	2.01%	0.289%
4	6.363	723	727	738	rBV	250279	260558	26.49%	3.809%
5	6.493	745	749	756	rBV	284922	257346	26.16%	3.762%
6	6.569	760	762	764	rVB	19063	13477	1.37%	0.197%
7	6.722	784	788	802	rBV	870421	733806	74.60%	10.727%
8	6.875	811	814	823	rBV	236005	209644	21.31%	3.065%
9	7.281	877	883	889	rBV	136959	151195	15.37%	2.210%
10	7.334	889	892	896	rVV	23542	24197	2.46%	0.354%
11	7.375	896	899	906	rVB4	7173	10835	1.10%	0.158%
12	8.004	1002	1006	1012	rBV	1047914	914384	92.96%	13.366%
13	8.610	1106	1109	1115	rVB3	14607	14843	1.51%	0.217%
14	9.081	1185	1189	1197	rBV	311393	302733	30.78%	4.425%
15	9.475	1252	1256	1261	rVB	17558	19658	2.00%	0.287%
16	9.757	1300	1304	1317	rVB	1058563	983593	100.00%	14.378%
17	10.198	1376	1379	1382	rVB3	9775	10677	1.09%	0.156%
18	10.539	1434	1437	1443	rBV	146270	143830	14.62%	2.102%
19	10.669	1456	1459	1464	rVB5	9991	10898	1.11%	0.159%
20	11.116	1530	1535	1538	rBV5	10363	11518	1.17%	0.168%
21	11.204	1544	1550	1551	rBV4	8860	12218	1.24%	0.179%
22	11.233	1551	1555	1563	rVV	964844	862503	87.69%	12.608%
23	11.769	1643	1646	1653	rBV3	40141	62826	6.39%	0.918%
24	12.557	1777	1780	1784	rBV5	16722	19542	1.99%	0.286%
25	12.816	1820	1824	1831	rBV	263076	256785	26.11%	3.754%
26	13.863	1998	2002	2009	rBV	814272	777412	79.04%	11.364%
27	15.274	2238	2242	2246	rBV	450347	522897	53.16%	7.644%


Sum of corrected areas: 6840962

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
Data File : BF113141.D
Acq On : 19 Mar 2019 22:34
Operator : JU/SJ
Sample : K1971-03 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-9(1-2)-031519

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

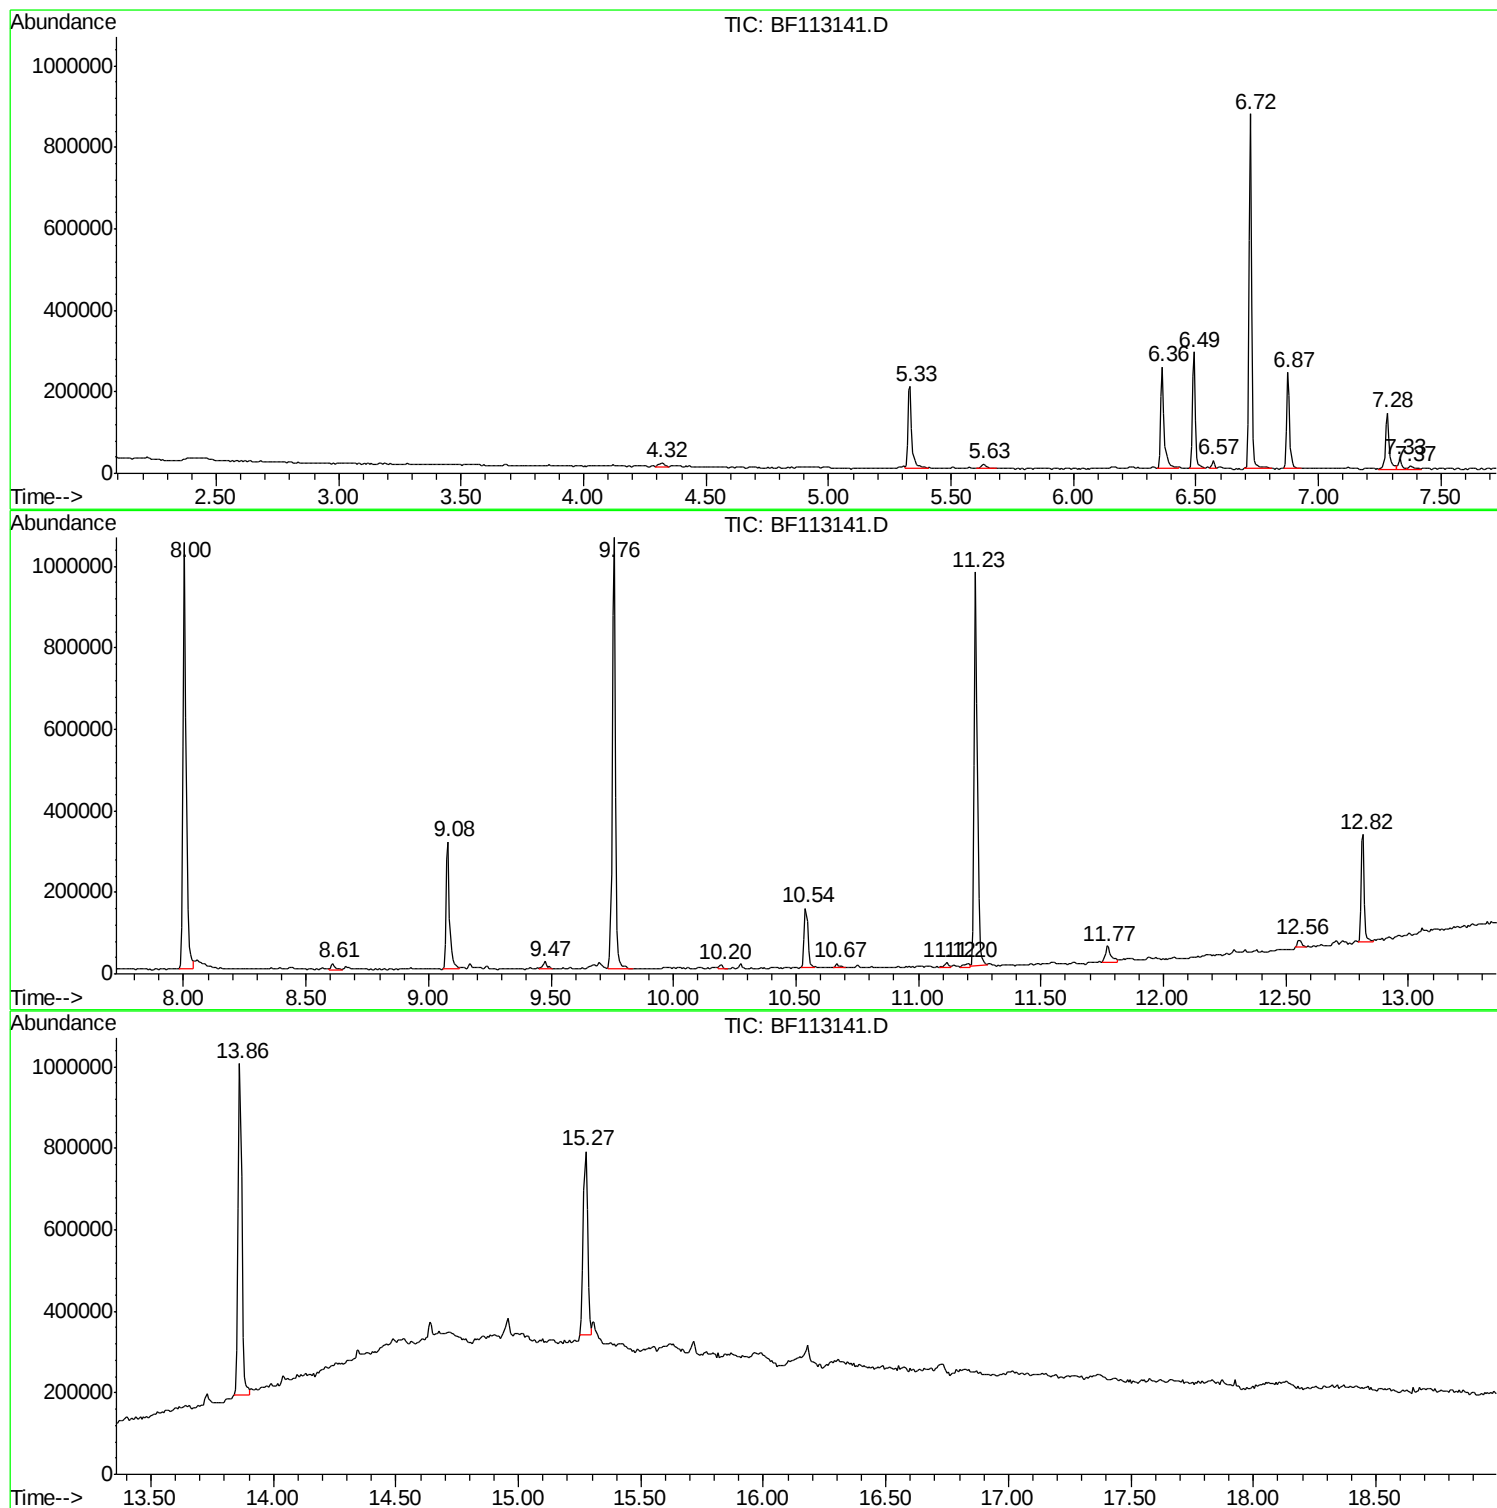

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
Data File : BF113141.D
Acq On : 19 Mar 2019 22:34
Operator : JU/SJ
Sample : K1971-03 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-9(1-2)-031519










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.49 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.49	7.01 ng	257346	1,4-Dichlorobenzene-d4	6.72

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	37
2			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4			5-Aminoindole	132	C8H8N2	005192-03-0	12
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

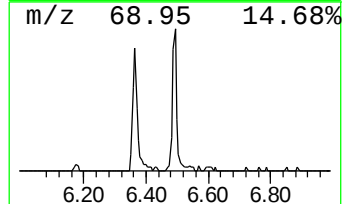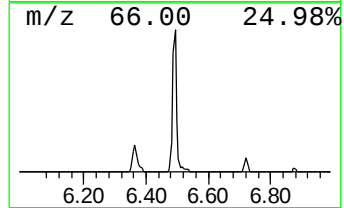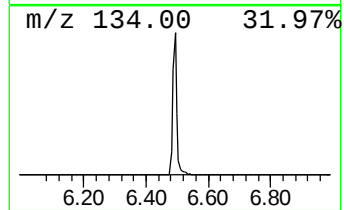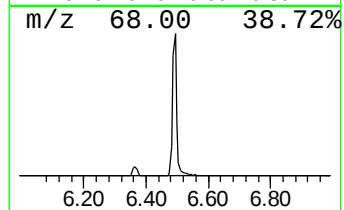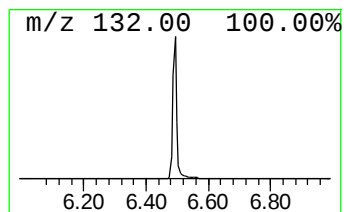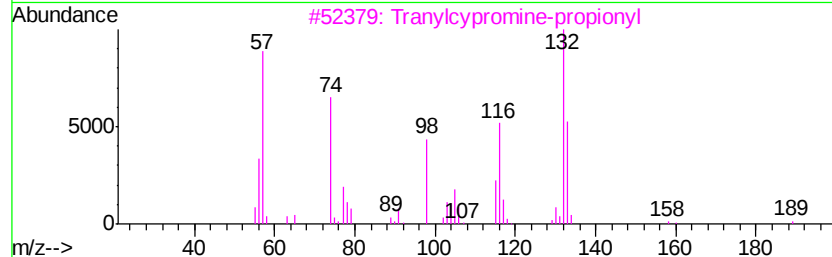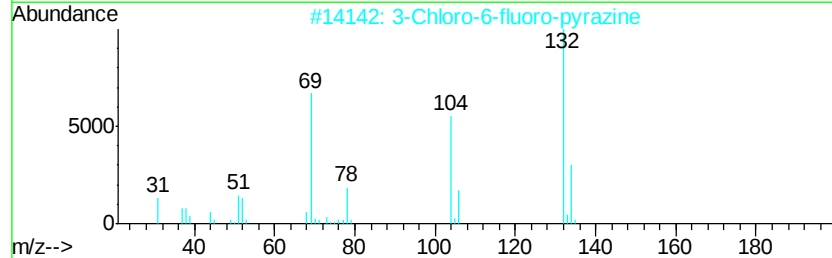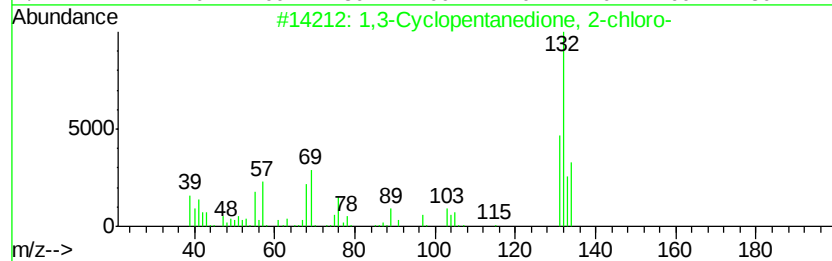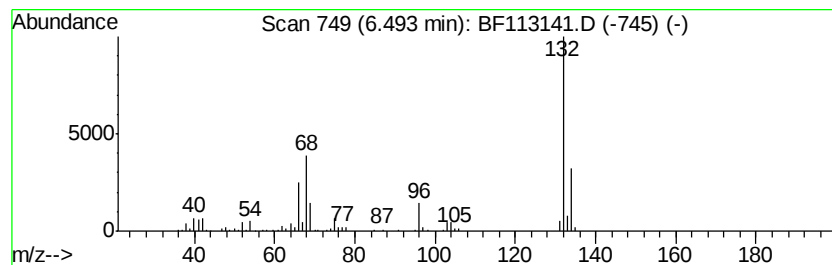

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
Data File : BF113141.D
Acq On : 19 Mar 2019 22:34
Operator : JU/SJ
Sample : K1971-03 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-9(1-2)-031519

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.49	6.49	7.0	ng	257346	1	6.72	733806	20.0