


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031919\
 Data File : BF113144.D
 Acq On : 20 Mar 2019 00:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 13 03:42:55 2019

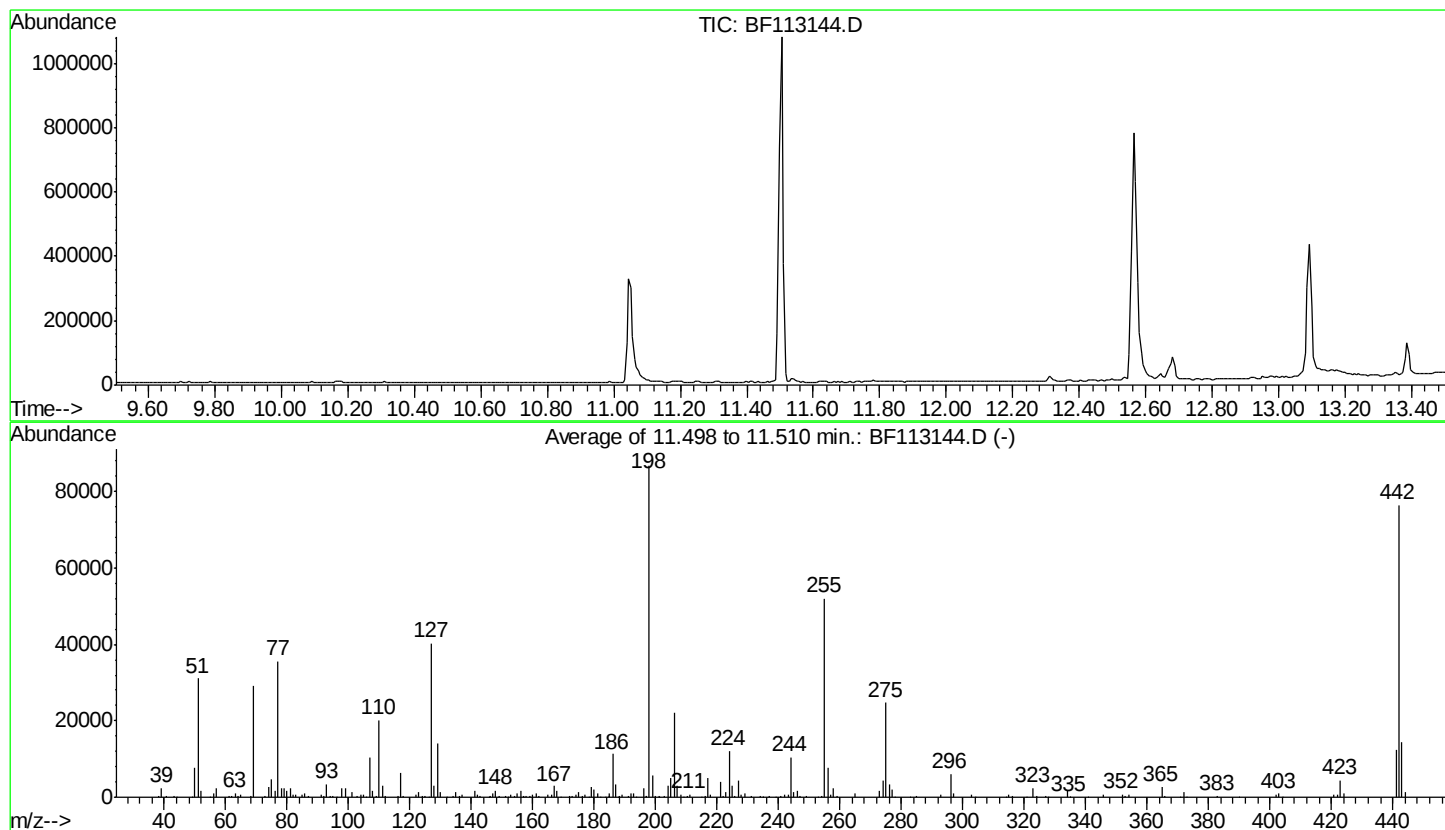

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	31170	PASS
68	69	0.00	2	1.7	504	PASS
69	198	0.00	100	33.6	29171	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.4	40287	PASS
197	198	0.00	2	0.3	287	PASS
198	198	100	100	100.0	86826	PASS
199	198	5	9	6.7	5777	PASS
275	198	10	60	28.6	24789	PASS
365	198	1	100	3.2	2808	PASS
441	198	0.01	100	14.1	12281	PASS
442	198	50	100	88.0	76424	PASS
443	442	15	24	18.7	14319	PASS