

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031920\
 Data File : BF119450.D
 Acq On : 19 Mar 2020 20:55
 Operator : CG/JU
 Sample : L1954-06MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-11AMS

Quant Time: Mar 20 03:50:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 18 15:11:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	340182	20.00	ng	0.00
21) Naphthalene-d8	8.14	136	1295579	20.00	ng	0.00
39) Acenaphthene-d10	9.90	164	652485	20.00	ng	0.00
64) Phenanthrene-d10	11.39	188	1187713	20.00	ng	0.00
76) Chrysene-d12	14.03	240	593344	20.00	ng	0.00
87) Perylene-d12	15.49	264	689104	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	2219753	103.87	ng	0.01
7) Phenol-d6	6.47	99	2919336	106.94	ng	0.00
23) Nitrobenzene-d5	7.42	82	1767352	74.14	ng	0.00
42) 2,4,6-Tribromophenol	10.69	330	729832	108.42	ng	0.00
45) 2-Fluorobiphenyl	9.22	172	3145374	71.42	ng	0.00
79) Terphenyl-d14	12.97	244	2822051	93.18	ng	0.00

Target Compounds					Qvalue
2) 1,4-Dioxane	2.68	88	386734	36.64 ng	99
3) Pyridine	3.42	79	963064	33.12 ng	99
4) n-Nitrosodimethylamine	3.37	42	575464	40.58 ng	96
6) Aniline	6.51	93	576543	15.30 ng	98
8) 2-Chlorophenol	6.63	128	1049205	46.75 ng	99
9) Benzaldehyde	6.40	77	670900	38.74 ng	99
10) Phenol	6.49	94	1346295	46.22 ng	95
11) bis(2-Chloroethyl)ether	6.59	93	1001334	42.98 ng	99
12) 1,3-Dichlorobenzene	6.79	146	1049383	43.20 ng	99
13) 1,4-Dichlorobenzene	6.87	146	1055562	43.44 ng	99
14) 1,2-Dichlorobenzene	7.02	146	984935	43.37 ng	99
15) Benzyl Alcohol	6.99	79	900926	43.87 ng	96
16) 2,2'-oxybis(1-Chloropropan	7.13	45	1892650	40.28 ng	98
17) 2-Methylphenol	7.10	107	856831	41.67 ng	99
18) Hexachloroethane	7.37	117	400745	45.01 ng	95
19) n-Nitroso-di-n-propylamine	7.27	70	708387	43.05 ng	99
20) 3+4-Methylphenols	7.25	107	1021685	40.54 ng	88
22) Acetophenone	7.26	105	1344237	43.42 ng	99
24) Nitrobenzene	7.43	77	1055670	41.44 ng	98
25) Isophorone	7.67	82	1995089	41.26 ng	99
26) 2-Nitrophenol	7.75	139	516922	51.53 ng	97
27) 2,4-Dimethylphenol	7.79	122	956850	46.13 ng	99
28) bis(2-Chloroethoxy)methane	7.89	93	1248103	43.65 ng	99
29) 2,4-Dichlorophenol	7.99	162	832494	43.68 ng	97
30) 1,2,4-Trichlorobenzene	8.08	180	905348	42.96 ng	100
31) Naphthalene	8.16	128	2856081	42.84 ng	99
32) Benzoic acid	7.91	122	616793	46.23 ng	98
33) 4-Chloroaniline	8.20	127	198386	6.49 ng	96
34) Hexachlorobutadiene	8.28	225	507410	43.03 ng	100
35) Caprolactam	8.58	113	170362	27.31 ng	98
36) 4-Chloro-3-methylphenol	8.69	107	889783	42.72 ng	99
37) 2-Methylnaphthalene	8.85	142	1916009	43.79 ng	100
38) 1-Methylnaphthalene	8.95	142	1803301	43.54 ng	100
40) 1,2,4,5-Tetrachlorobenzene	9.02	216	808761	42.29 ng	99

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031920\
 Data File : BF119450.D
 Acq On : 19 Mar 2020 20:55
 Operator : CG/JU
 Sample : L1954-06MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-11AMS

Quant Time: Mar 20 03:50:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 18 15:11:18 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Hexachlorocyclopentadiene	9.01	237	879069	80.85	ng	98
43) 2,4,6-Trichlorophenol	9.13	196	622609	45.49	ng	99
44) 2,4,5-Trichlorophenol	9.16	196	613763	40.03	ng	96
46) 1,1'-Biphenyl	9.32	154	2215832	41.70	ng	100
47) 2-Chloronaphthalene	9.35	162	1745374	41.93	ng	97
48) 2-Nitroaniline	9.43	65	618817	43.07	ng	98
49) Acenaphthylene	9.76	152	2760777	42.23	ng	100
50) Dimethylphthalate	9.62	163	2180797	47.05	ng	99
51) 2,6-Dinitrotoluene	9.68	165	444755	44.77	ng	# 85
52) Acenaphthene	9.93	154	1798753	44.14	ng	99
53) 3-Nitroaniline	9.84	138	171145	13.65	ng	99
54) 2,4-Dinitrophenol	9.95	184	310966	73.04	ng	91
55) Dibenzofuran	10.10	168	2468098	42.24	ng	99
56) 4-Nitrophenol	10.00	139	773192	78.15	ng	91
57) 2,4-Dinitrotoluene	10.08	165	586076	46.83	ng	88
58) Fluorene	10.45	166	1825820	42.26	ng	98
59) 2,3,4,6-Tetrachlorophenol	10.22	232	509886	44.49	ng	99
60) Diethylphthalate	10.32	149	1997908	42.47	ng	99
61) 4-Chlorophenyl-phenylether	10.44	204	881769	41.73	ng	98
62) 4-Nitroaniline	10.46	138	418606	34.81	ng	98
63) Azobenzene	10.60	77	1961663	41.41	ng	99
65) 4,6-Dinitro-2-methylphenol	10.49	198	230192	46.22	ng	89
66) n-Nitrosodiphenylamine	10.56	169	1709146	43.83	ng	98
67) 4-Bromophenyl-phenylether	10.93	248	568275	42.01	ng	# 91
68) Hexachlorobenzene	11.00	284	607706	43.90	ng	# 91
69) Atrazine	11.09	200	482968	45.18	ng	99
70) Pentachlorophenol	11.19	266	642274	79.12	ng	99
71) Phenanthrene	11.41	178	2635702	42.80	ng	99
72) Anthracene	11.46	178	2667469	42.62	ng	99
73) Carbazole	11.62	167	2394117	38.64	ng	99
74) Di-n-butylphthalate	11.95	149	2918294	44.03	ng	98
75) Fluoranthene	12.60	202	2682341	40.24	ng	99
77) Benzidine	12.72	184	859678	34.24	ng	98
78) Pyrene	12.83	202	2592307	53.24	ng	99
80) Butylbenzylphthalate	13.45	149	1042714	52.94	ng	98
81) Benzo(a)anthracene	14.02	228	1814873	47.04	ng	99
82) 3,3'-Dichlorobenzidine	13.98	252	375985	24.71	ng	95
83) Chrysene	14.06	228	1839735	46.20	ng	99
84) Bis(2-ethylhexyl)phthalate	14.02	149	1230347	52.40	ng	99
85) Di-n-octyl phthalate	14.63	149	2052776	49.71	ng	100
86) Indeno(1,2,3-cd)pyrene	16.97	276	2232287	59.52	ng	99
88) Benzo(b)fluoranthene	15.07	252	1876694	40.77	ng	100
89) Benzo(k)fluoranthene	15.10	252	1771648	40.42	ng	99
90) Benzo(a)pyrene	15.43	252	1743858	41.69	ng	99
91) Dibenzo(a,h)anthracene	16.99	278	1818035	49.69	ng	99
92) Benzo(g,h,i)perylene	17.42	276	1921379	52.27	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031920\
Data File : BF119450.D
Acq On : 19 Mar 2020 20:55
Operator : CG/JU
Sample : L1954-06MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-11AMS

Quant Time: Mar 20 03:50:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 18 15:11:18 2020
Response via : Initial Calibration

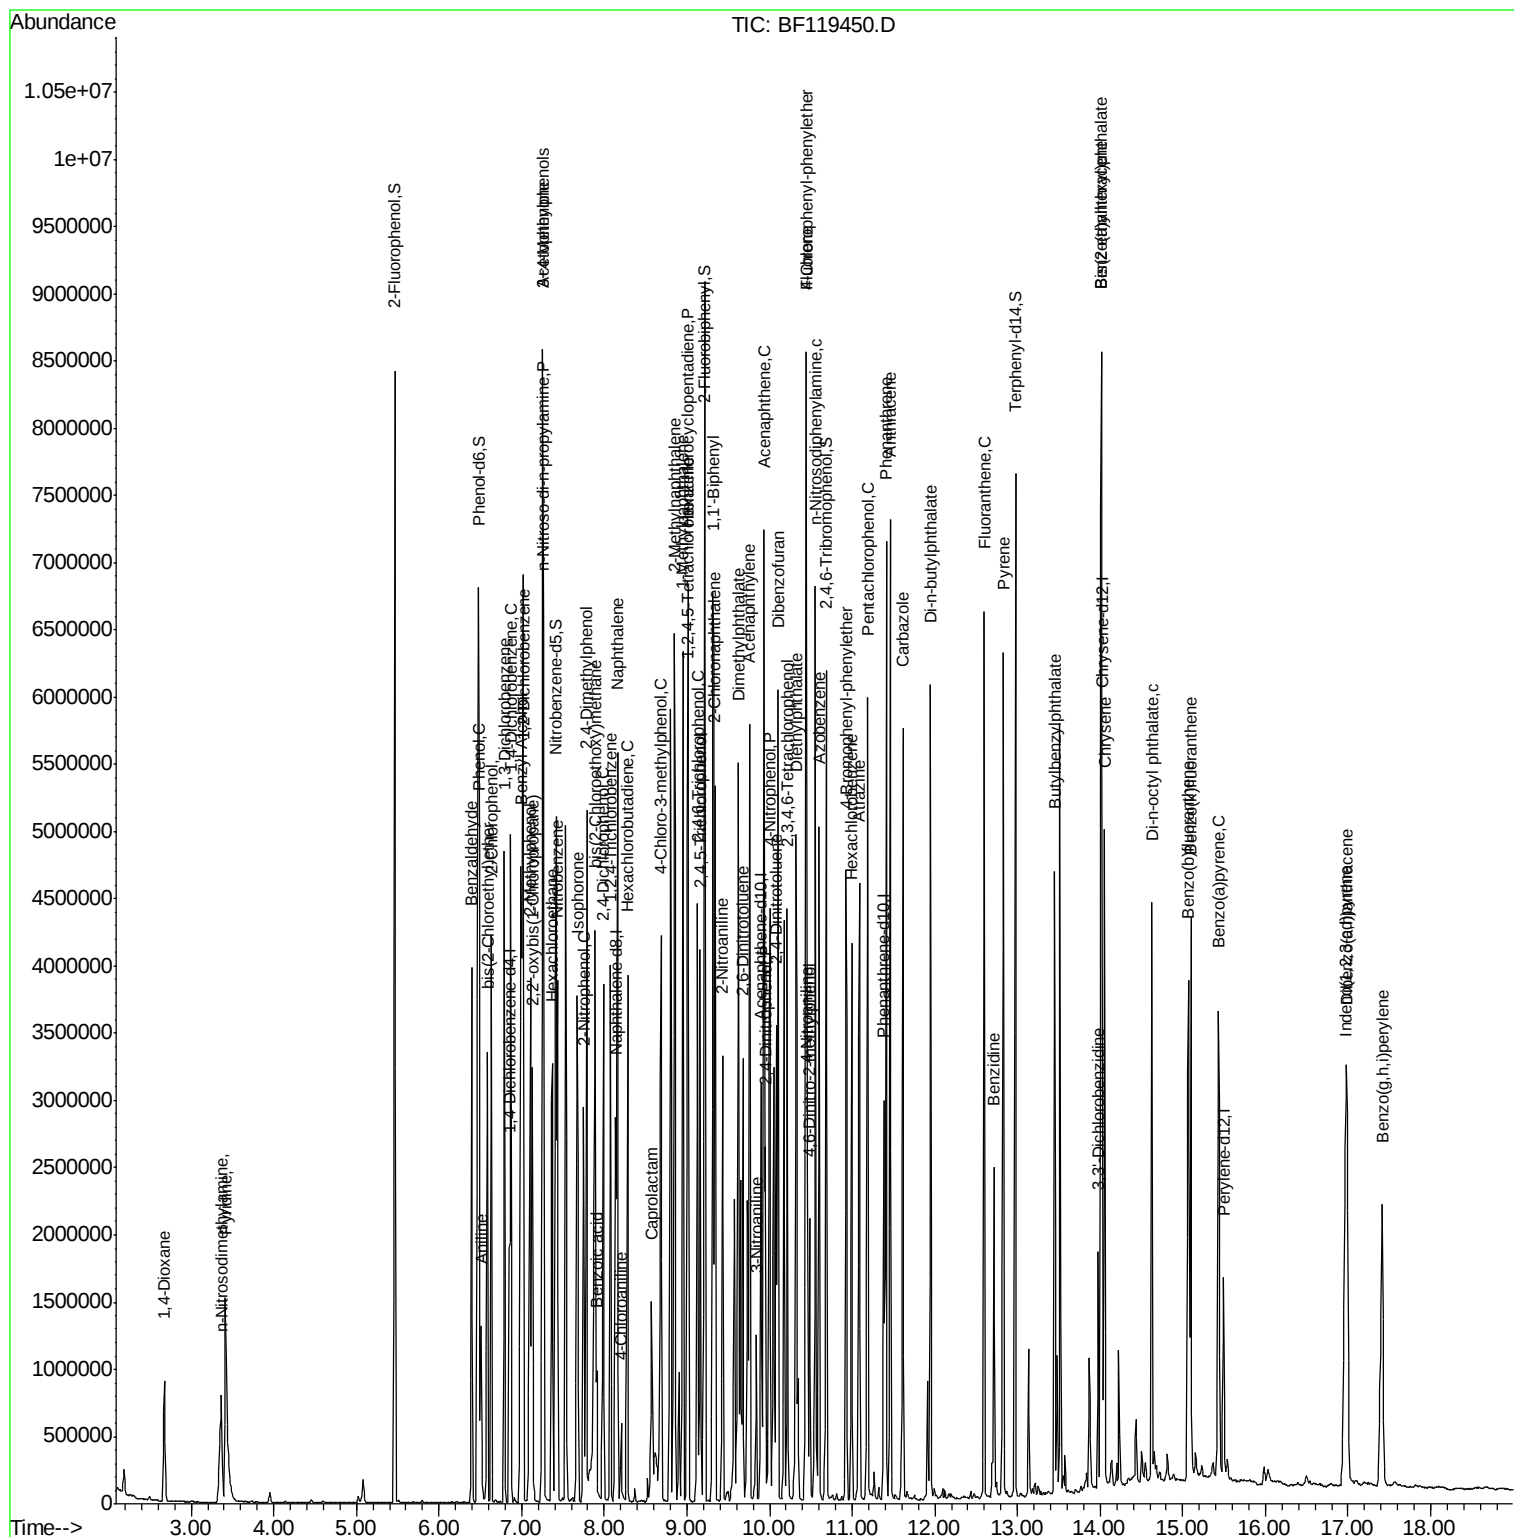

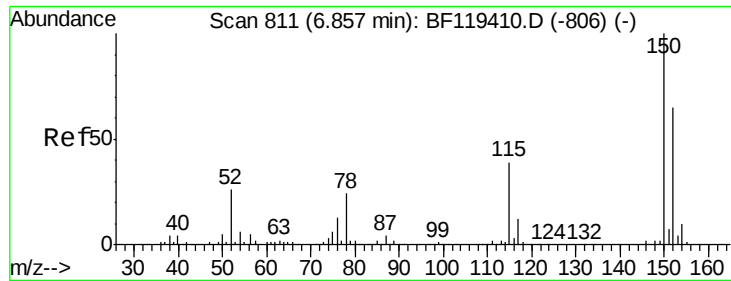

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.85 min Scan# 810

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion:152 Resp: 340182

Ion Ratio Lower Upper

152 100

150 155.2 123.9 185.9




115 58.0 47.8 71.6



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

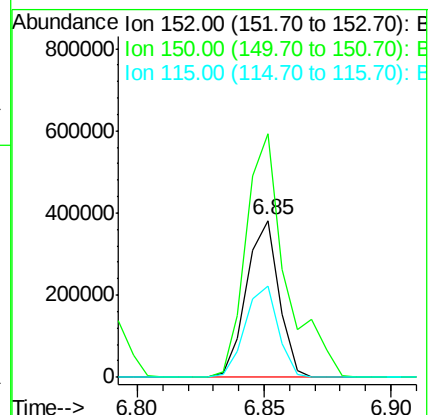

#2

1,4-Dioxane

Concen: 36.64 ng

RT: 2.68 min Scan# 100

Delta R.T. 0.07 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion: 88 Resp: 386734

Ion Ratio Lower Upper

88 100

58 100.1 79.4 119.2



43 35.1 28.4 42.6




Abundance Ion 88.00 (87.70 to 88.70): BF1

Ion 58.00 (57.70 to 58.70): BF1

Ion 43.00 (42.70 to 43.70): BF1

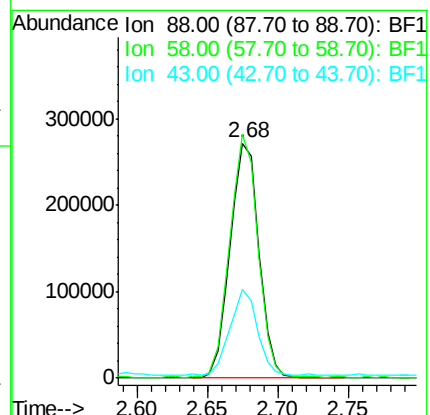



#3

Pyridine

Concen: 33.12 ng

RT: 3.42 min Scan# 226

Delta R.T. 0.06 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS





Tgt Ion: 79 Resp: 963064

Ion Ratio Lower Upper

79 100

52 99.1 80.0 120.0

51 45.7 37.9 56.9

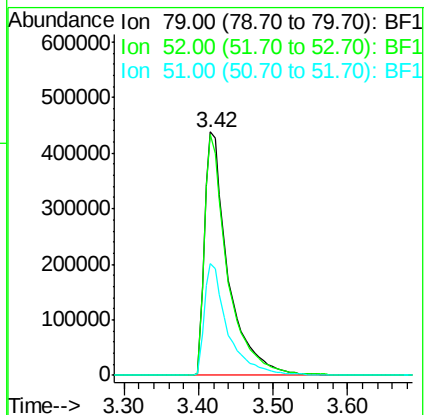

#4

n-Nitrosodimethylamine

Concen: 40.58 ng

RT: 3.37 min Scan# 218

Delta R.T. 0.07 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55




Tgt Ion: 42 Resp: 575464


Ion Ratio Lower Upper

42 100

74 118.1 91.3 136.9

44 7.9 7.1 10.7

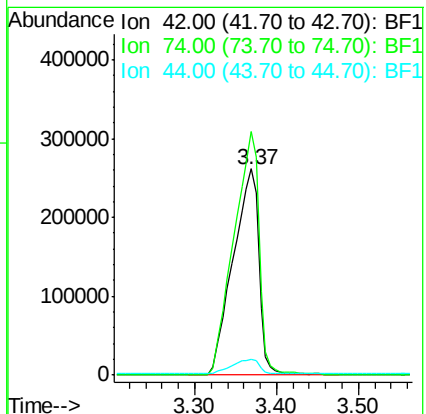



#5

2-Fluorophenol

Concen: 103.87 ng

RT: 5.47 min Scan# 575

Delta R.T. 0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion: 112 Resp: 2219753

Ion Ratio Lower Upper

112 100

64 71.6 58.1 87.1




63 37.0 29.7 44.5



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

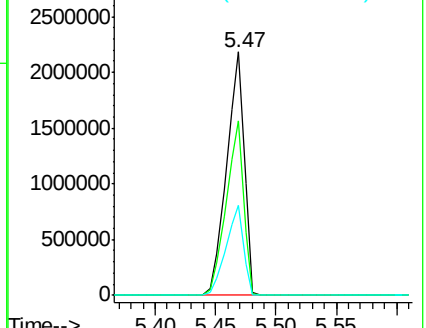

#6

Aniline

Concen: 15.30 ng

RT: 6.51 min Scan# 752

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion: 93 Resp: 576543

Ion Ratio Lower Upper

93 100

66 41.3 34.2 51.4



65 21.9 18.2 27.4




Abundance Ion 93.00 (92.70 to 93.70): BF1

Ion 66.00 (65.70 to 66.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

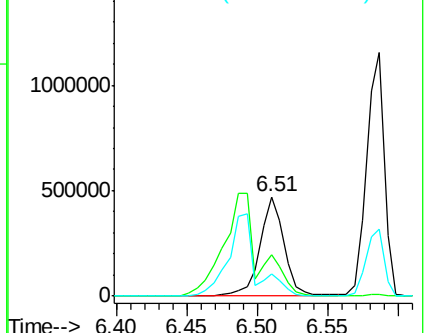

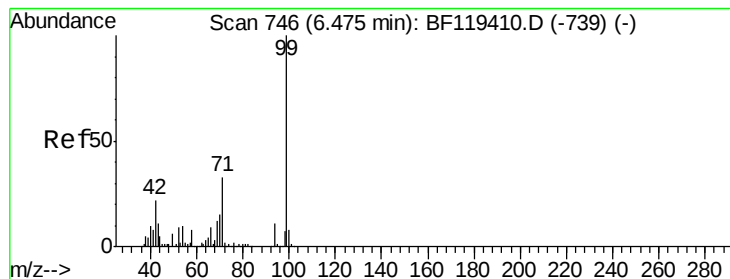

#7

Phenol-d6

Concen: 106.94 ng

RT: 6.47 min Scan# 746

Delta R.T. 0.00 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion: 99 Resp: 2919336

Ion Ratio Lower Upper

99 100

42 21.1 17.8 26.6




71 33.4 26.0 39.0



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

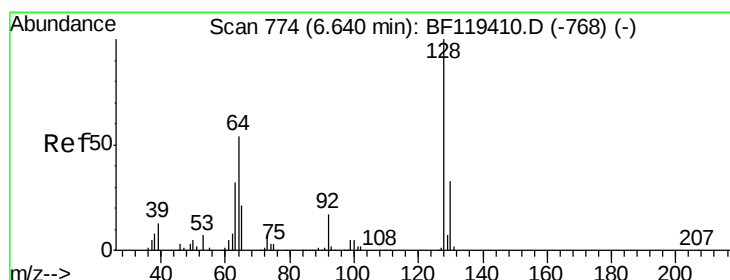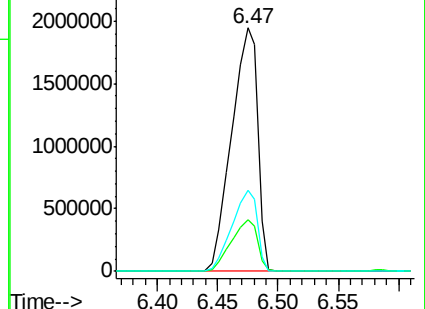

#8

2-Chlorophenol

Concen: 46.75 ng

RT: 6.63 min Scan# 773

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion: 128 Resp: 1049205

Ion Ratio Lower Upper

128 100

130 33.7 13.0 53.0



64 55.1 35.1 75.1




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 130.00 (129.70 to 130.70): E

Ion 64.00 (63.70 to 64.70): BF1

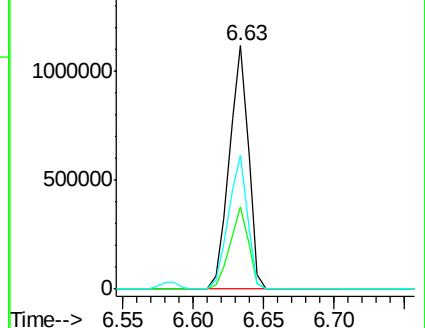



#9

Benzaldehyde

Concen: 38.74 ng

RT: 6.40 min Scan# 733

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion: 77 Resp: 670900

Ion Ratio Lower Upper

77 100

105 100.9 78.6 118.6




106 97.0 76.5 116.5



Abundance Ion 77.00 (76.70 to 77.70): BF1

Ion 105.00 (104.70 to 105.70): BF1

Ion 106.00 (105.70 to 106.70): BF1

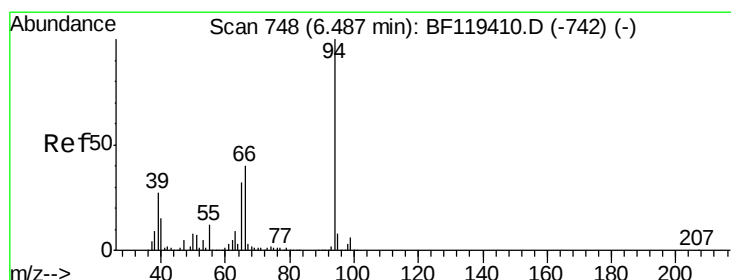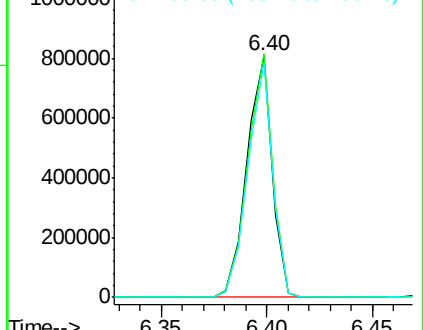

#10

Phenol

Concen: 46.22 ng

RT: 6.49 min Scan# 749

Delta R.T. 0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion: 94 Resp: 1346295

Ion Ratio Lower Upper

94 100

65 29.7 12.0 52.0



66 36.8 20.6 60.6




Abundance Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1




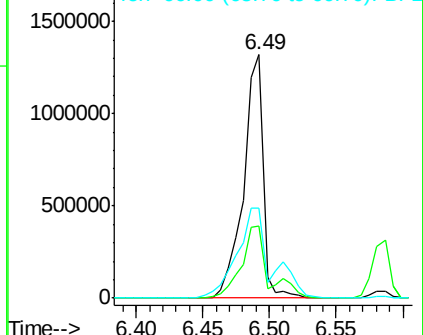




#11
 bis(2-Chloroethyl)ether
 Concen: 42.98 ng
 RT: 6.59 min Scan# 765
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55




Instrument :
 BNA_F
 ClientSampleId :
 TP-11AMS


Tgt Ion: 93 Resp: 1001334
 Ion Ratio Lower Upper
 93 100
 63 87.2 68.4 108.4
 95 33.5 13.4 53.4

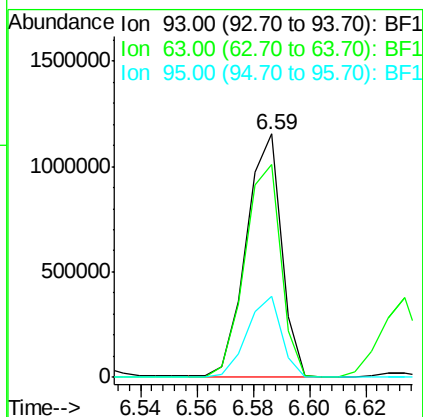

#12
 1,3-Dichlorobenzene
 Concen: 43.20 ng
 RT: 6.79 min Scan# 800
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55

Tgt Ion: 146 Resp: 1049383
 Ion Ratio Lower Upper
 146 100
 148 64.7 51.4 77.0
 75 31.2 25.8 38.8



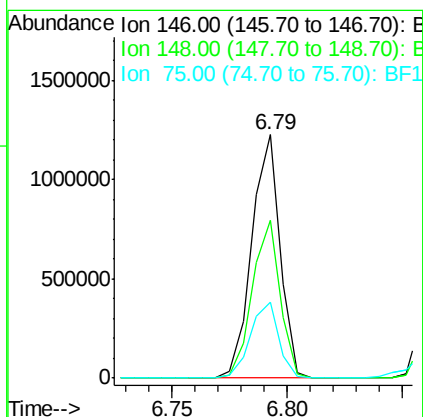



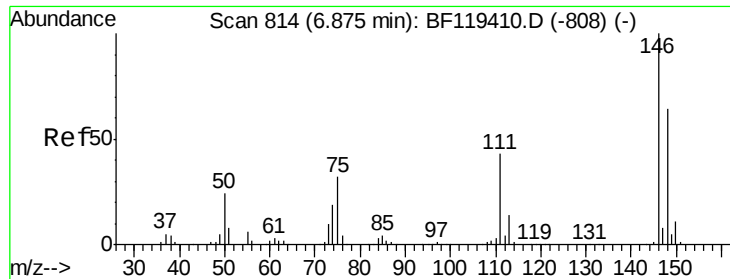

#13
 1,4-Dichlorobenzene
 Concen: 43.44 ng
 RT: 6.87 min Scan# 813
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55




Instrument :
 BNA_F
 ClientSampleId :
 TP-11AMS

Tgt Ion:146 Resp: 1055562
 Ion Ratio Lower Upper
 146 100
 148 64.3 50.9 76.3
 111 42.0 34.6 52.0

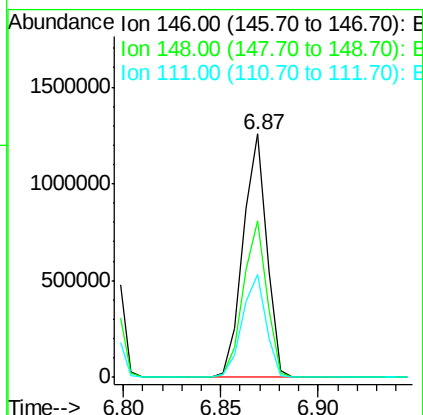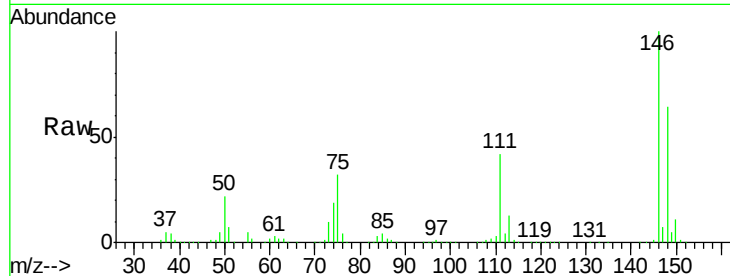

#14
 1,2-Dichlorobenzene
 Concen: 43.37 ng
 RT: 7.02 min Scan# 839
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55

Tgt Ion:146 Resp: 984935
 Ion Ratio Lower Upper
 146 100
 148 63.6 51.7 77.5
 111 45.9 36.4 54.6

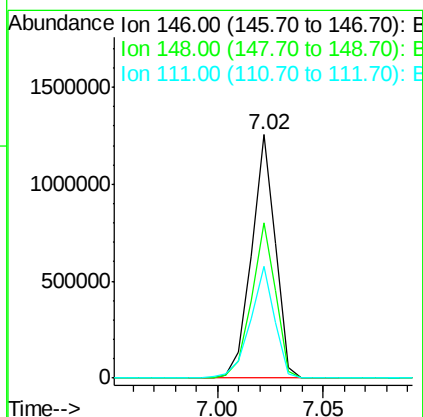



#15

Benzyl Alcohol

Concen: 43.87 ng

RT: 6.99 min Scan# 834

Delta R.T. -0.00 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampled :

TP-11AMS





Tgt Ion: 79 Resp: 900926

Ion Ratio Lower Upper

79 100

108 80.8 60.4 90.6

77 62.4 49.0 73.4

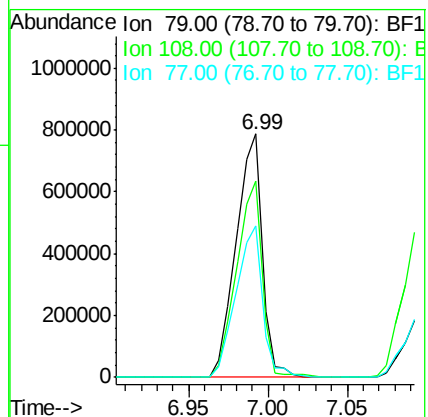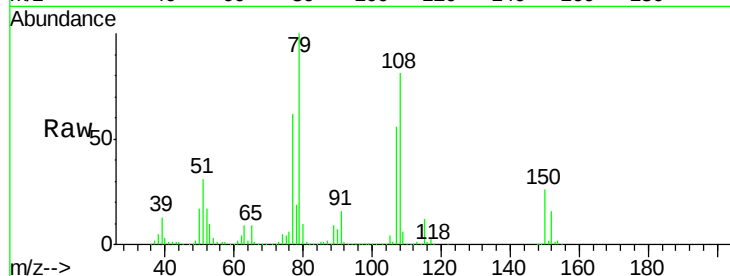

#16

2,2'-oxybis(1-Chloropropane)

Concen: 40.28 ng

RT: 7.13 min Scan# 857

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55




Tgt Ion: 45 Resp: 1892650


Ion Ratio Lower Upper

45 100

77 10.6 0.0 30.1

79 8.0 0.0 27.4

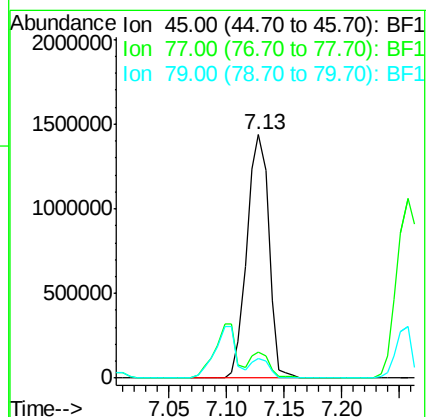


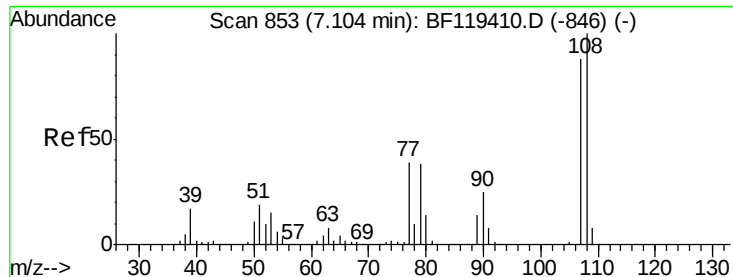




#17
2-Methylphenol
Concen: 41.67 ng
RT: 7.10 min Scan# 853
Delta R.T. 0.00 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Instrument :
BNA_F
ClientSampleId :
TP-11AMS

Tgt Ion:107 Resp: 856831
Ion Ratio Lower Upper
107 100
108 114.9 90.7 136.1
77 44.7 35.6 53.4
79 42.8 34.7 52.1

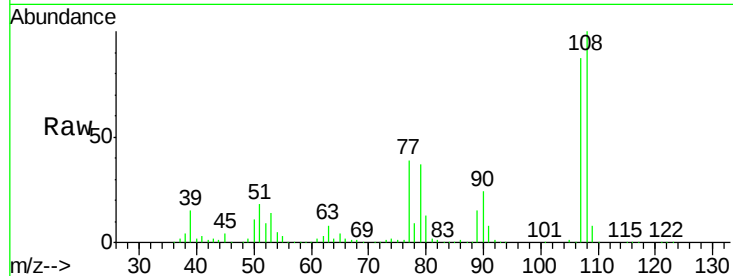


Abundance Ion 107.00 (106.70 to 107.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 77.00 (76.70 to 77.70): BF1
Ion 79.00 (78.70 to 79.70): BF1

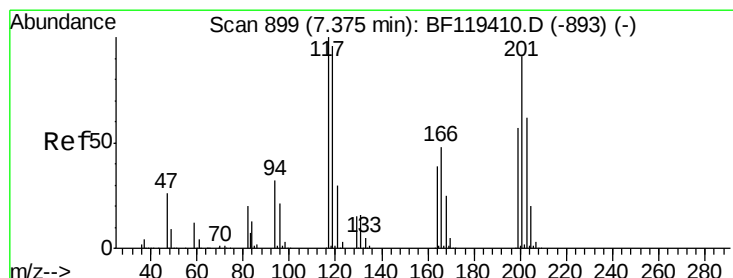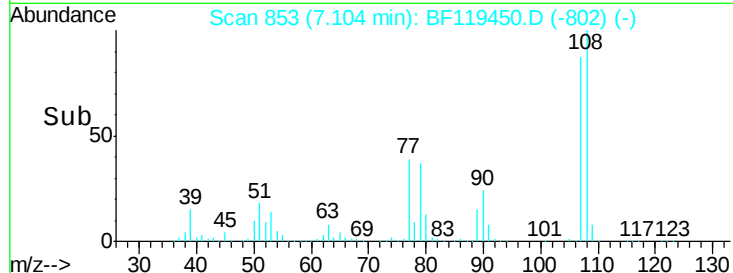
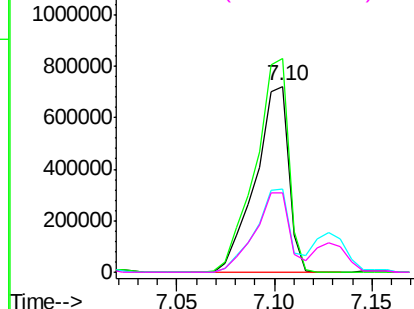





#18
Hexachloroethane
Concen: 45.01 ng
RT: 7.37 min Scan# 898
Delta R.T. -0.01 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Tgt Ion:117 Resp: 400745
Ion Ratio Lower Upper
117 100
119 97.3 76.8 115.2
201 99.2 72.5 108.7

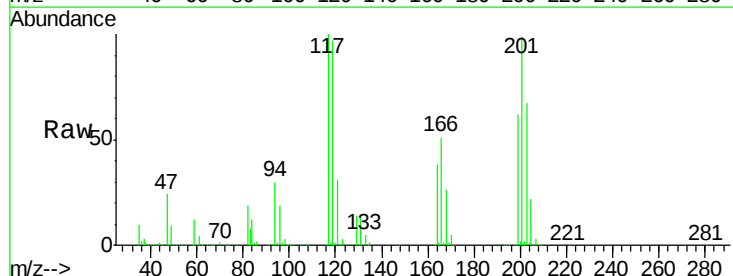

Abundance Ion 117.00 (116.70 to 117.70): E
Ion 119.00 (118.70 to 119.70): E
Ion 201.00 (200.70 to 201.70): E

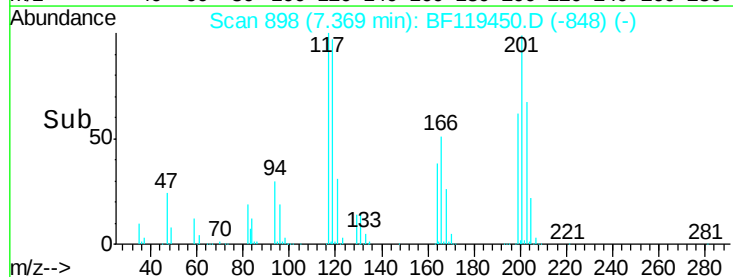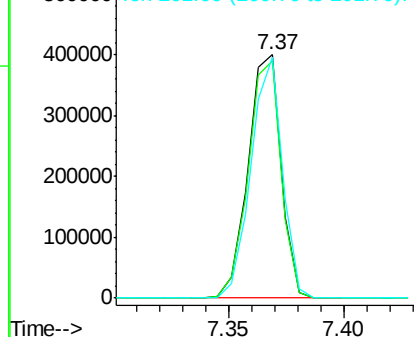

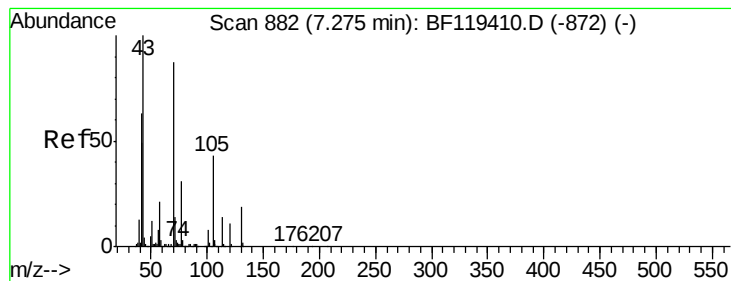

#19

n-Nitroso-di-n-propylamine

Concen: 43.05 ng

RT: 7.27 min Scan# 881

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS

Tgt Ion: 70 Resp: 708387





Ion Ratio Lower Upper

70 100

42 71.5 58.2 87.4

101 9.1 7.4 11.2

130 22.0 17.8 26.8

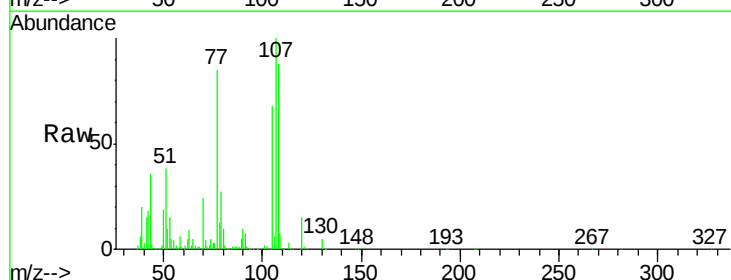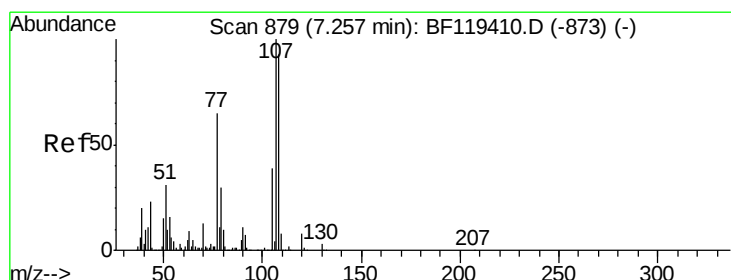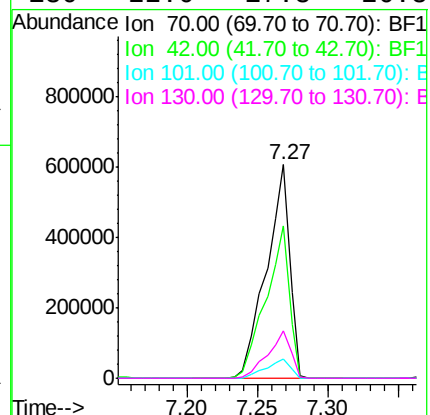

#20

3+4-Methylphenols

Concen: 40.54 ng

RT: 7.25 min Scan# 878

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Tgt Ion: 107 Resp: 1021685


Ion Ratio Lower Upper


107 100

108 88.2 72.6 112.6

77 84.6 44.7 84.7

79 27.4 10.2 50.2

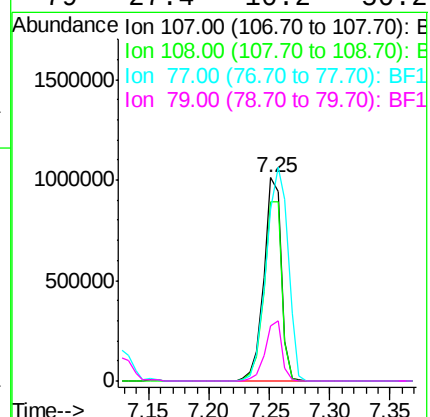




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.14 min Scan# 1029
Delta R.T. -0.01 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55




Instrument :
BNA_F
ClientSampleId :
TP-11AMS

Tgt Ion:136 Resp: 1295579

Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.4	12.6
54	10.0	8.3	12.5
68	5.6	4.9	7.3




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

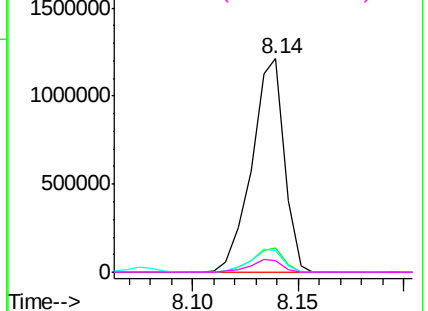



#22
Acetophenone
Concen: 43.42 ng
RT: 7.26 min Scan# 880
Delta R.T. -0.01 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55


Tgt Ion:105 Resp: 1344237

Ion	Ratio	Lower	Upper
105	100		
71	6.7	5.8	8.6
51	34.4	26.8	40.2
120	22.9	18.0	27.0



Abundance Ion 105.00 (104.70 to 105.70): E
Ion 71.00 (70.70 to 71.70): BF1
Ion 51.00 (50.70 to 51.70): BF1
Ion 120.00 (119.70 to 120.70): E




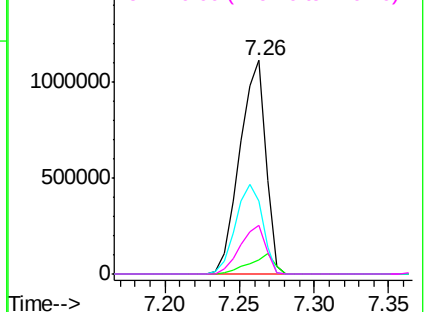




#23
 Nitrobenzene-d5
 Concen: 74.14 ng
 RT: 7.42 min Scan# 906
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55




Instrument :
 BNA_F
 ClientSampleId :
 TP-11AMS


Tgt Ion: 82 Resp: 1767352
 Ion Ratio Lower Upper
 82 100
 128 46.0 35.8 53.8
 54 63.8 53.4 80.0

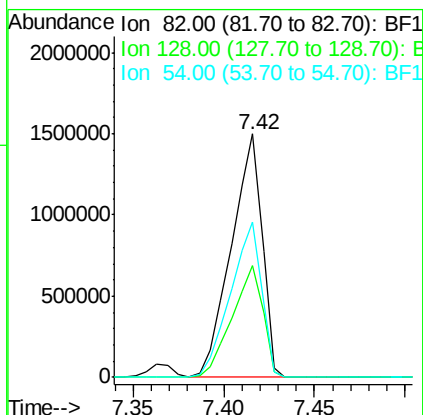

#24
 Nitrobenzene
 Concen: 41.44 ng
 RT: 7.43 min Scan# 909
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55

Tgt Ion: 77 Resp: 1055670
 Ion Ratio Lower Upper
 77 100
 123 47.9 36.9 55.3
 65 16.0 12.2 18.4

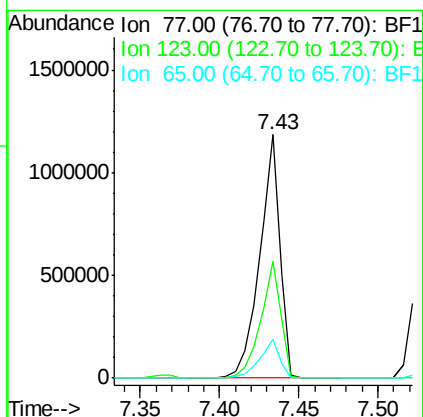



#25

Isophorone

Concen: 41.26 ng

RT: 7.67 min Scan# 950

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS





Tgt Ion: 82 Resp: 1995089

Ion Ratio Lower Upper

82 100

95 7.0 5.4 8.2

138 18.1 13.8 20.8

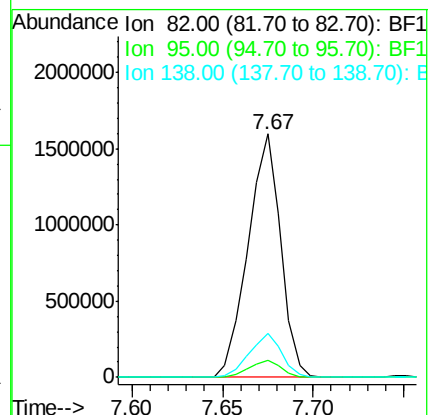

#26

2-Nitrophenol

Concen: 51.53 ng

RT: 7.75 min Scan# 963

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55




Tgt Ion: 139 Resp: 516922


Ion Ratio Lower Upper

139 100

109 25.3 21.7 32.5

65 53.2 43.9 65.9

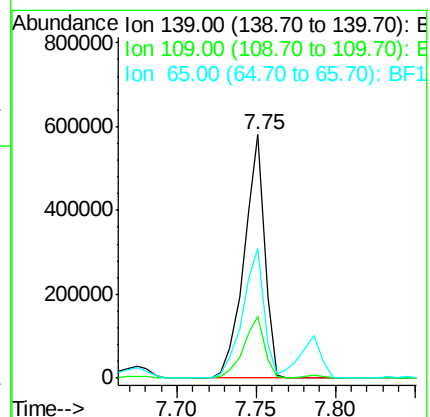







#27
2,4-Dimethylphenol
Concen: 46.13 ng
RT: 7.79 min Scan# 969
Delta R.T. -0.00 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Instrument :
BNA_F
ClientSampleId :
TP-11AMS

Tgt Ion:122 Resp: 956850
Ion Ratio Lower Upper
122 100
107 113.3 91.8 137.6
121 58.1 46.5 69.7




Abundance Ion 122.00 (121.70 to 122.70): E
Ion 107.00 (106.70 to 107.70): E
Ion 121.00 (120.70 to 121.70): E

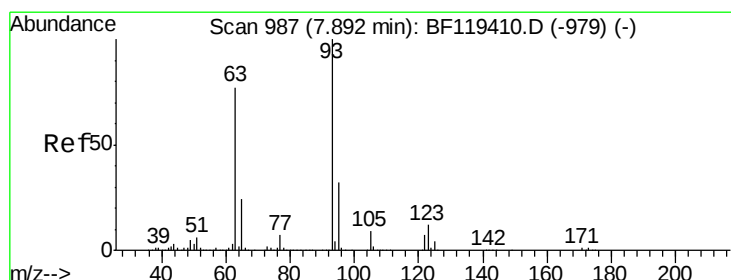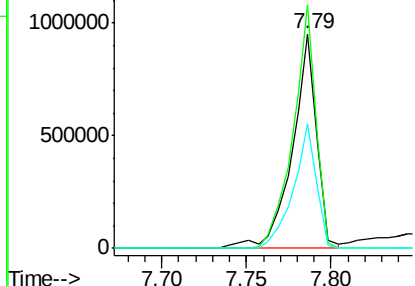




#28
bis(2-Chloroethoxy)methane
Concen: 43.65 ng
RT: 7.89 min Scan# 986
Delta R.T. -0.01 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Tgt Ion: 93 Resp: 1248103
Ion Ratio Lower Upper
93 100
95 33.2 26.0 39.0
123 11.8 9.7 14.5



Abundance Ion 93.00 (92.70 to 93.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 123.00 (122.70 to 123.70): E



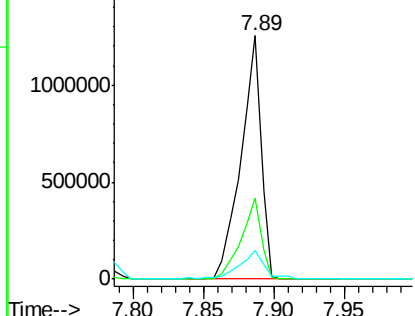





#29
 2,4-Dichlorophenol
 Concen: 43.68 ng
 RT: 7.99 min Scan# 1004
 Delta R.T. -0.00 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55




Instrument :
 BNA_F
 ClientSampleId :
 TP-11AMS


Tgt Ion:162 Resp: 832494
 Ion Ratio Lower Upper
 162 100
 164 64.9 43.6 83.6
 98 37.8 20.4 60.4

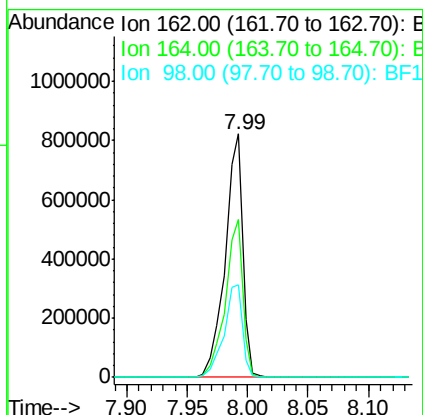

#30
 1,2,4-Trichlorobenzene
 Concen: 42.96 ng
 RT: 8.08 min Scan# 1019
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55

Tgt Ion:180 Resp: 905348
 Ion Ratio Lower Upper
 180 100
 182 95.9 76.6 115.0
 145 29.7 23.2 34.8

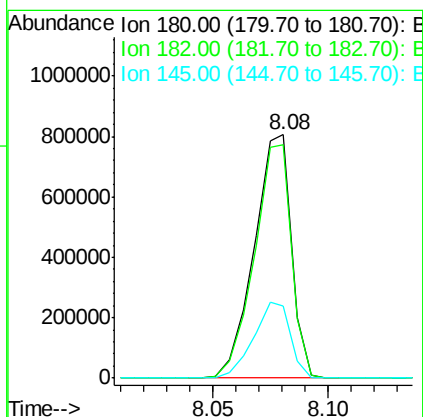



#31

Naphthalene

Concen: 42.84 ng

RT: 8.16 min Scan# 1033

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion:128 Resp: 2856081

Ion Ratio Lower Upper

128 100

129 11.3 9.3 13.9




127 13.8 11.0 16.4



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

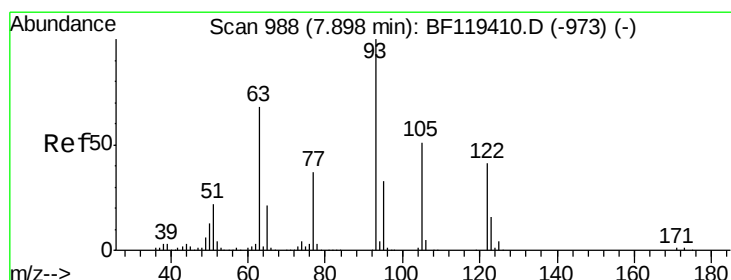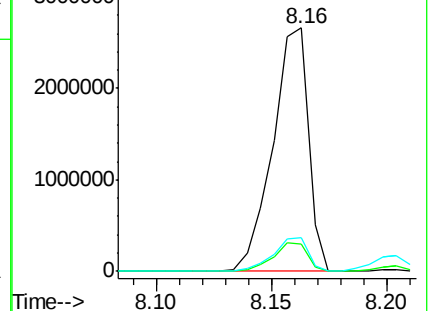

#32

Benzoic acid

Concen: 46.23 ng

RT: 7.91 min Scan# 990

Delta R.T. 0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion:122 Resp: 616793

Ion Ratio Lower Upper

122 100

105 119.2 102.9 142.9



77 91.0 70.1 110.1




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF1

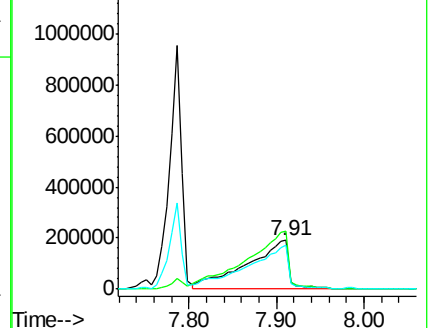

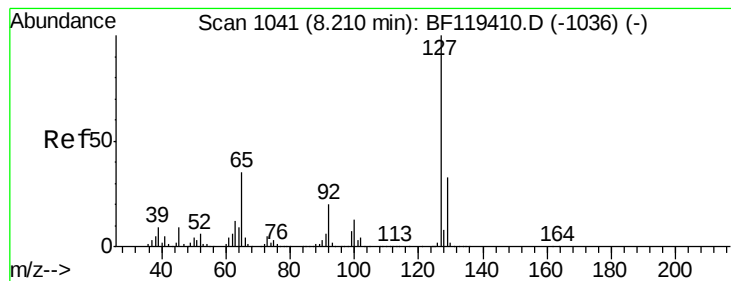

#33

4-Chloroaniline

Concen: 6.49 ng

RT: 8.20 min Scan# 1040

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS

Tgt Ion:127 Resp: 198386


Ion Ratio Lower Upper

127 100

129 30.8 26.2 39.4

65 31.1 27.7 41.5

92 18.5 15.8 23.6






Abundance Ion 127.00 (126.70 to 127.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 65.00 (64.70 to 65.70): BF1

Ion 92.00 (91.70 to 92.70): BF1

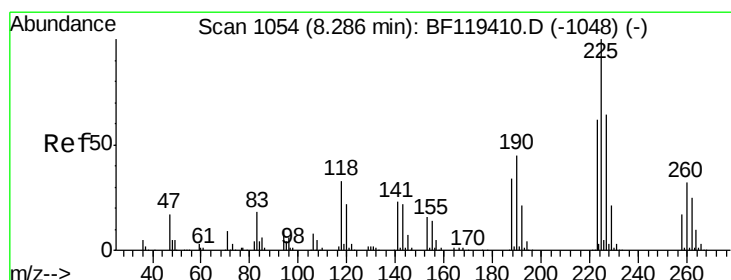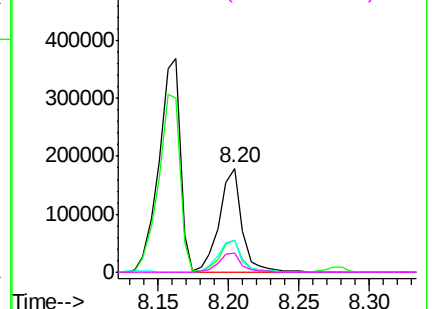

#34

Hexachlorobutadiene

Concen: 43.03 ng

RT: 8.28 min Scan# 1053

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion:225 Resp: 507410

Ion Ratio Lower Upper

225 100

223 61.7 49.2 73.8



227 63.8 51.1 76.7




Abundance Ion 225.00 (224.70 to 225.70): E

Ion 223.00 (222.70 to 223.70): E

Ion 227.00 (226.70 to 227.70): E



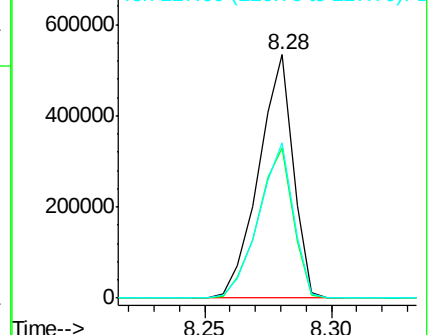





#35
 Caprolactam
 Concen: 27.31 ng
 RT: 8.58 min Scan# 1104
 Delta R.T. -0.00 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55




Instrument :
 BNA_F
 ClientSampleId :
 TP-11AMS


Tgt Ion:113 Resp: 170362
 Ion Ratio Lower Upper
 113 100
 55 224.4 208.4 248.4
 56 159.4 138.9 178.9

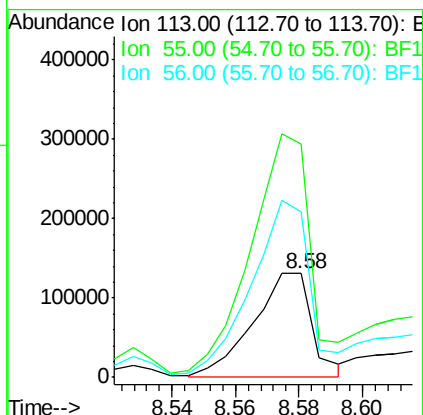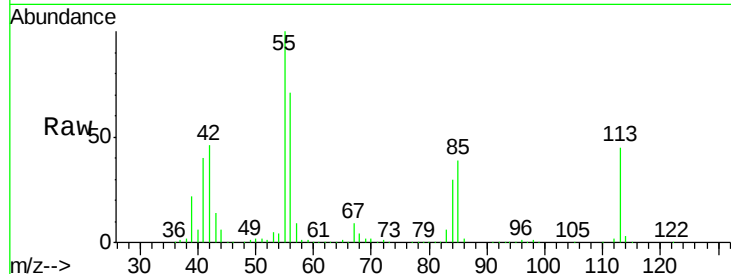

#36
 4-Chloro-3-methylphenol
 Concen: 42.72 ng
 RT: 8.69 min Scan# 1122
 Delta R.T. 0.00 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55

Tgt Ion:107 Resp: 889783
 Ion Ratio Lower Upper
 107 100
 144 26.6 20.6 31.0
 142 80.5 63.8 95.6

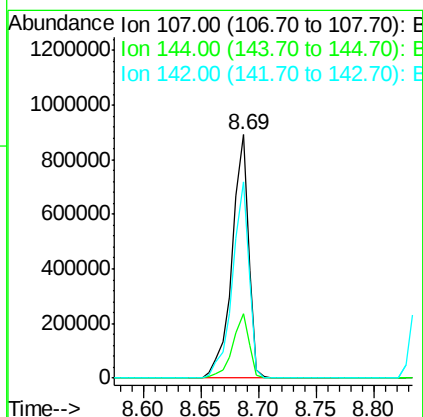

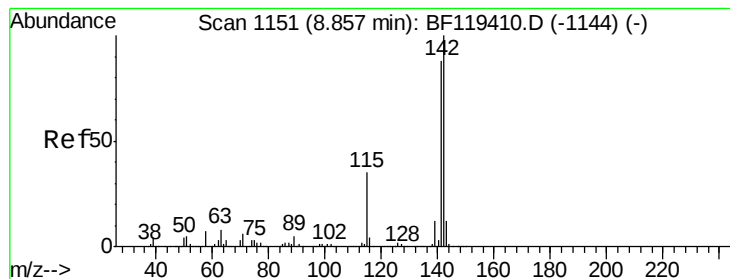

#37

2-Methylnaphthalene

Concen: 43.79 ng

RT: 8.85 min Scan# 1150

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion:142 Resp: 1916009

Ion Ratio Lower Upper

142 100

141 88.2 70.4 105.6




115 34.9 27.8 41.6



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

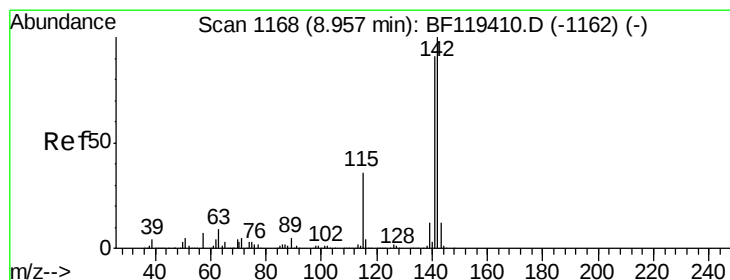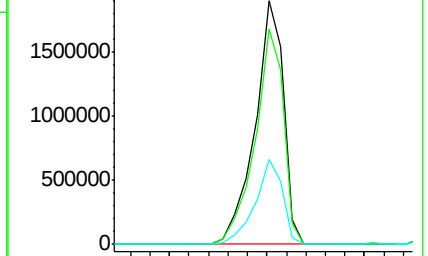

#38

1-Methylnaphthalene

Concen: 43.54 ng

RT: 8.95 min Scan# 1167

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion:142 Resp: 1803301

Ion Ratio Lower Upper

142 100

141 91.4 73.1 109.7



116 3.8 3.0 4.6




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

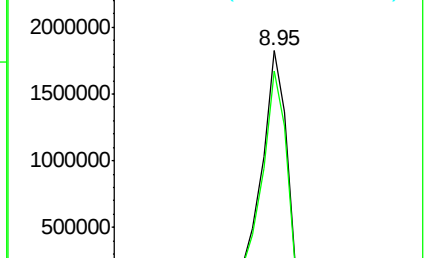



#39

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.90 min Scan# 1328

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion:164 Resp: 652485

Ion Ratio Lower Upper




164 100

162 104.9 80.7 121.1

160 47.0 35.5 53.3



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

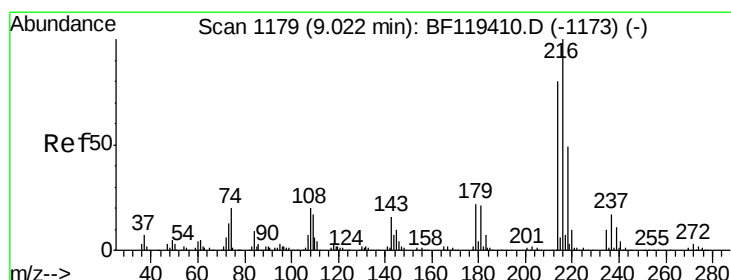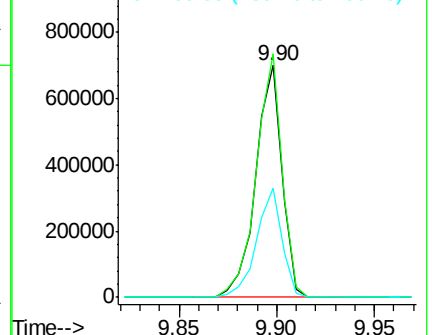

#40

1,2,4,5-Tetrachlorobenzene

Concen: 42.29 ng

RT: 9.02 min Scan# 1179

Delta R.T. -0.00 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Tgt Ion:216 Resp: 808761


Ion Ratio Lower Upper

216 100



214 78.8 63.0 94.6


179 21.5 17.0 25.4

108 20.8 15.4 23.0

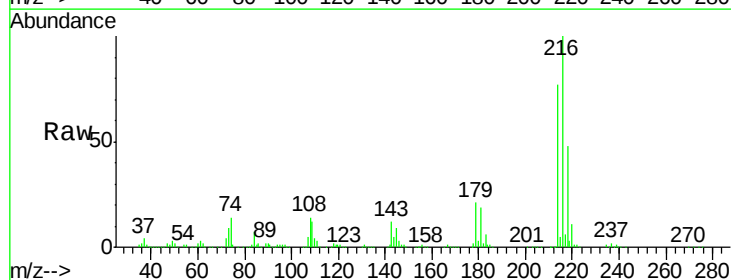

Abundance Ion 216.00 (215.70 to 216.70): E
Ion 214.00 (213.70 to 214.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 108.00 (107.70 to 108.70): E

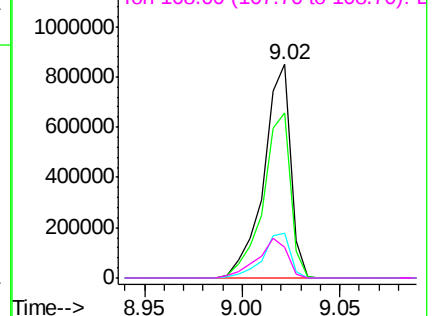

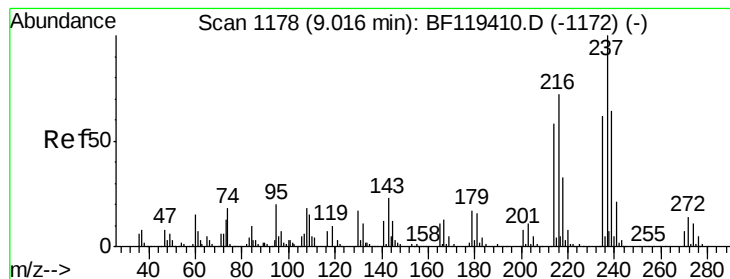

#41

Hexachlorocyclopentadiene

Concen: 80.85 ng

RT: 9.01 min Scan# 1177

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion:237 Resp: 879069

Ion Ratio Lower Upper




237 100

235 63.9 42.5 82.5

272 13.8 0.0 34.3



Abundance Ion 236.80 (236.50 to 237.50): E
Ion 234.90 (234.60 to 235.60): E
Ion 271.75 (271.45 to 272.45): E

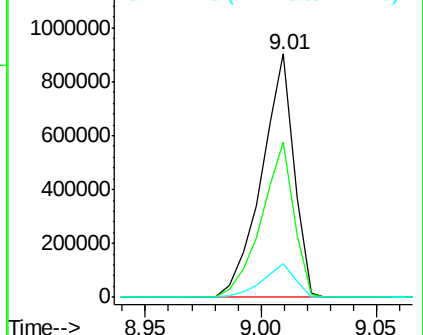

#42

2,4,6-Tribromophenol

Concen: 108.42 ng

RT: 10.69 min Scan# 1462

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion:330 Resp: 729832

Ion Ratio Lower Upper



330 100

332 97.2 77.6 116.4

141 32.4 26.6 40.0



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



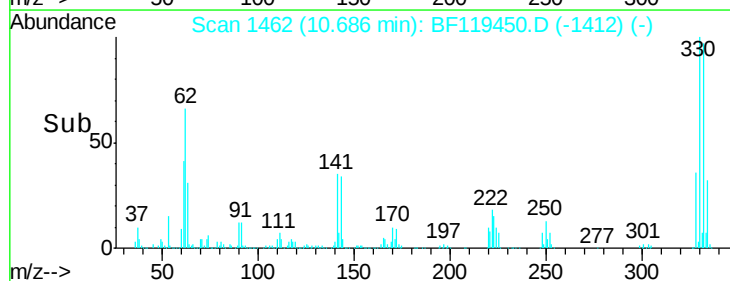
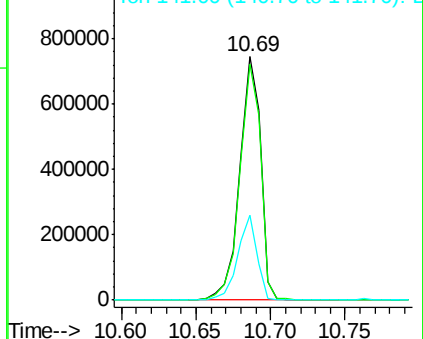




#43
 2,4,6-Trichlorophenol
 Concen: 45.49 ng
 RT: 9.13 min Scan# 1197
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55




Instrument :
 BNA_F
 ClientSampleId :
 TP-11AMS


Tgt Ion:196 Resp: 622609
 Ion Ratio Lower Upper
 196 100
 198 97.0 77.0 115.4
 200 31.3 25.1 37.7

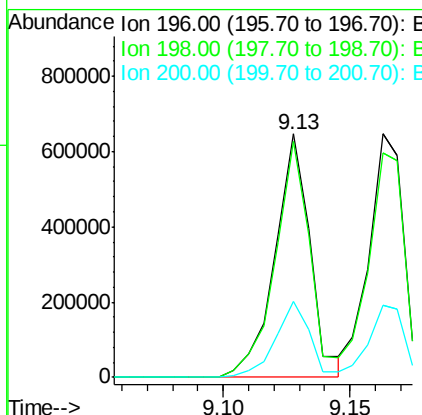

#44
 2,4,5-Trichlorophenol
 Concen: 40.03 ng
 RT: 9.16 min Scan# 1203
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55

Tgt Ion:196 Resp: 613763
 Ion Ratio Lower Upper
 196 100
 198 92.3 75.3 112.9
 97 54.9 39.0 58.4
 132 31.2 22.9 34.3

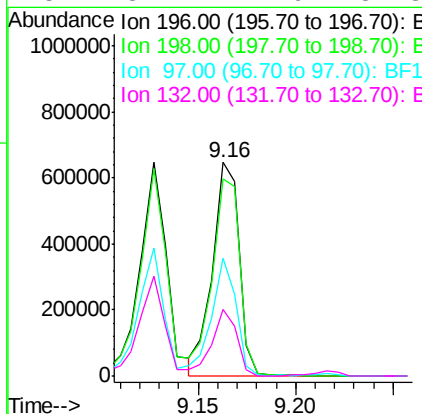







#45
2-Fluorobiphenyl
Concen: 71.42 ng
RT: 9.22 min Scan# 1212
Delta R.T. -0.01 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Instrument :
BNA_F
ClientSampleId :
TP-11AMS

Tgt Ion:172 Resp: 3145374
Ion Ratio Lower Upper
172 100
171 37.1 29.9 44.9
170 25.1 20.1 30.1




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


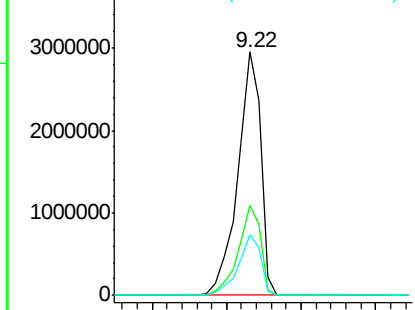



#46
1,1'-Biphenyl
Concen: 41.70 ng
RT: 9.32 min Scan# 1229
Delta R.T. -0.01 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Tgt Ion:154 Resp: 2215832
Ion Ratio Lower Upper
154 100
153 41.5 21.4 61.4
76 14.2 0.0 33.6



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 76.00 (75.70 to 76.70): BF1

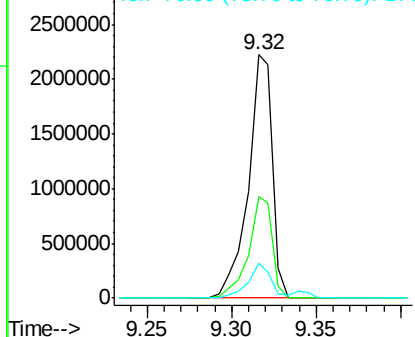







#47
2-Chloronaphthalene
Concen: 41.93 ng
RT: 9.35 min Scan# 1234
Delta R.T. 0.00 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Instrument :
BNA_F
ClientSampleId :
TP-11AMS

Tgt Ion: 162 Resp: 1745374
Ion Ratio Lower Upper
162 100
127 39.9 33.7 50.5
164 34.3 26.2 39.4

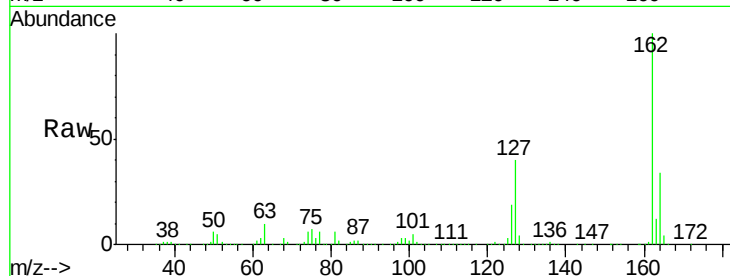


Abundance Ion 162.00 (161.70 to 162.70): E
Ion 127.00 (126.70 to 127.70): E
Ion 164.00 (163.70 to 164.70): E


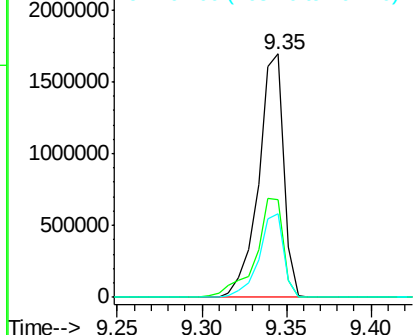



#48
2-Nitroaniline
Concen: 43.07 ng
RT: 9.43 min Scan# 1249
Delta R.T. -0.01 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Tgt Ion: 65 Resp: 618817
Ion Ratio Lower Upper
65 100
92 61.9 50.5 75.7
138 92.4 75.8 113.8



Abundance Ion 65.00 (64.70 to 65.70): BF1
Ion 92.00 (91.70 to 92.70): BF1
Ion 138.00 (137.70 to 138.70): E

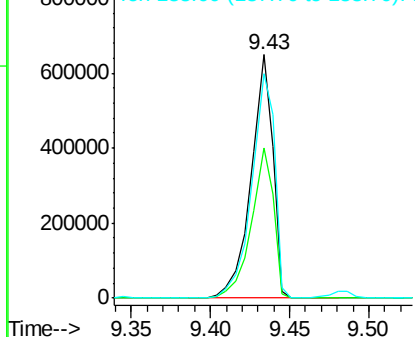



#49

Acenaphthylene

Concen: 42.23 ng

RT: 9.76 min Scan# 1305

Delta R.T. 0.00 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion:152 Resp: 2760777

Ion Ratio Lower Upper

152 100

151 21.0 16.8 25.2




153 13.6 11.2 16.8



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

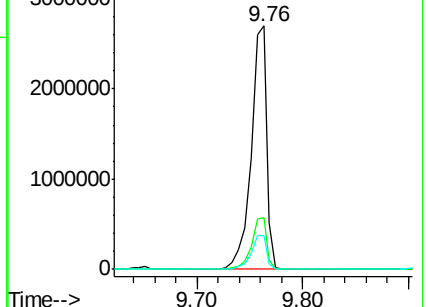

#50

Dimethylphthalate

Concen: 47.05 ng

RT: 9.62 min Scan# 1281

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion:163 Resp: 2180797

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8



164 10.8 8.1 12.1




Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E




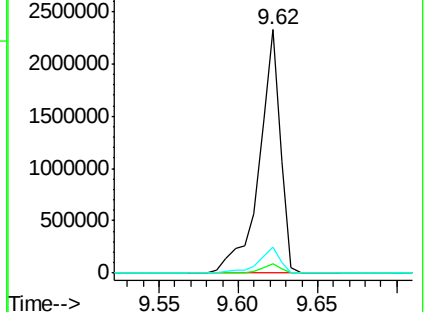


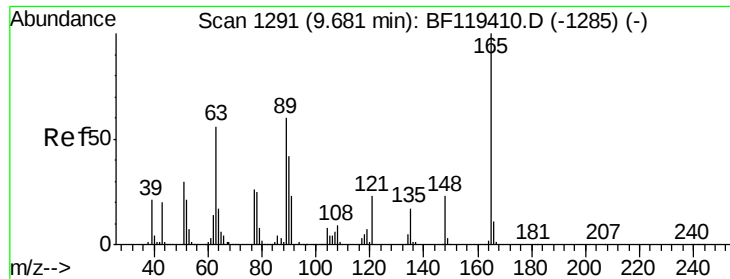

#51
 2,6-Dinitrotoluene
 Concen: 44.77 ng
 RT: 9.68 min Scan# 1291
 Delta R.T. -0.00 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55




Instrument :
 BNA_F
 ClientSampleId :
 TP-11AMS

Tgt Ion:165 Resp: 444755
 Ion Ratio Lower Upper
 165 100
 63 56.6 57.3 85.9#
 89 51.7 47.8 71.8

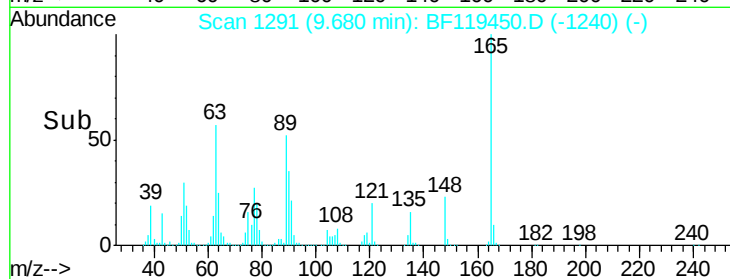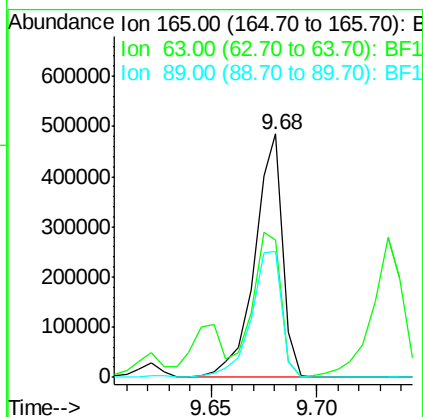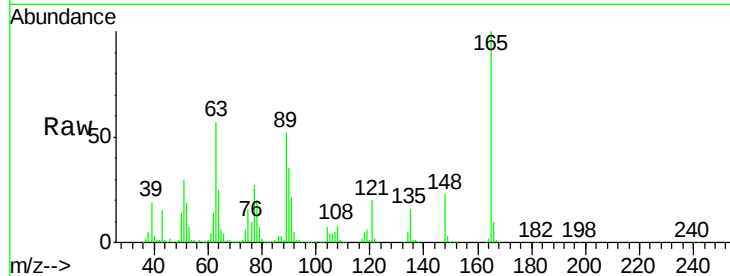

#52
 Acenaphthene
 Concen: 44.14 ng
 RT: 9.93 min Scan# 1334
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55

Tgt Ion:154 Resp: 1798753
 Ion Ratio Lower Upper
 154 100
 153 110.1 89.0 133.6
 152 53.4 43.1 64.7

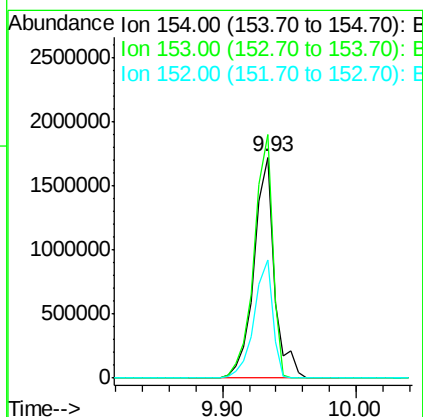







#53
3-Nitroaniline
Concen: 13.65 ng
RT: 9.84 min Scan# 1318
Delta R.T. -0.01 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Instrument :
BNA_F
ClientSampleId :
TP-11AMS

Tgt Ion:138 Resp: 171145
Ion Ratio Lower Upper
138 100
108 11.7 9.0 13.6
92 117.5 93.2 139.8




Abundance Ion 138.00 (137.70 to 138.70): E
Ion 108.00 (107.70 to 108.70): E
Ion 92.00 (91.70 to 92.70): BF1


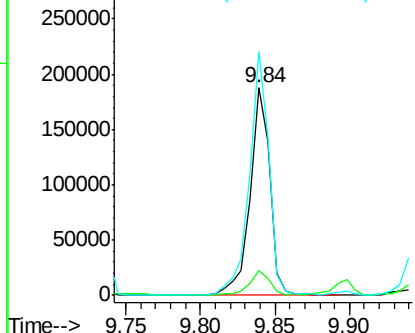



#54
2,4-Dinitrophenol
Concen: 73.04 ng
RT: 9.95 min Scan# 1337
Delta R.T. 0.00 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Tgt Ion:184 Resp: 310966
Ion Ratio Lower Upper
184 100
63 67.1 58.5 87.7
154 56.7 51.8 77.6



Abundance Ion 184.00 (183.70 to 184.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 154.00 (153.70 to 154.70): E

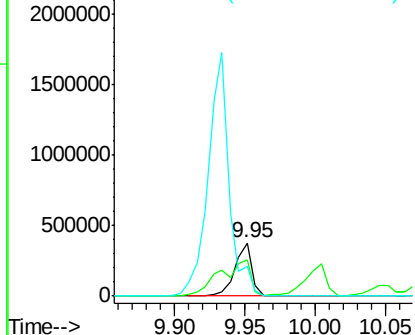



#55

Dibenzofuran

Concen: 42.24 ng

RT: 10.10 min Scan# 1363

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion:168 Resp: 2468098

Ion Ratio Lower Upper

168 100

139 38.8 30.2 45.4




169 14.1 11.1 16.7



Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E

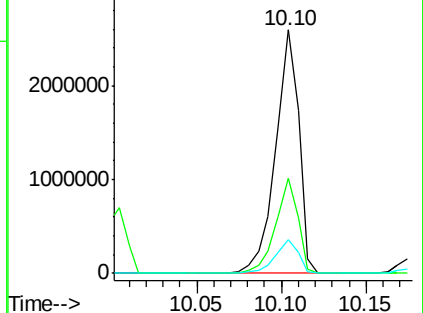

#56

4-Nitrophenol

Concen: 78.15 ng

RT: 10.00 min Scan# 1346

Delta R.T. 0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion:139 Resp: 773192

Ion Ratio Lower Upper

139 100

109 64.5 39.6 79.6



65 109.1 78.3 118.3




Abundance Ion 139.00 (138.70 to 139.70): E

Ion 109.00 (108.70 to 109.70): E

Ion 65.00 (64.70 to 65.70): BF1




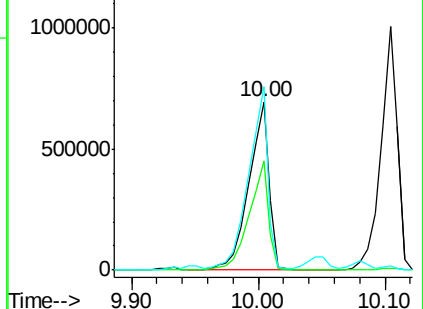




#57
2,4-Dinitrotoluene
Concen: 46.83 ng
RT: 10.08 min Scan# 1359
Delta R.T. -0.01 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55




Instrument :
BNA_F
ClientSampleId :
TP-11AMS


Tgt Ion:	165	Resp:	586076
Ion	Ratio	Lower	Upper
165	100		
63	53.3	36.2	54.4
89	77.5	54.3	81.5
182	2.6	2.0	3.0

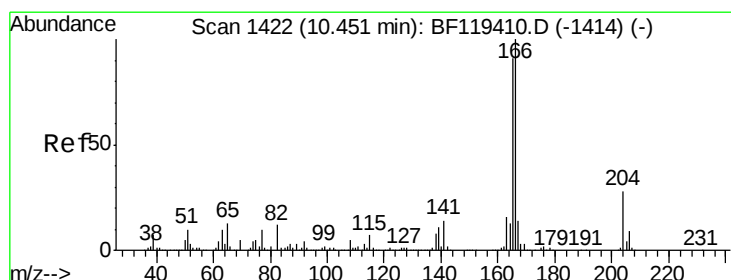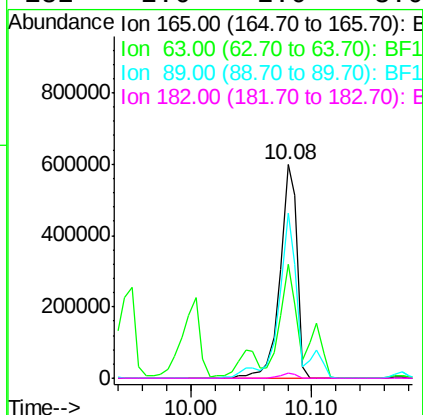

#58
Fluorene
Concen: 42.26 ng
RT: 10.45 min Scan# 1421
Delta R.T. -0.01 min
Lab File: BF119450.D
Acq: 19 Mar 2020 20:55

Tgt Ion:	166	Resp:	1825820
Ion	Ratio	Lower	Upper
166	100		
165	93.5	73.1	109.7
167	14.4	11.0	16.6

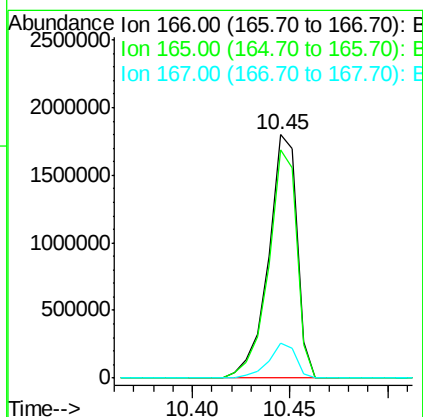


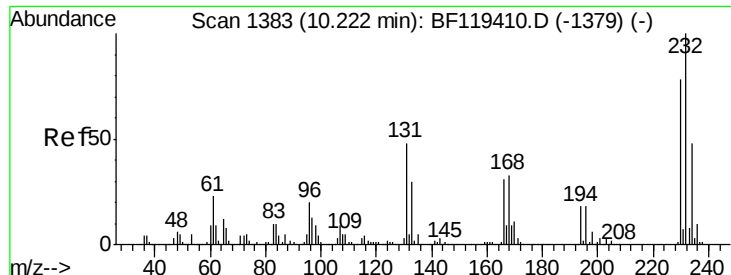




#59
 2,3,4,6-Tetrachlorophenol
 Concen: 44.49 ng
 RT: 10.22 min Scan# 1382
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55

Instrument :
 BNA_F
 ClientSampleId :
 TP-11AMS

Tgt Ion: 232 Resp: 509886
 Ion Ratio Lower Upper
 232 100
 131 46.7 36.3 54.5
 130 2.2 1.8 2.6
 166 31.5 24.9 37.3




Abundance Ion 232.00 (231.70 to 232.70): E
 Ion 131.00 (130.70 to 131.70): E
 Ion 130.00 (129.70 to 130.70): E
 Ion 166.00 (165.70 to 166.70): E

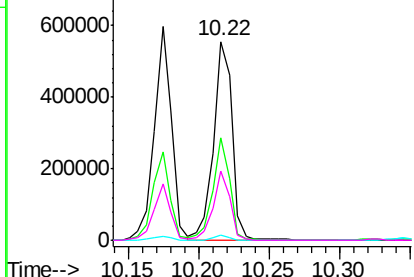




#60
 Diethylphthalate
 Concen: 42.47 ng
 RT: 10.32 min Scan# 1400
 Delta R.T. -0.01 min
 Lab File: BF119450.D
 Acq: 19 Mar 2020 20:55

Tgt Ion: 149 Resp: 1997908
 Ion Ratio Lower Upper
 149 100
 177 21.4 17.0 25.6
 150 13.4 10.2 15.4



Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 177.00 (176.70 to 177.70): E
 Ion 150.00 (149.70 to 150.70): E

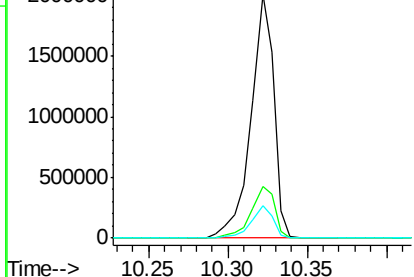



#61

4-Chlorophenyl-phenylether

Concen: 41.73 ng

RT: 10.44 min Scan# 1420

Delta R.T. -0.01 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

TP-11AMS


Tgt Ion:204 Resp: 881769

Ion Ratio Lower Upper

204 100

206 32.5 26.7 40.1




141 59.7 48.8 73.2



Abundance Ion 204.00 (203.70 to 204.70): E

Ion 206.00 (205.70 to 206.70): E

Ion 141.00 (140.70 to 141.70): E

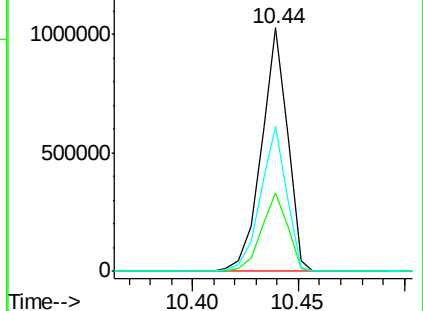

#62

4-Nitroaniline

Concen: 34.81 ng

RT: 10.46 min Scan# 1424

Delta R.T. -0.00 min

Lab File: BF119450.D

Acq: 19 Mar 2020 20:55


Tgt Ion:138 Resp: 418606

Ion Ratio Lower Upper

138 100

92 51.1 32.0 72.0

108 63.7 46.0 86.0



Abundance Ion 138.00 (137.70 to 138.70): E

Ion 92.00 (91.70 to 92.70): BF1

Ion 108.00 (107.70 to 108.70): E

