


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF031920\
 Data File : BF119441.D
 Acq On : 19 Mar 2020 15:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 18 15:11:18 2020

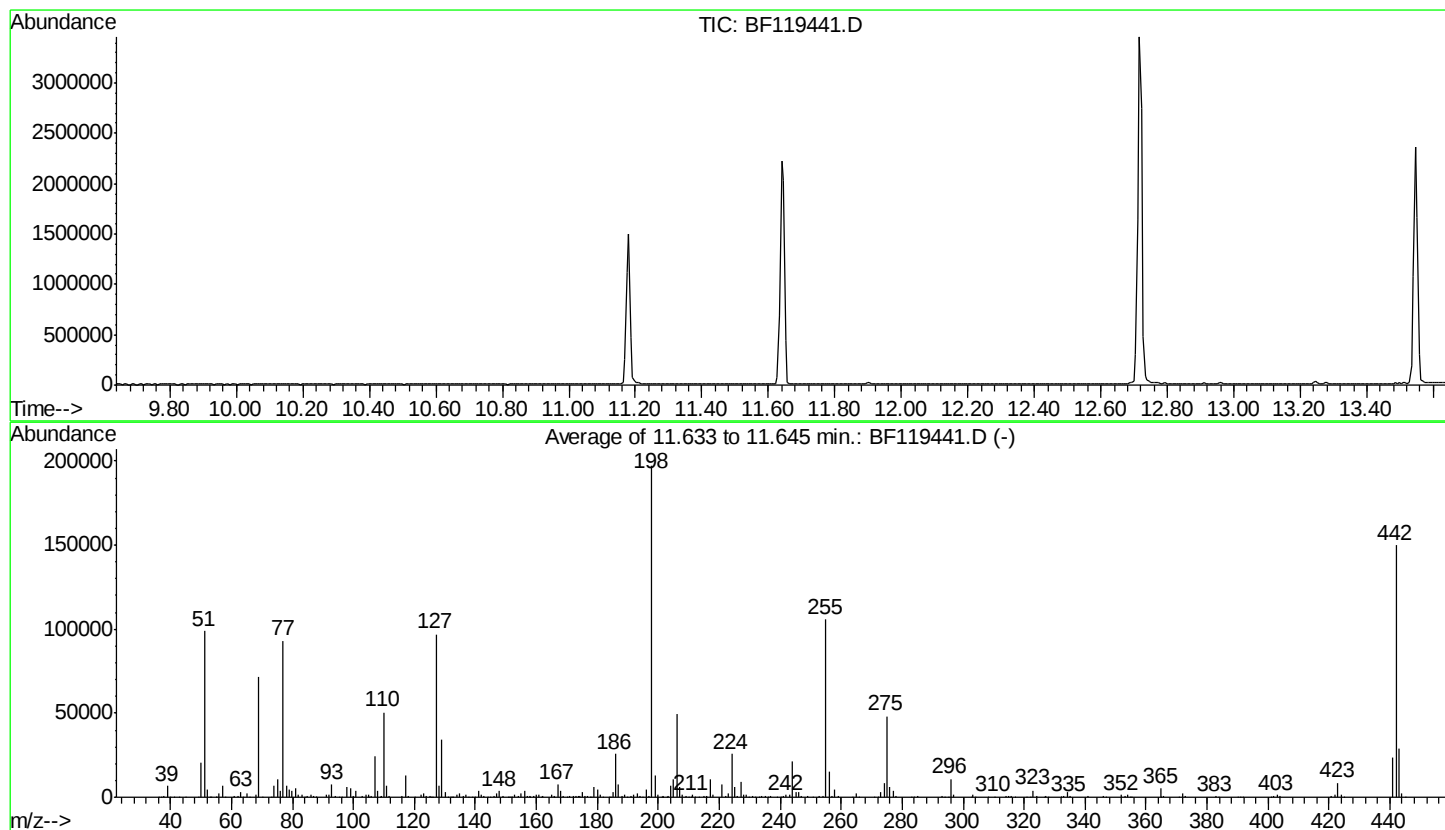

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	98928	PASS
68	69	0.00	2	2.0	1402	PASS
69	198	0.00	100	36.2	71437	PASS
70	69	0.00	2	0.3	237	PASS
127	198	10	80	49.2	96976	PASS
197	198	0.00	2	0.3	635	PASS
198	198	100	100	100.0	197288	PASS
199	198	5	9	6.5	12733	PASS
275	198	10	60	24.4	48116	PASS
365	198	1	100	2.6	5061	PASS
441	198	0.01	100	12.1	23820	PASS
442	198	50	100	75.9	149816	PASS
443	442	15	24	19.2	28824	PASS