
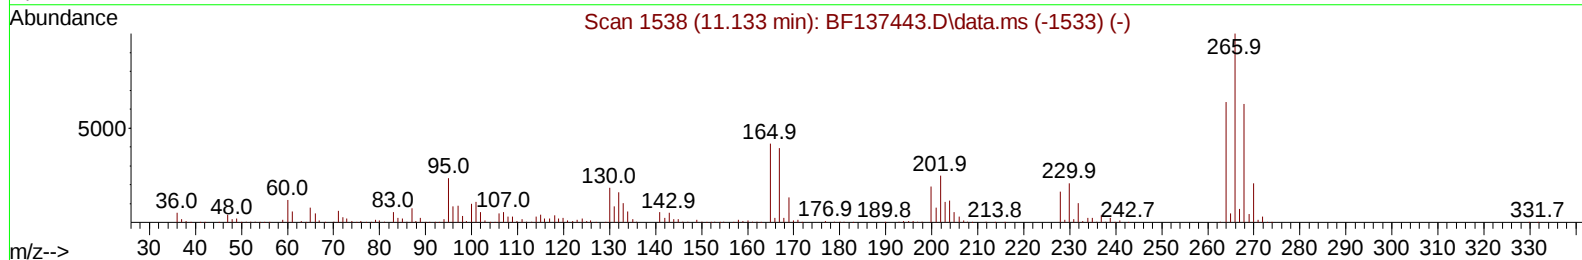
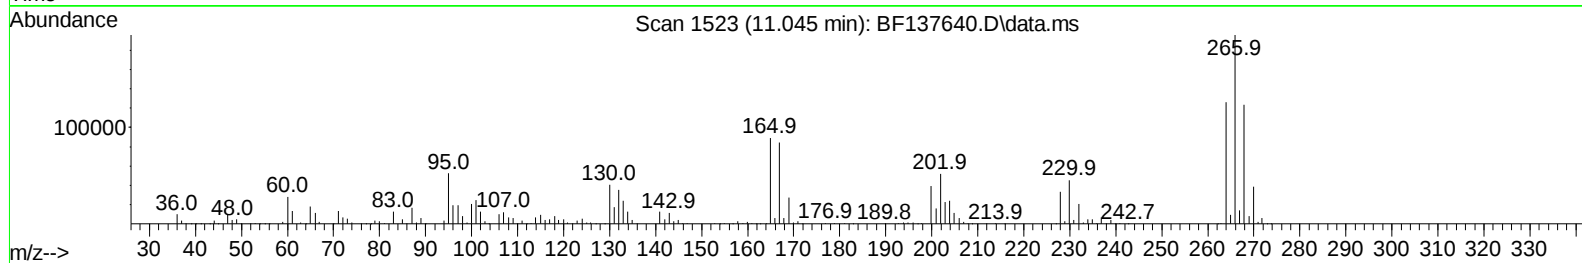


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031924\
Data File : BF137640.D
Acq On : 19 Mar 2024 11:14
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 00:30:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

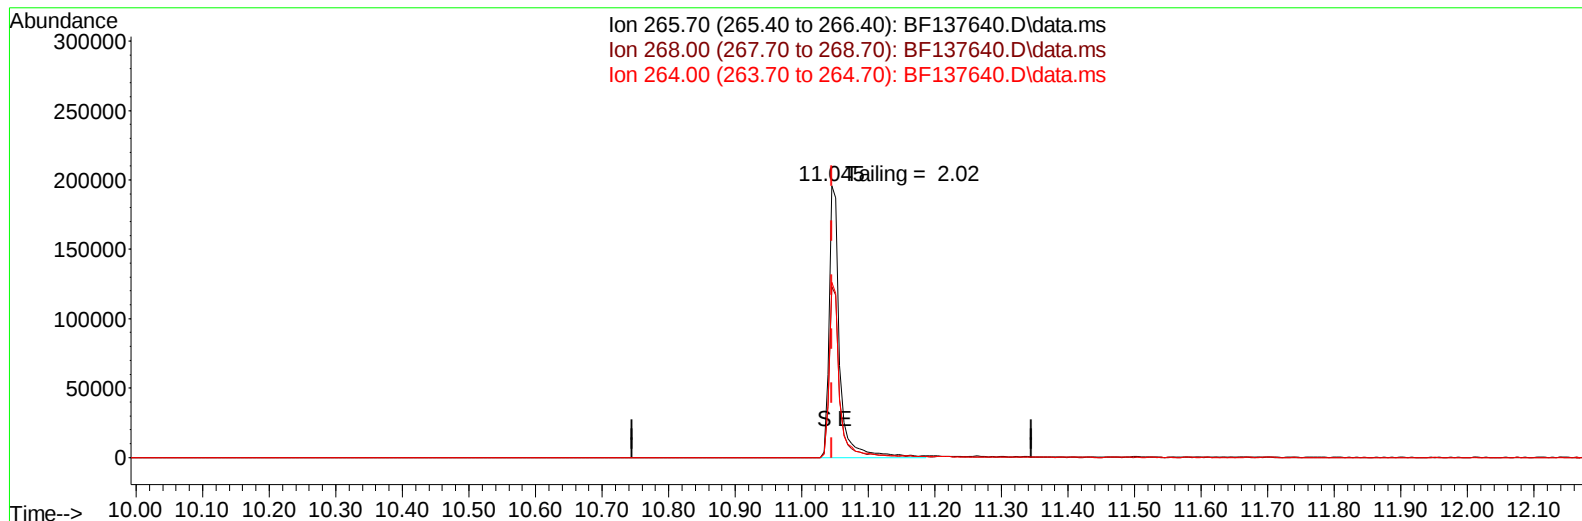

TIC: BF137640.D\data.ms




(70) Pentachlorophenol (C)

11.045min (-0.000) 41357.50 ng

response 215904

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.96
264.00	63.60	64.39
0.00	0.00	0.00

Quant Time: Mar 20 00:30:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

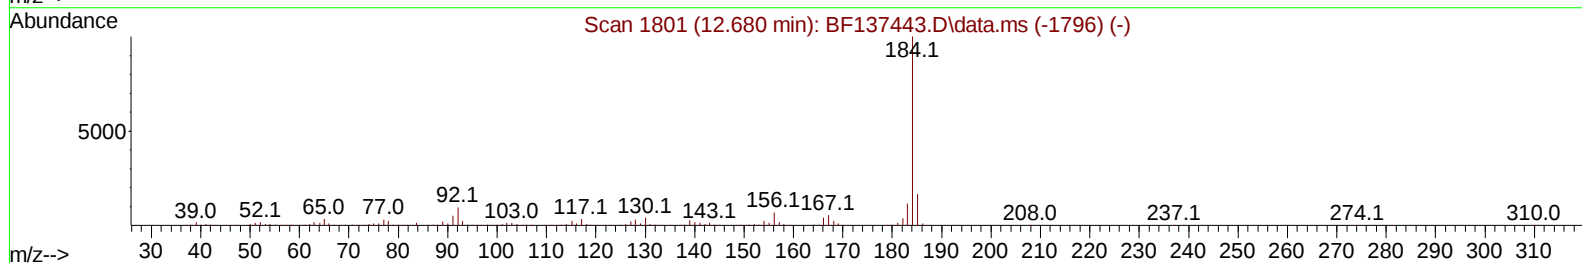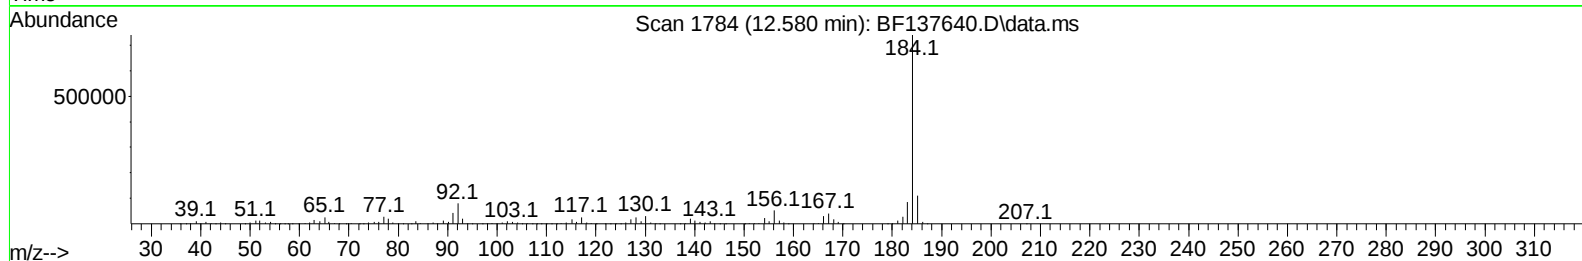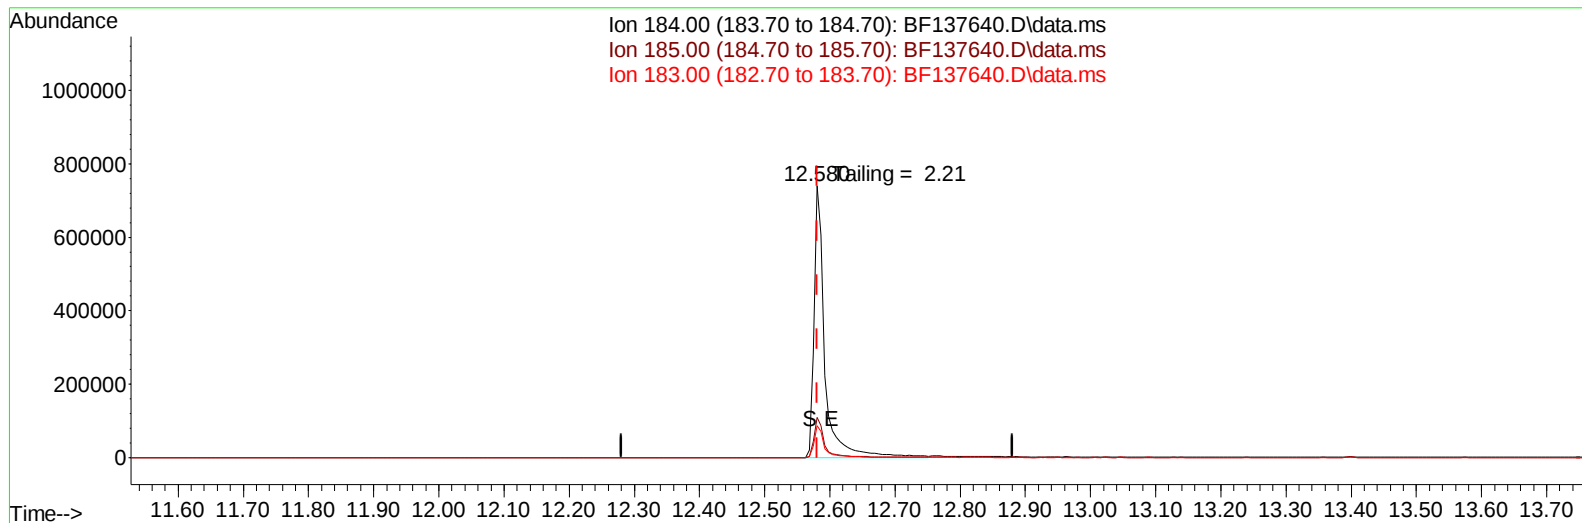

TIC: BF137640.D\data.ms

(77) Benzidine

12.580min (-0.000) 0.00 ng

response **852580**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.84
183.00	11.60	11.67
0.00	0.00	0.00