
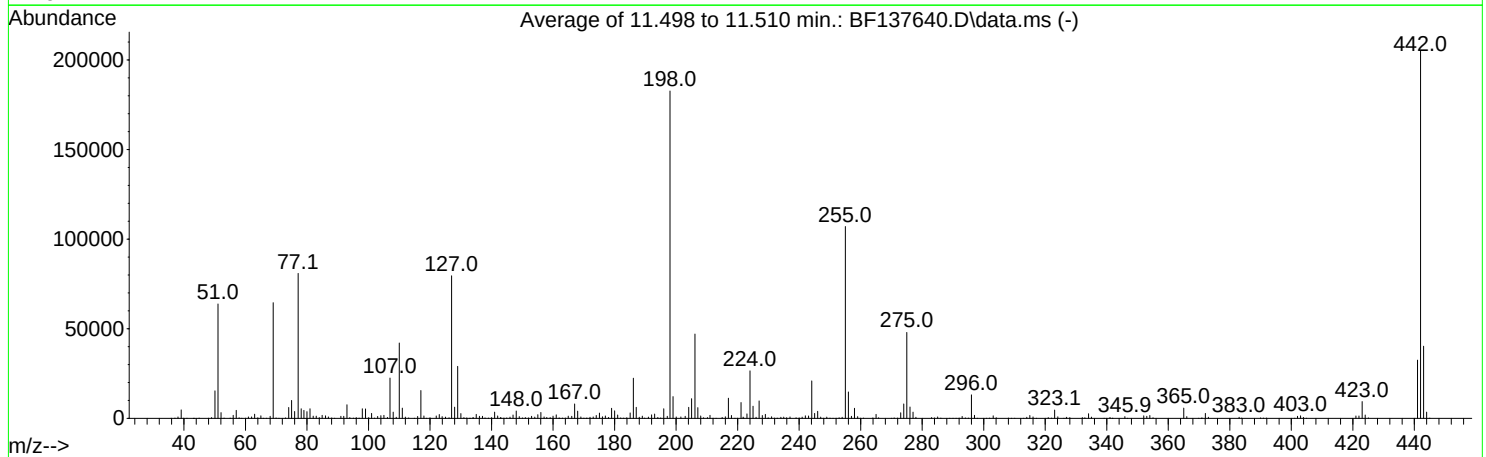


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031924\
Data File : BF137640.D
Acq On : 19 Mar 2024 11:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 14:45:20 2024

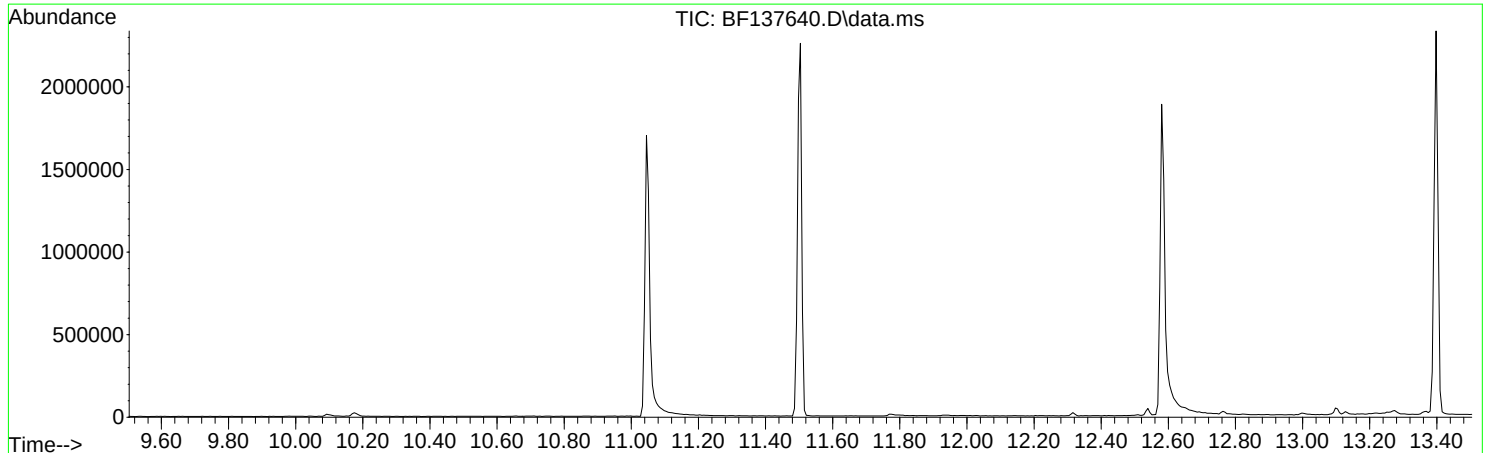




AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	63851	PASS
68	69	0.00	2	1.8	1149	PASS
69	198	0.00	100	35.4	64577	PASS
70	69	0.00	2	0.4	242	PASS
127	198	10	80	43.6	79555	PASS
197	198	0.00	2	0.6	1168	PASS
198	198	100	100	100.0	182603	PASS
199	198	5	9	6.6	12137	PASS
275	198	10	60	26.3	47976	PASS
365	198	1	100	3.1	5677	PASS
441	198	0.01	100	17.8	32517	PASS
442	442	50	100	100.0	205227	PASS
443	442	15	24	19.6	40283	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031924\
Data File : BF137640.D
Acq On : 19 Mar 2024 11:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 20 00:30:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 14:45:20 2024
Response via : Initial Calibration

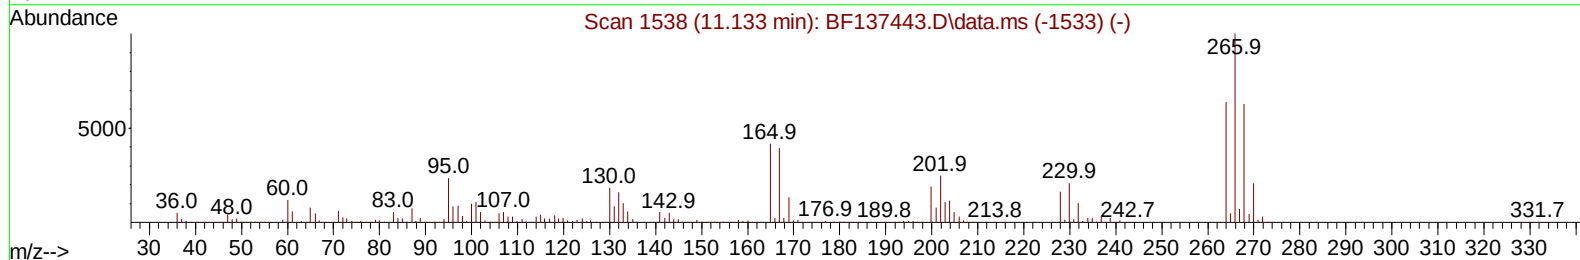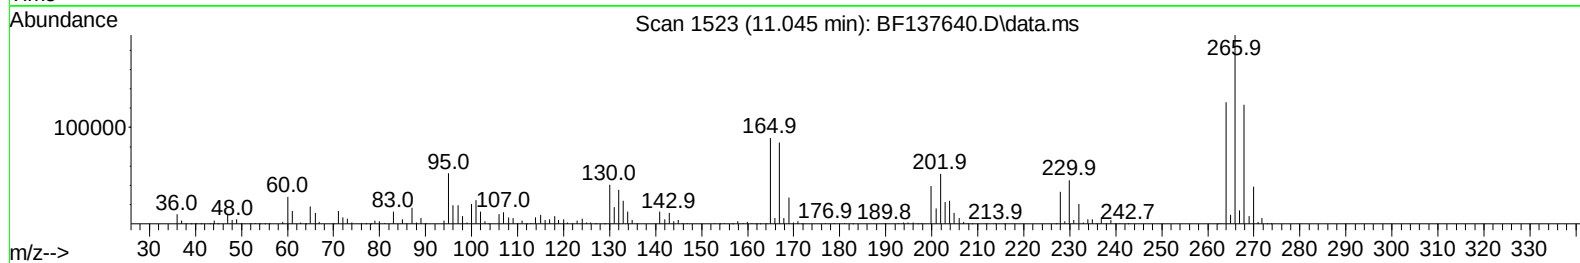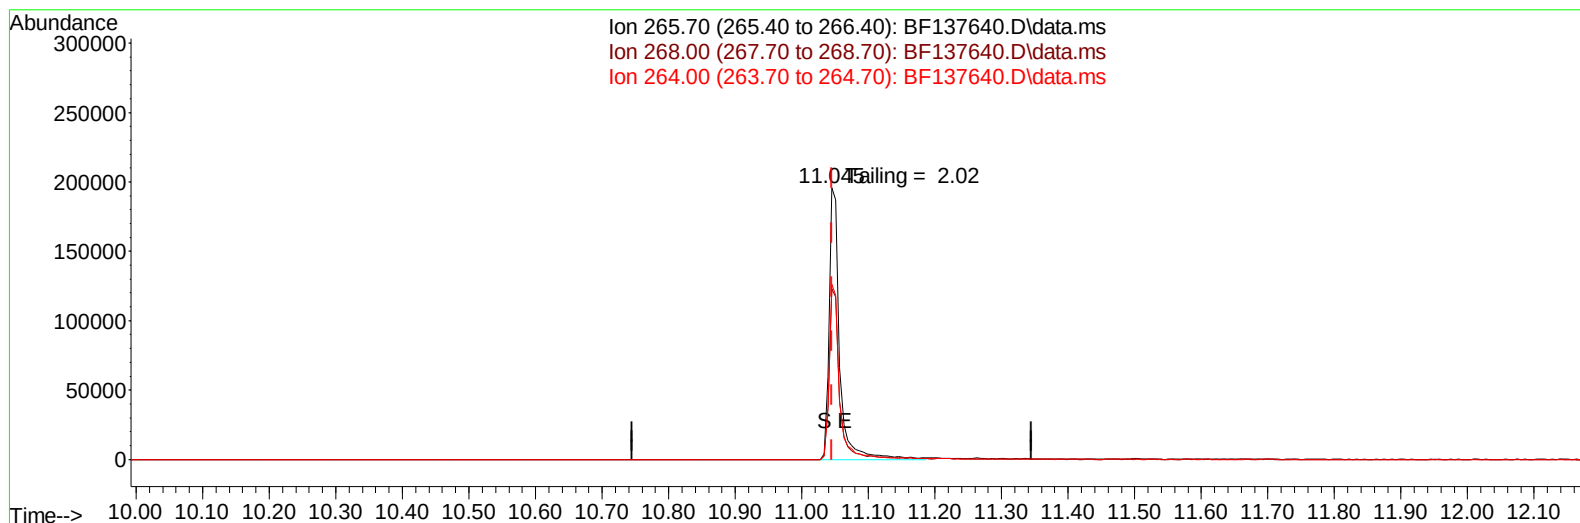

TIC: BF137640.D\data.ms

(70) Pentachlorophenol (C)

11.045min (-0.000) 41357.50 ng

response 215904

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.96
264.00	63.60	64.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/19/2024	BNA_F	<u>BF137640.D</u>
Compound Name	Response	Retention Time
DDT	368991	13.398
DDD	11418	13.104
DDE	2043	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13461	382452	3.52

Instrument :
BNA_F
ClientSampleId :
DFTPP