
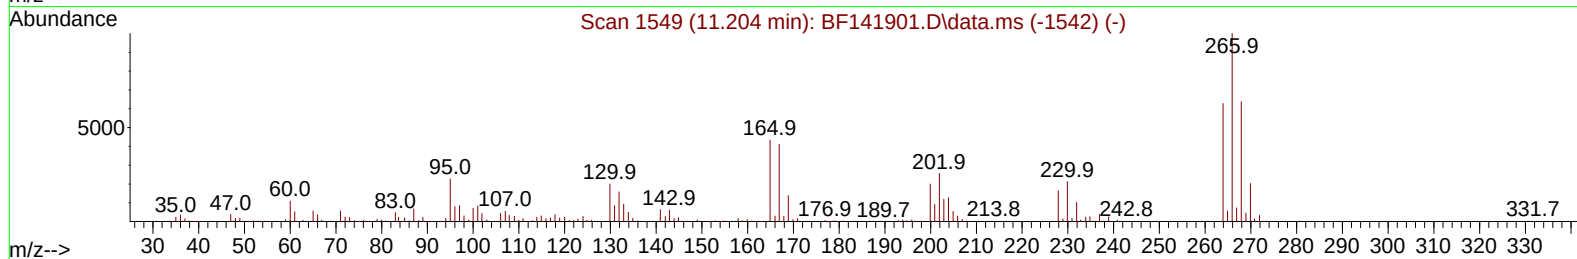
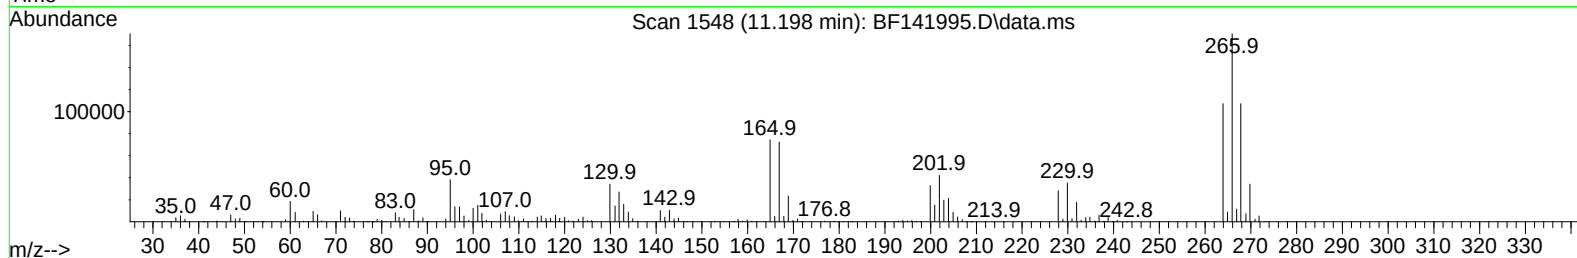


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031925\
Data File : BF141995.D
Acq On : 19 Mar 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 11:06:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

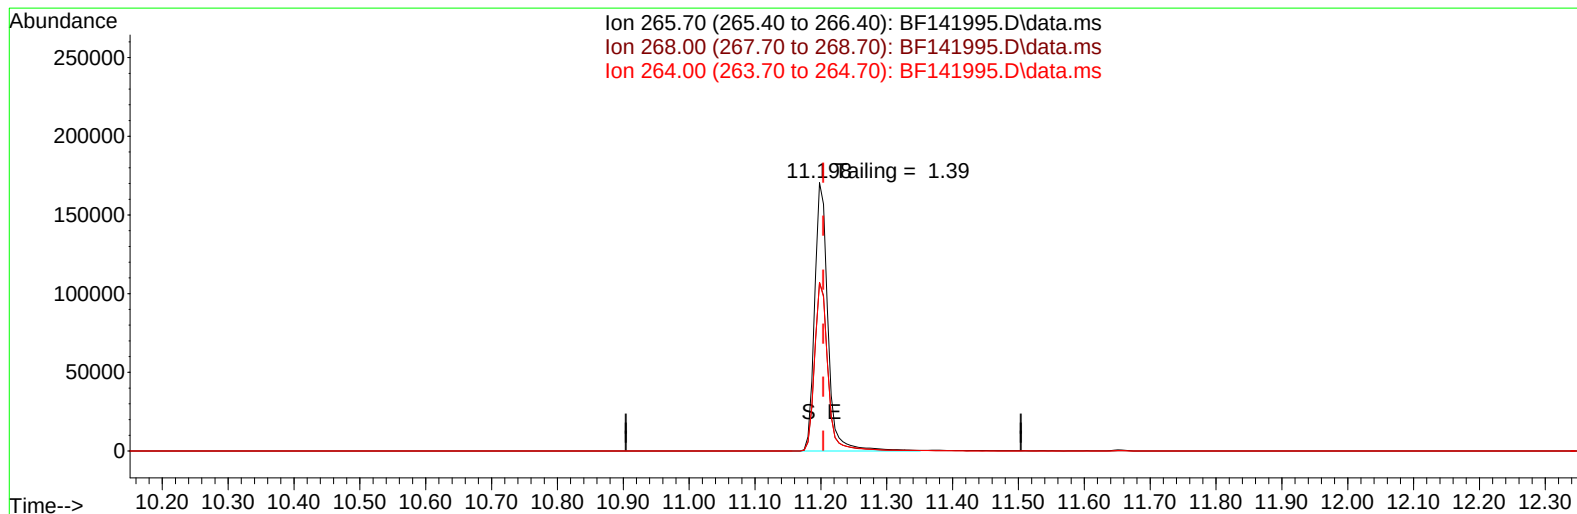

TIC: BF141995.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.006) 25049.43 ng

response 240010

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.86
264.00	62.70	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031925\
Data File : BF141995.D
Acq On : 19 Mar 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 19 11:06:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

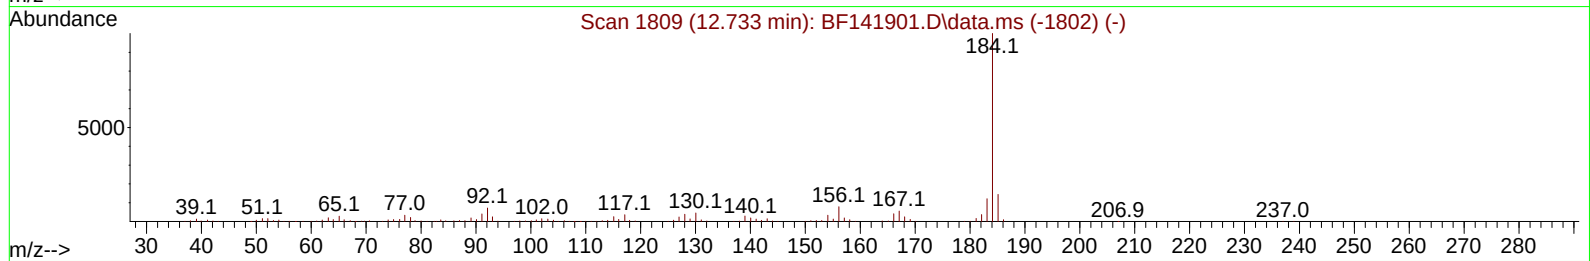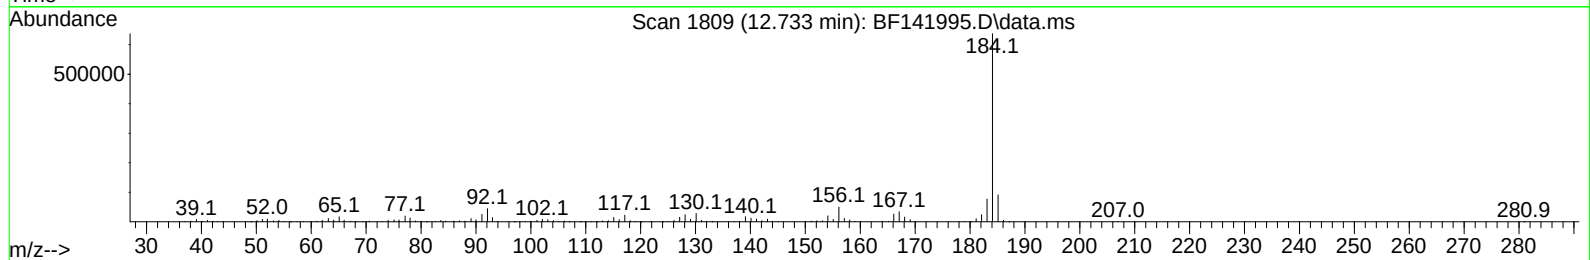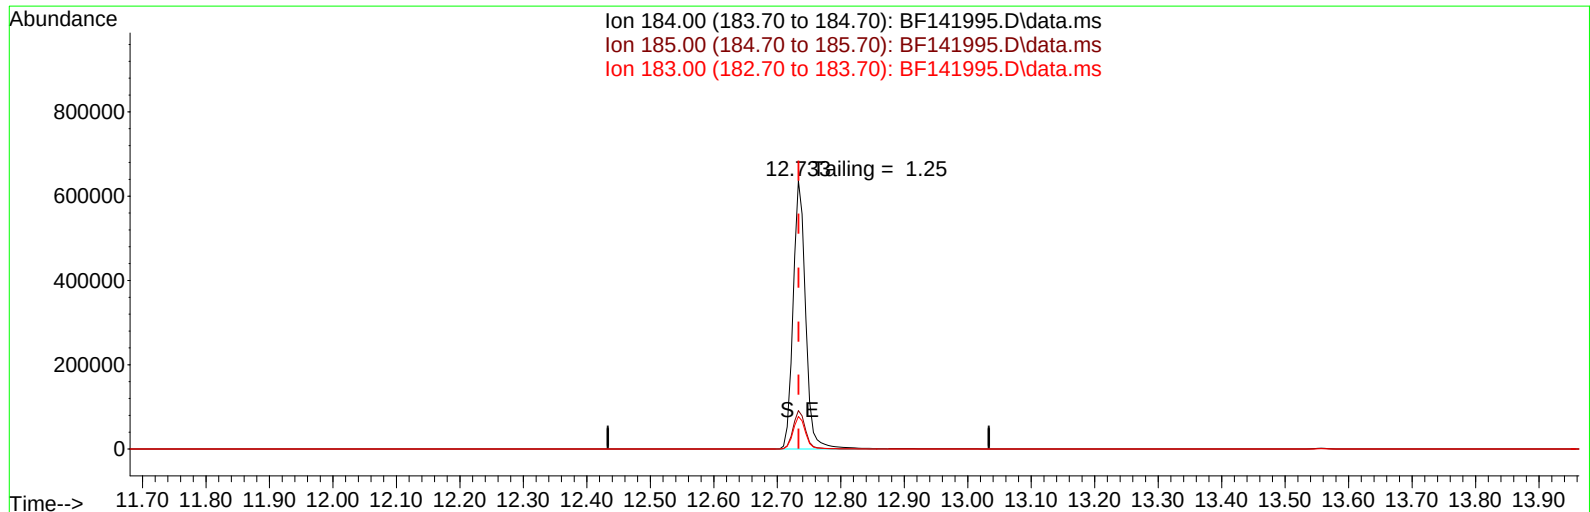

TIC: BF141995.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 0.00 ng

response 878029

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.31
183.00	12.10	12.12
0.00	0.00	0.00