
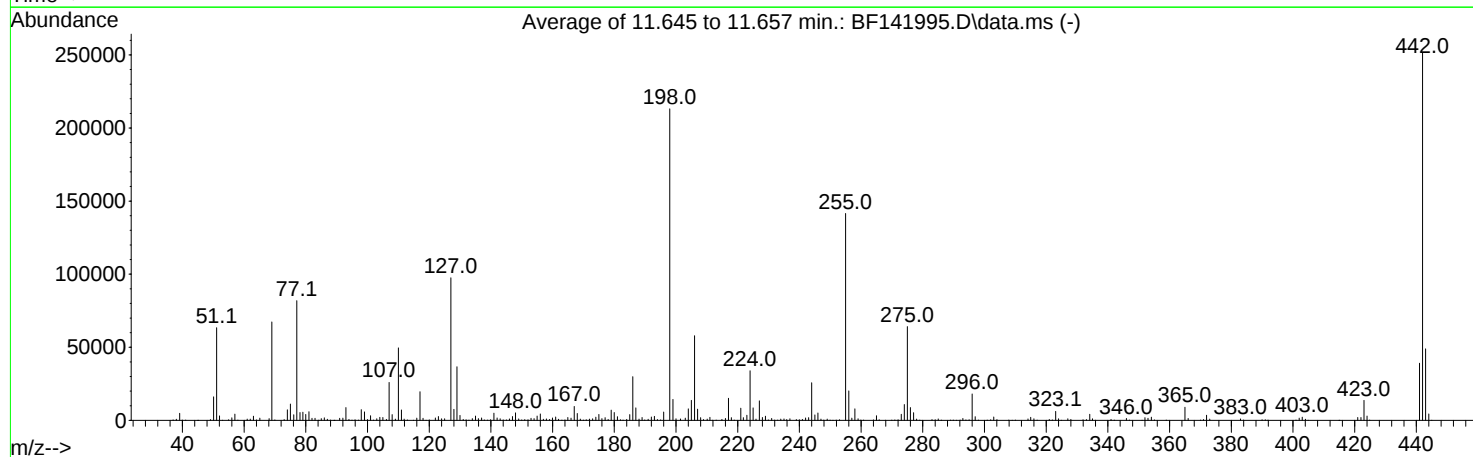


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031925\
Data File : BF141995.D
Acq On : 19 Mar 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

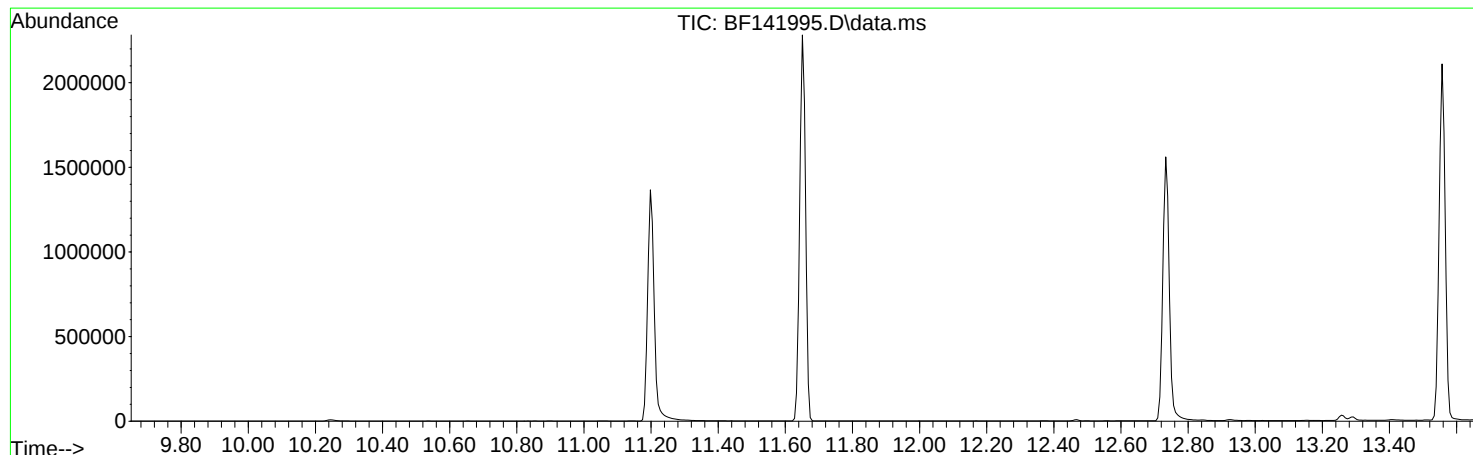

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	63333	PASS
68	69	0.00	2	1.9	1263	PASS
69	198	0.00	100	31.6	67357	PASS
70	69	0.00	2	0.4	298	PASS
127	198	10	80	45.8	97589	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	213099	PASS
199	198	5	9	6.7	14344	PASS
275	198	10	60	30.1	64112	PASS
365	198	1	100	4.2	8971	PASS
441	198	0.01	100	18.3	39096	PASS
442	442	50	100	100.0	251669	PASS
443	442	15	24	19.4	48896	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/19/2025	BNA_F	<u>BF141995.D</u>
Compound Name	Response	Retention Time
DDT	541725	13.557
DDD	15448	13.257
DDE	2115	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17563	559288	3.14

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031925\
Data File : BF141995.D
Acq On : 19 Mar 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 19 11:06:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

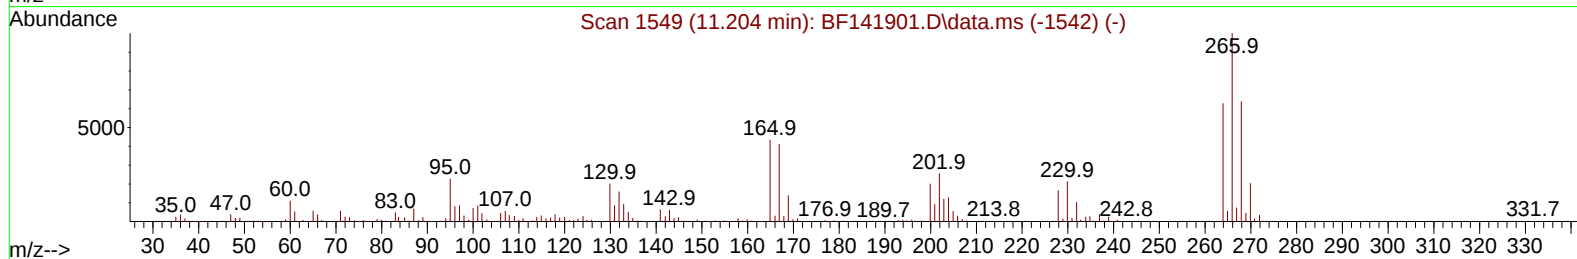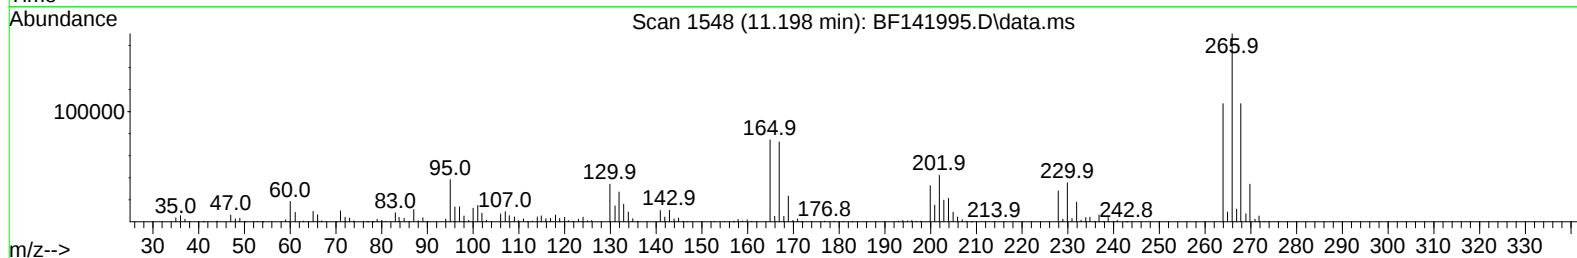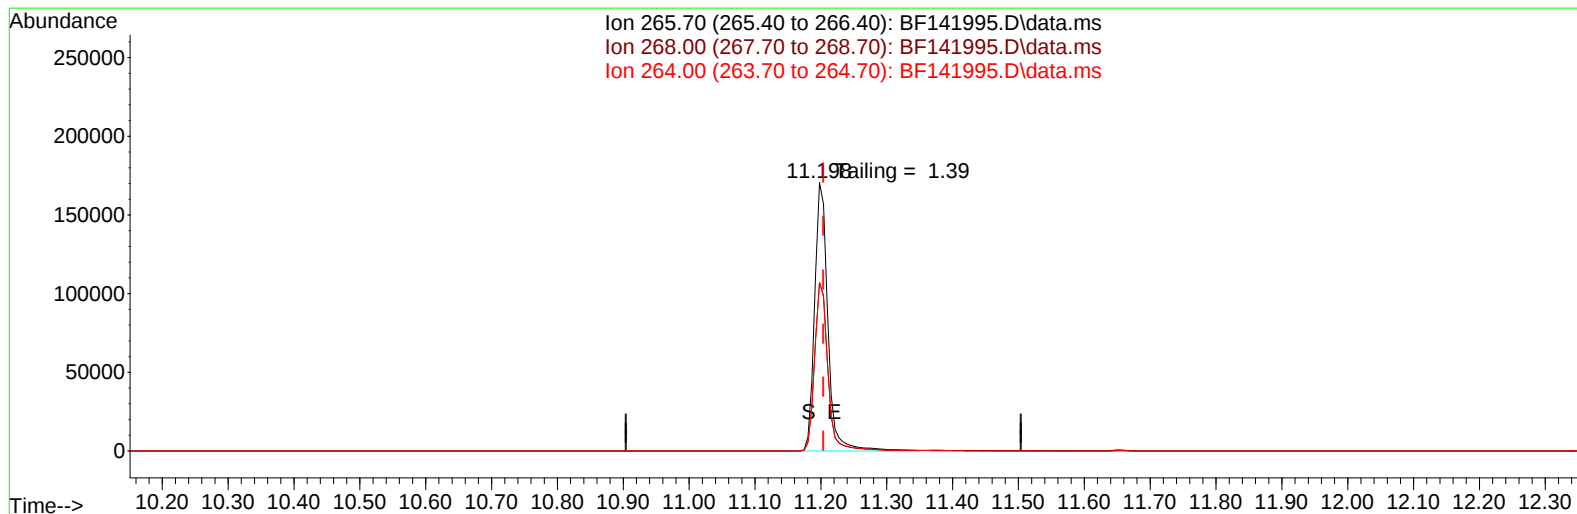

TIC: BF141995.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 25049.43 ng




response 240010

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.86
264.00	62.70	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031925\
Data File : BF141995.D
Acq On : 19 Mar 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 19 11:06:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

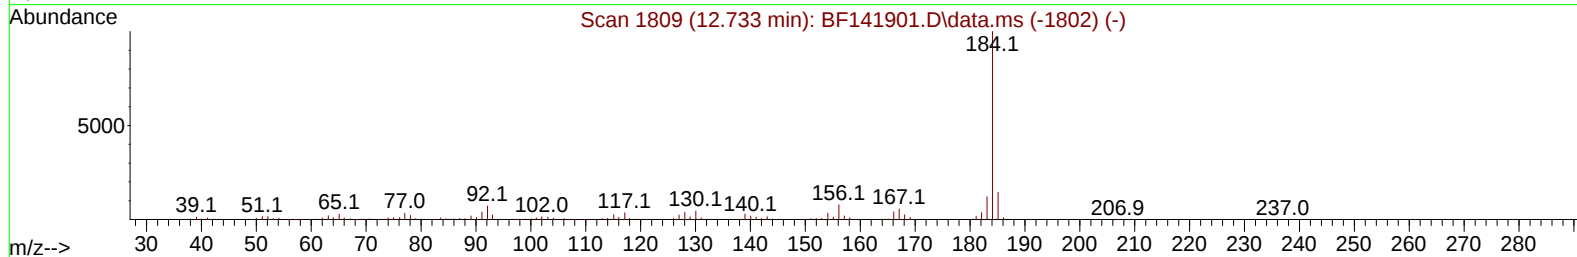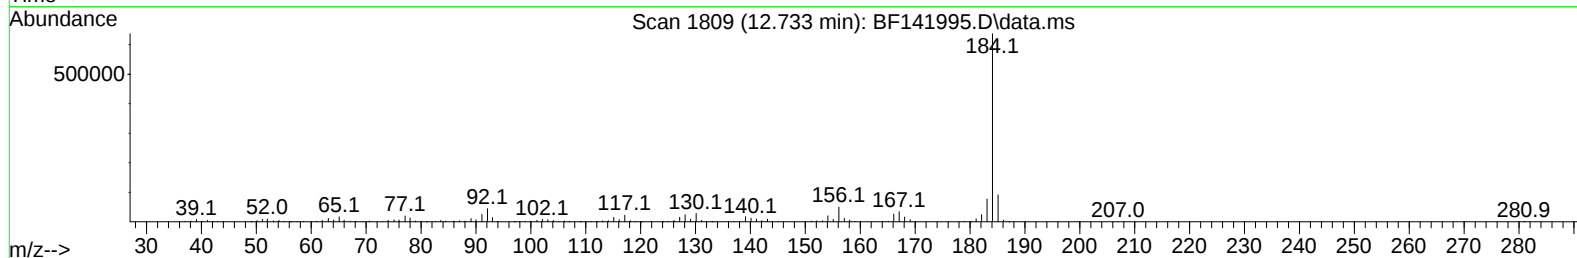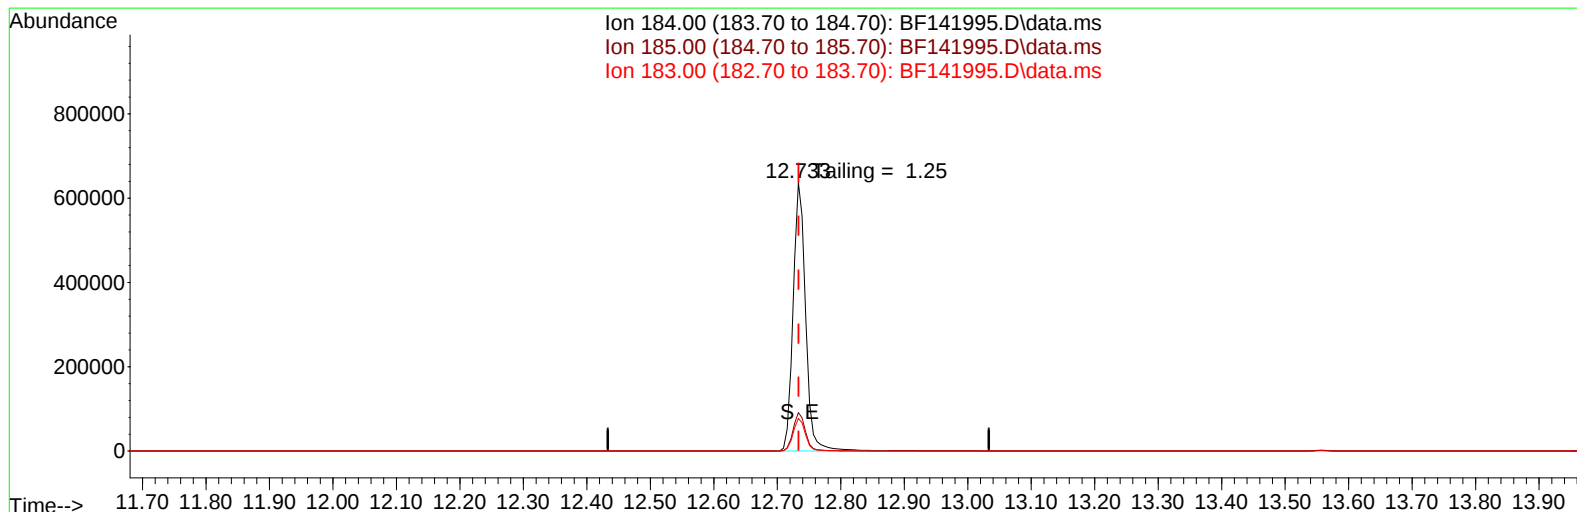

TIC: BF141995.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 0.00 ng

response 878029

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.31
183.00	12.10	12.12
0.00	0.00	0.00