


Data Path : Z:\HPCHEM1\BNA_F\Data\BF032015\
 Data File : BF077862.D
 Acq On : 20 Mar 2015 13:55
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 02:09:19 2015

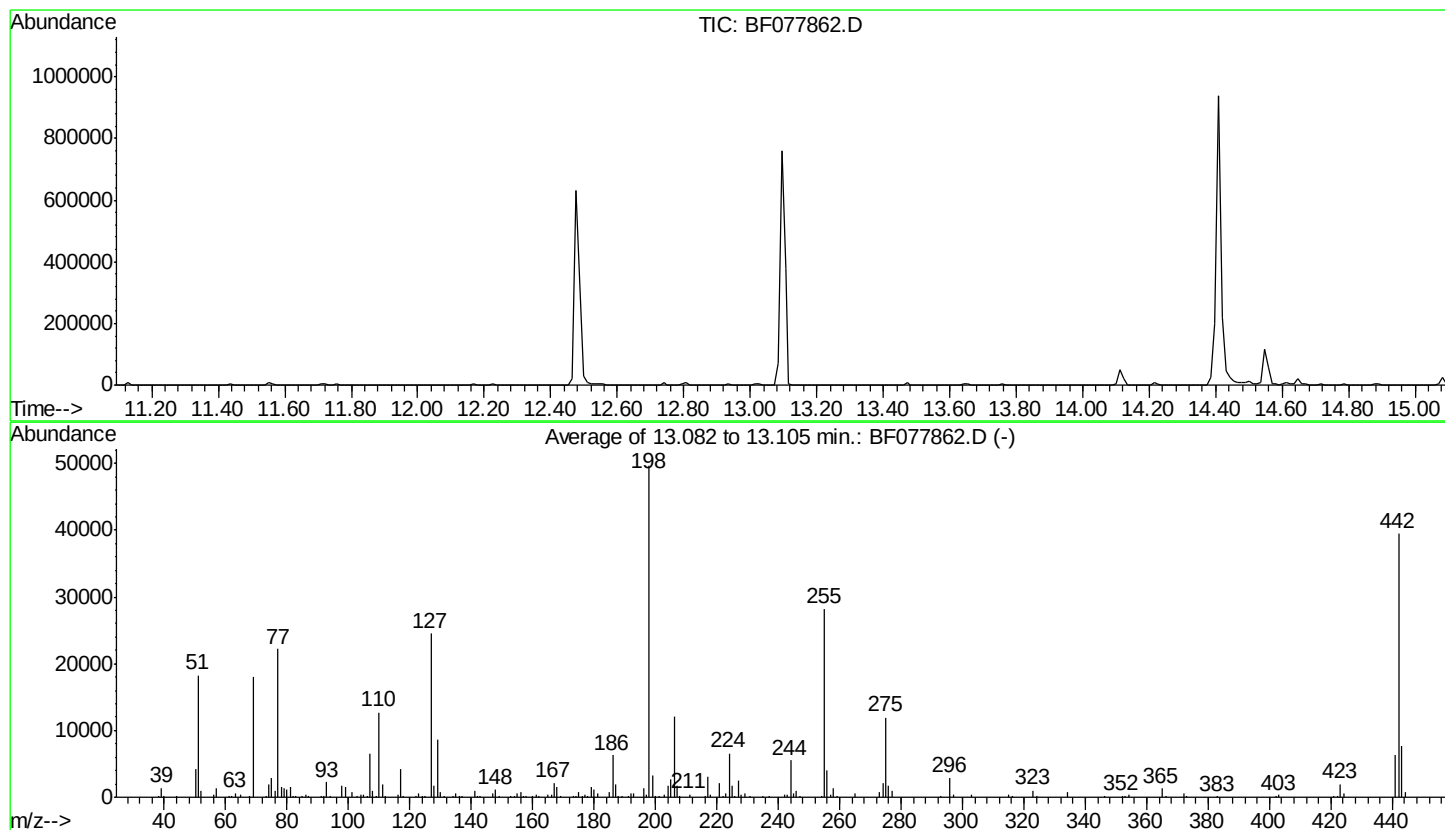

AutoFind: Scans 1067, 1068, 1069; Background Corrected with Scan 1064

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	18253	PASS
68	69	0.00	2	1.3	239	PASS
69	198	0.00	100	36.5	18118	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	24529	PASS
197	198	0.00	2	0.7	331	PASS
198	198	100	100	100.0	49685	PASS
199	198	5	9	6.8	3358	PASS
275	198	10	60	24.1	11974	PASS
365	198	1	100	2.7	1317	PASS
441	442	0.01	24	16.0	6296	PASS
442	198	50	100	79.4	39459	PASS
443	442	15	24	19.6	7733	PASS