

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
 Data File : BF077876.D
 Acq On : 20 Mar 2015 21:22
 Operator : TP/IZ
 Sample : G1575-11
 Misc : W
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-24V

Quant Time: Mar 21 01:08:59 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 20 23:52:05 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.13	152	45129	20.00	ng	0.00
21) Naphthalene-d8	8.70	136	183262	20.00	ng	0.00
38) Acenaphthene-d10	10.86	164	90470	20.00	ng	-0.01
63) Phenanthrene-d10	12.71	188	180765	20.00	ng	-0.01
75) Chrysene-d12	15.99	240	190518	20.00	ng	-0.02
86) Perylene-d12	17.72	264	182867	20.00	ng	-0.11
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	58873	22.77	ng	0.00
7) Phenol-d6	6.70	99	56657	17.74	ng	0.00
23) Nitrobenzene-d5	7.81	82	81684	29.22	ng	-0.01
41) 2,4,6-Tribromophenol	11.85	330	36349	41.99	ng	-0.01
44) 2-Fluorobiphenyl	10.05	172	184214	29.92	ng	0.00
78) Terphenyl-d14	14.71	244	236627	30.34	ng	0.00
Target Compounds						
10) Phenol	6.72	94	36714	9.72	ng	Qvalue # 71
32) Benzoic acid	8.41	122	24680	18.50	ng	98
49) Dimethylphthalate	10.56	163	22774	3.39	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V

Quant Time: Mar 21 01:08:59 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 20 23:52:05 2015
Response via : Initial Calibration

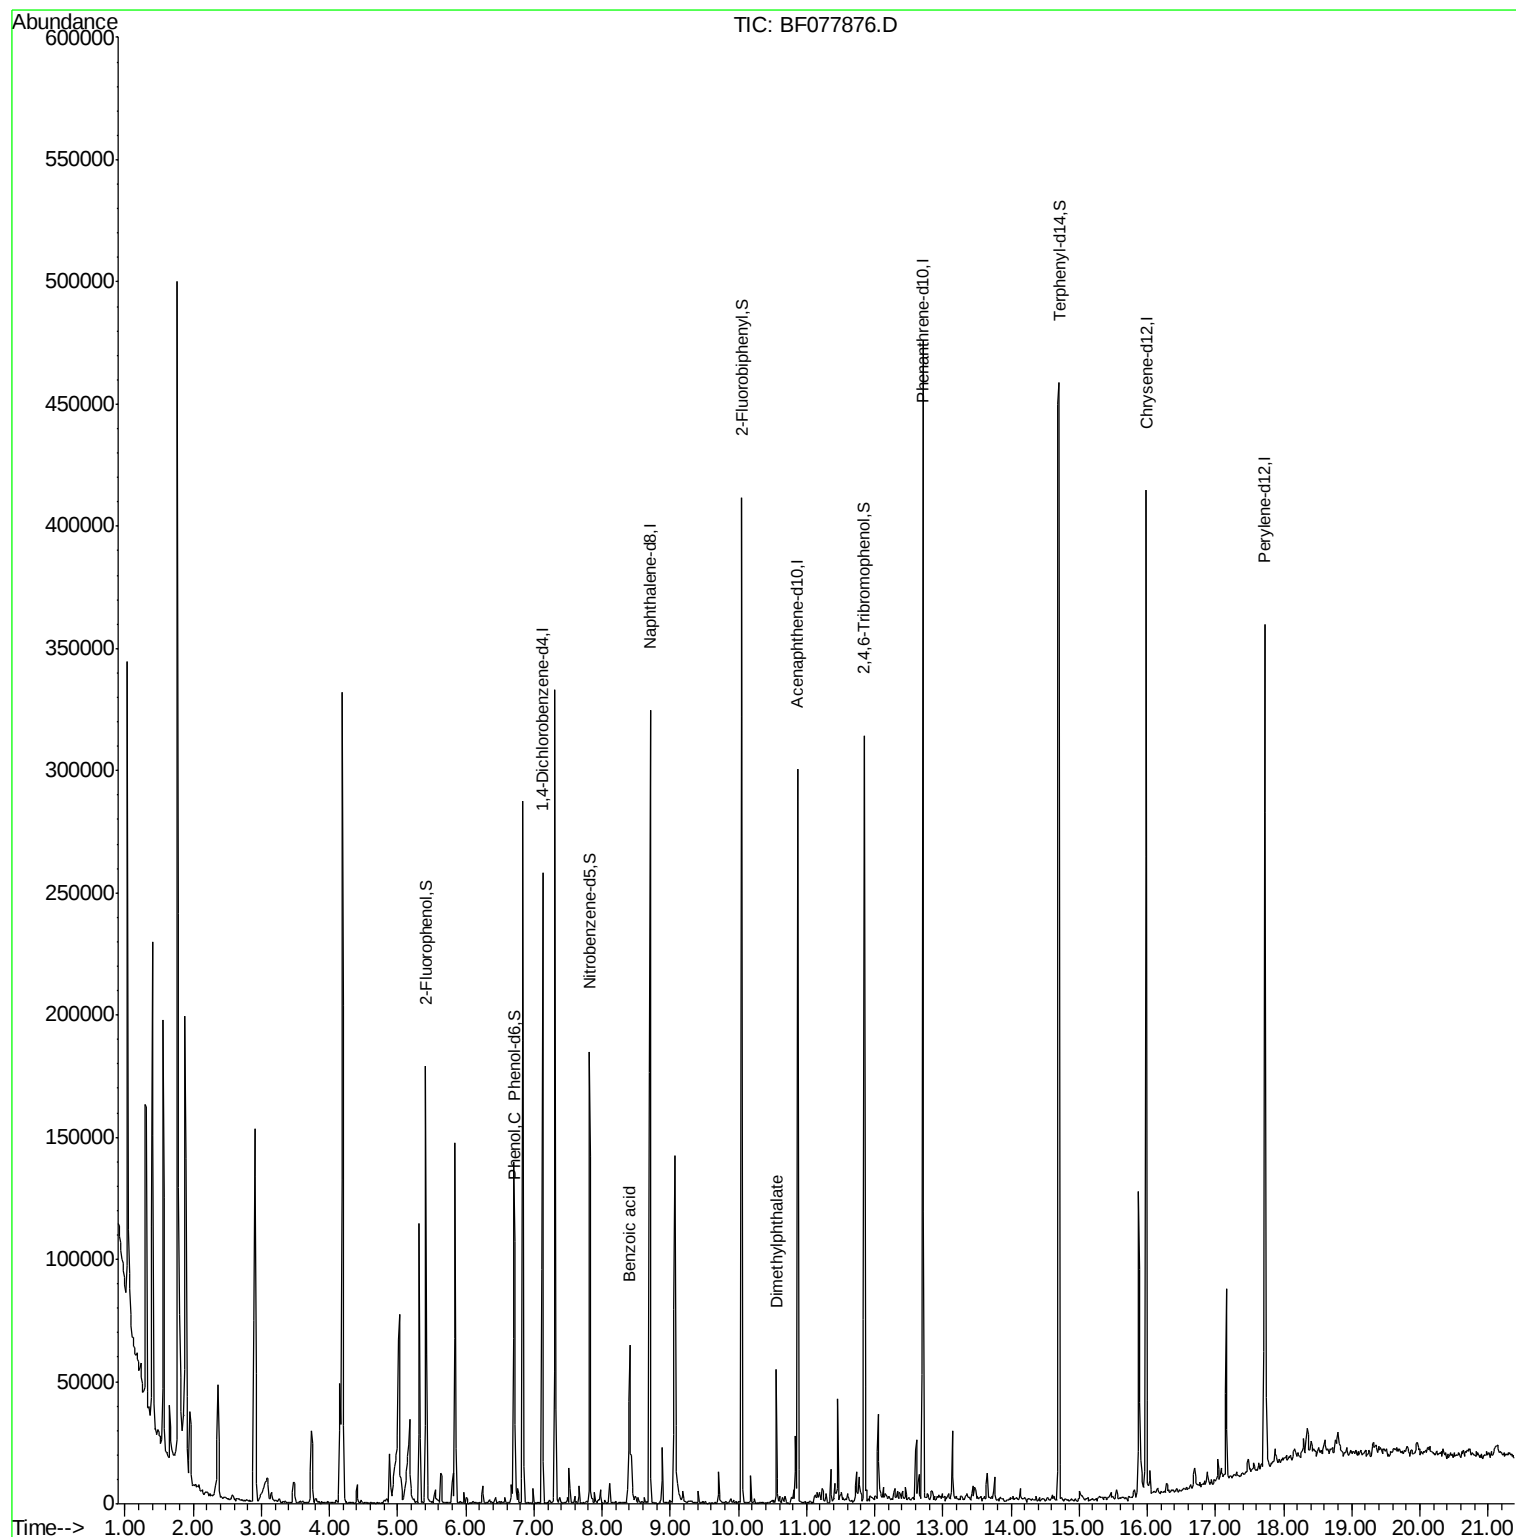

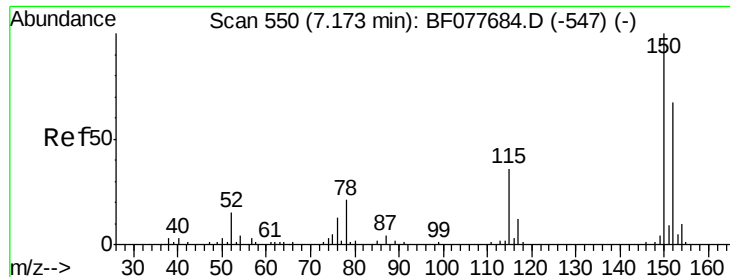

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.13 min Scan# 546

Delta R.T. -0.00 min

Lab File: BF077876.D

Acq: 20 Mar 2015 21:22

Instrument :

BNA_F

ClientSampleId :

MW-24V


Tot Ion:152 Resp: 45129

Ion Ratio Lower Upper

152 100

150 156.8 119.5 179.3




115 53.6 43.0 64.4

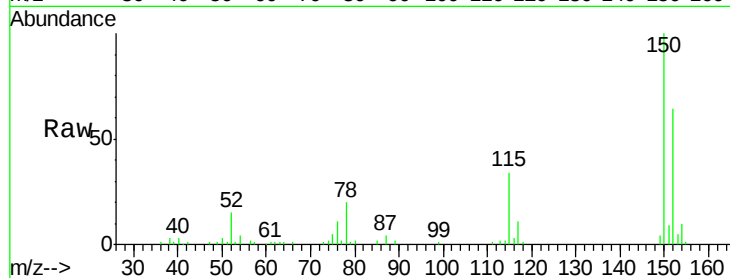

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

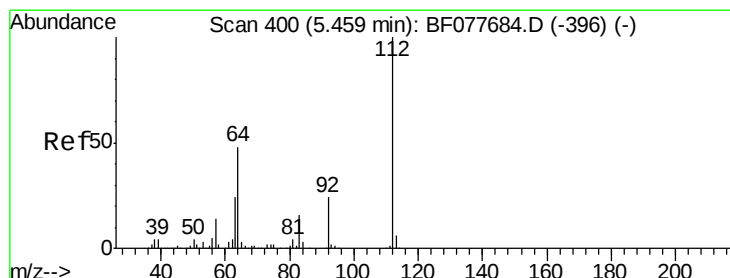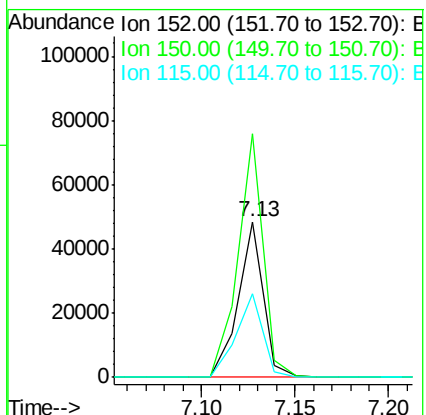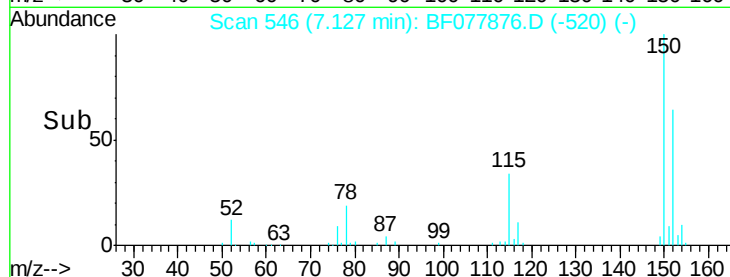

#5

2-Fluorophenol

Concen: 22.77 ng

RT: 5.41 min Scan# 396

Delta R.T. -0.00 min

Lab File: BF077876.D

Acq: 20 Mar 2015 21:22


Tgt Ion:112 Resp: 58873

Ion Ratio Lower Upper

112 100

64 55.2 38.6 57.8



63 28.0 19.3 28.9

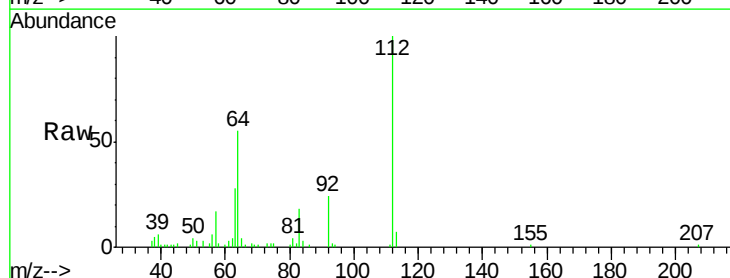


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

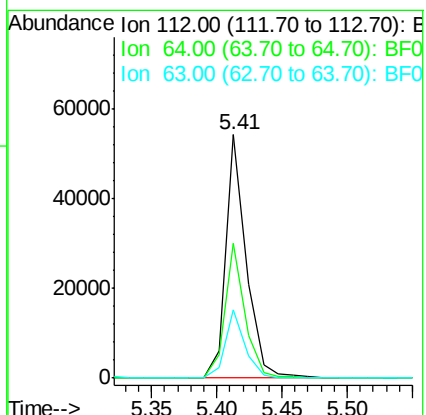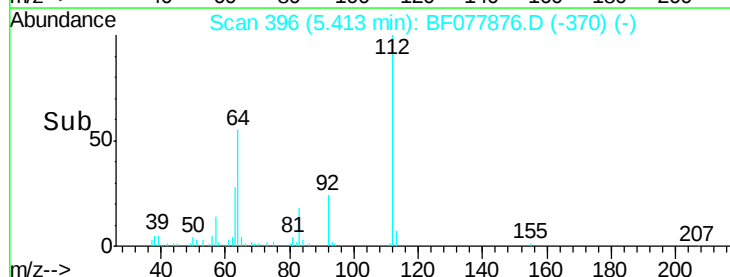

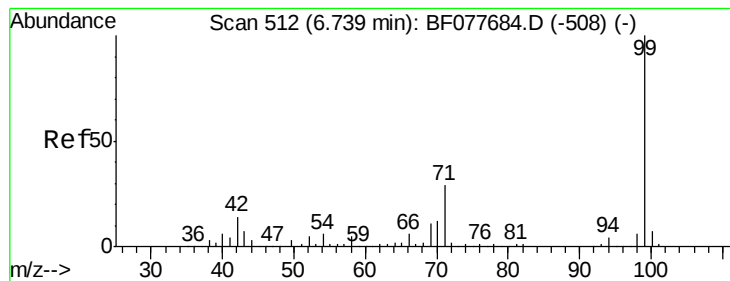

#7

Phenol-d6

Concen: 17.74 ng

RT: 6.70 min Scan# 509

Delta R.T. -0.00 min

Lab File: BF077876.D

Acq: 20 Mar 2015 21:22

Instrument :

BNA_F

ClientSampleId :

MW-24V


Tot Ion: 99 Resp: 56657

Ion Ratio Lower Upper

99 100

42 14.8 11.0 16.4




71 28.3 23.4 35.2

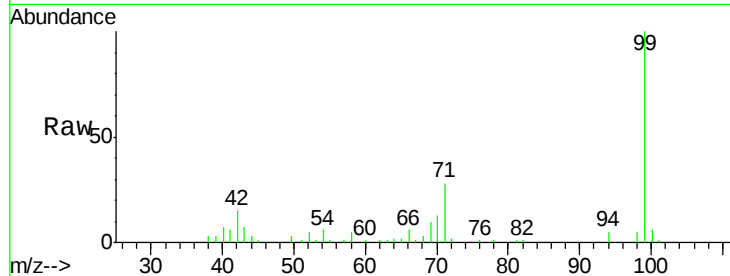

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

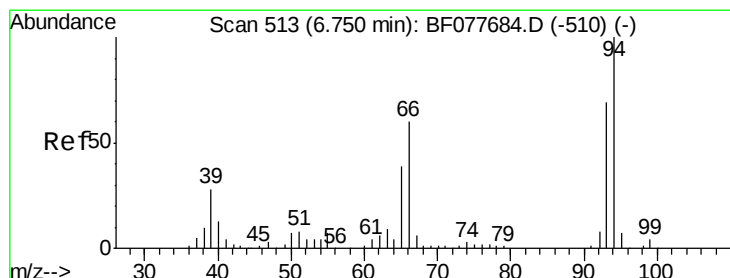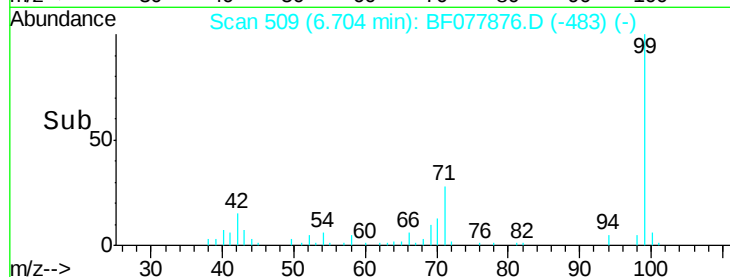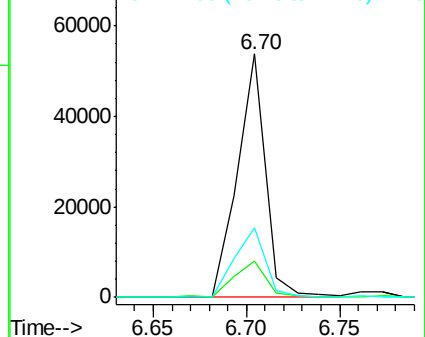

#10

Phenol

Concen: 9.72 ng

RT: 6.72 min Scan# 510

Delta R.T. -0.00 min

Lab File: BF077876.D

Acq: 20 Mar 2015 21:22


Tgt Ion: 94 Resp: 36714

Ion Ratio Lower Upper

94 100

65 25.6 18.8 58.8



66 34.3 39.9 79.9#

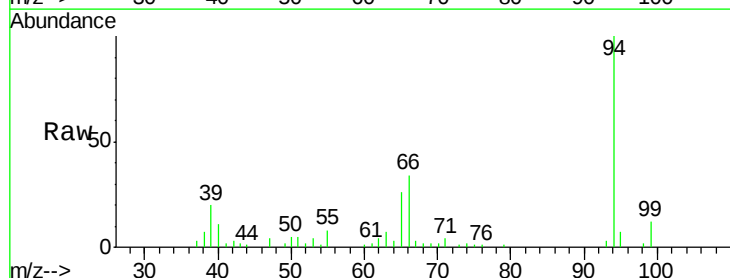


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

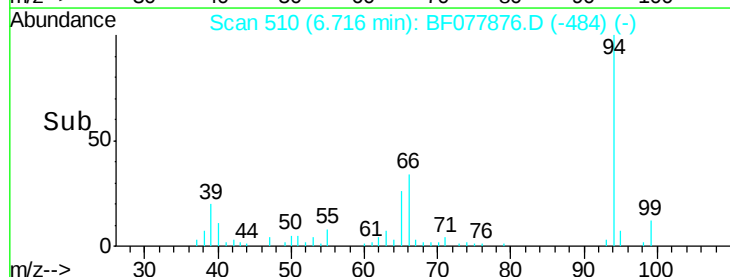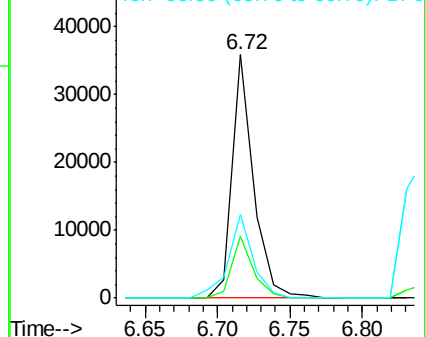


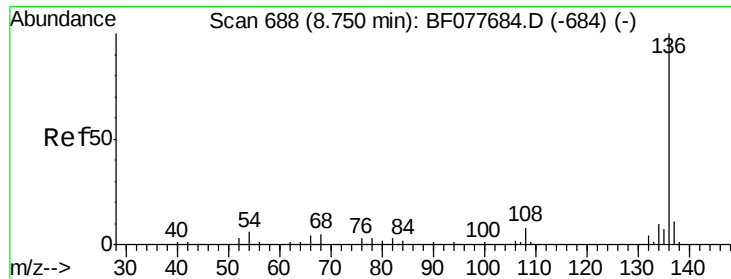




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.70 min Scan# 684
Delta R.T. -0.00 min
Lab File: BF077876.D
Acq: 20 Mar 2015 21:22

Instrument :
BNA_F
ClientSampleId :
MW-24V

Tot Ion:	136	Resp:	183262
Ion	Ratio	Lower	Upper
136	100		
137	10.0	8.7	13.1
54	5.4	4.6	6.8
68	4.2	3.7	5.5

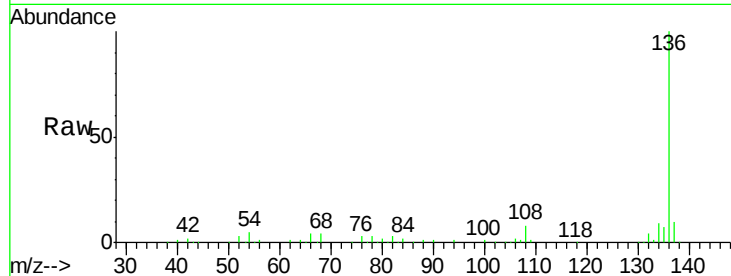


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

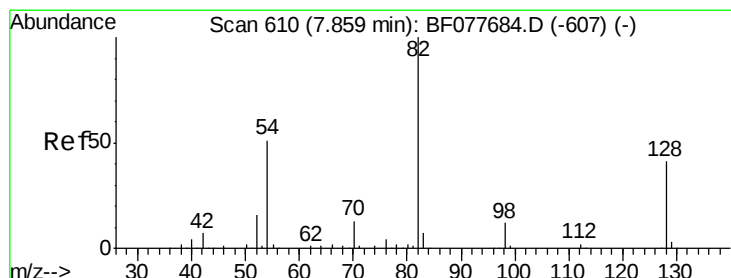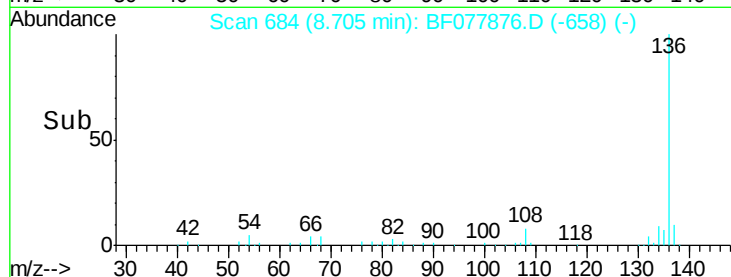
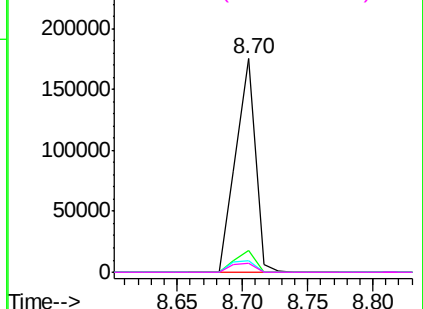



#23
Nitrobenzene-d5
Concen: 29.22 ng
RT: 7.81 min Scan# 606
Delta R.T. -0.01 min
Lab File: BF077876.D
Acq: 20 Mar 2015 21:22

Tgt Ion:	82	Resp:	81684
Ion	Ratio	Lower	Upper
82	100		
128	35.2	32.8	49.2
54	51.9	40.6	60.8

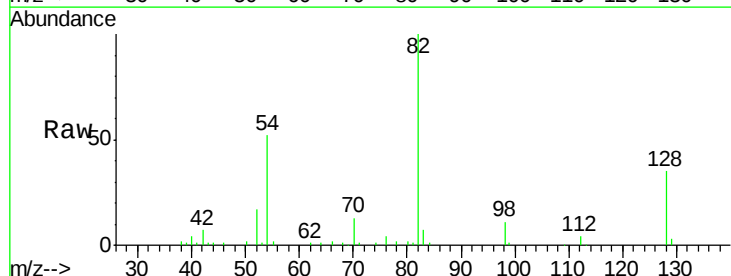

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

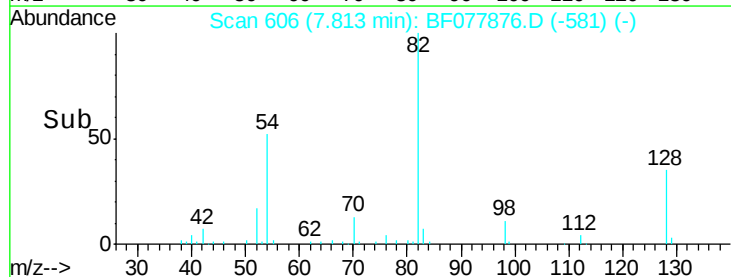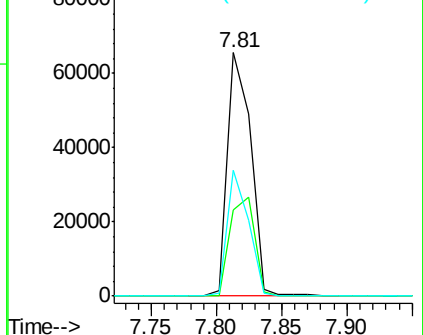


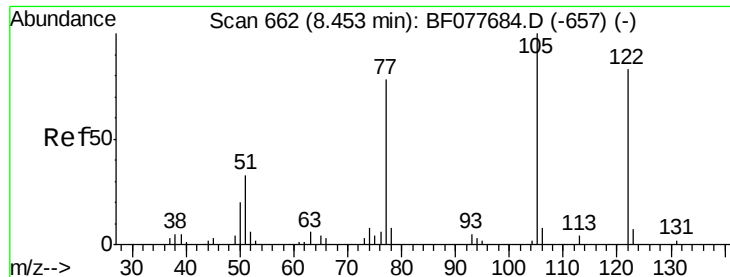




#32
Benzoic acid
Concen: 18.50 ng
RT: 8.41 min Scan# 658
Delta R.T. -0.02 min
Lab File: BF077876.D
Acq: 20 Mar 2015 21:22

Instrument :
BNA_F
ClientSampleId :
MW-24V

Tot Ion:122 Resp: 24680
Ion Ratio Lower Upper
122 100
105 118.9 99.9 139.9
77 89.7 73.7 113.7

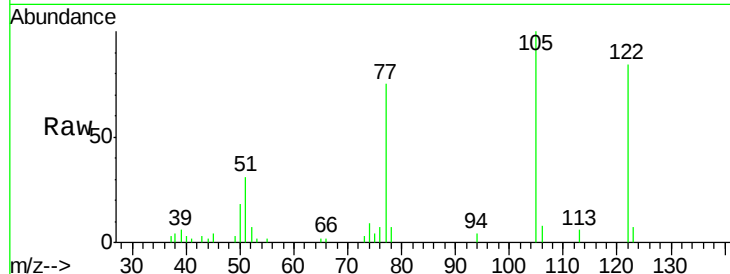


Abundance Ion 122.00 (121.70 to 122.70): E
Ion 105.00 (104.70 to 105.70): E
Ion 77.00 (76.70 to 77.70): BF0

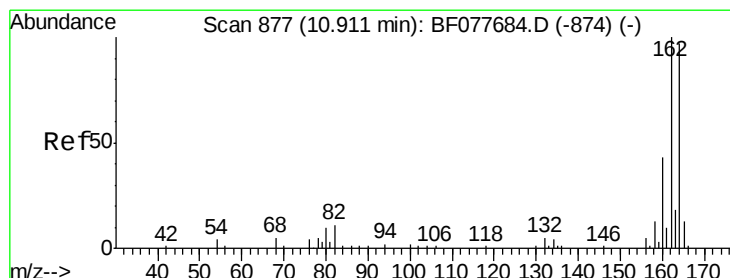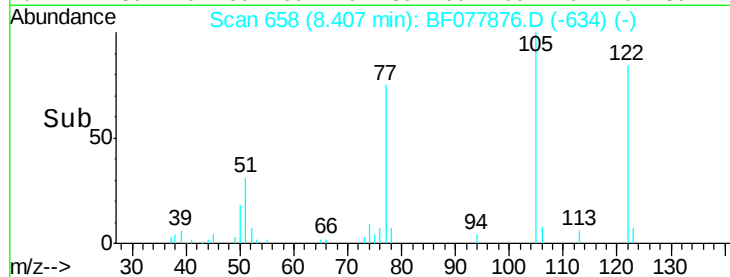
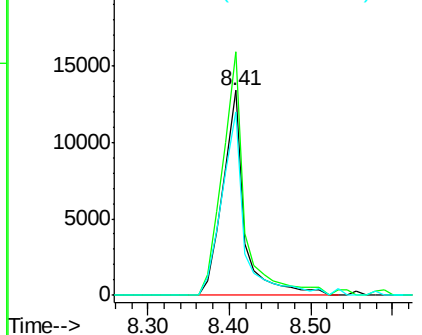


#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 10.86 min Scan# 873
Delta R.T. -0.01 min
Lab File: BF077876.D
Acq: 20 Mar 2015 21:22

Tgt Ion:164 Resp: 90470
Ion Ratio Lower Upper
164 100
162 104.0 82.4 123.6
160 43.7 35.8 53.6

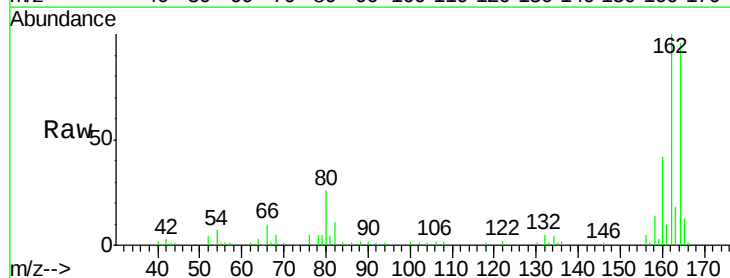

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E



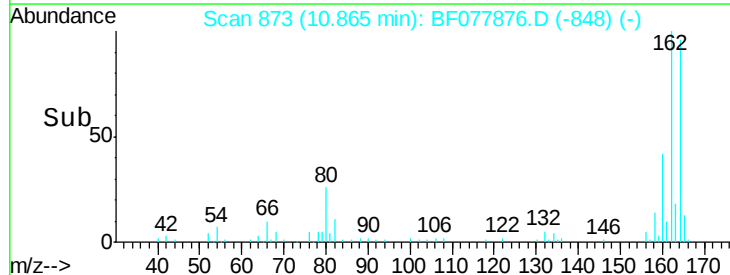
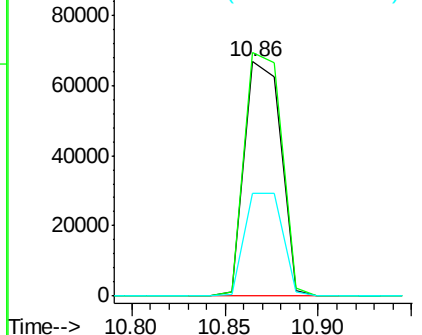




#41
 2,4,6-Tribromophenol
 Concen: 41.99 ng
 RT: 11.85 min Scan# 959
 Delta R.T. -0.01 min
 Lab File: BF077876.D
 Acq: 20 Mar 2015 21:22




Instrument :
 BNA_F
 ClientSampled :
 MW-24V


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	0.0	0.0#
141	38.1	0.0	0.0#

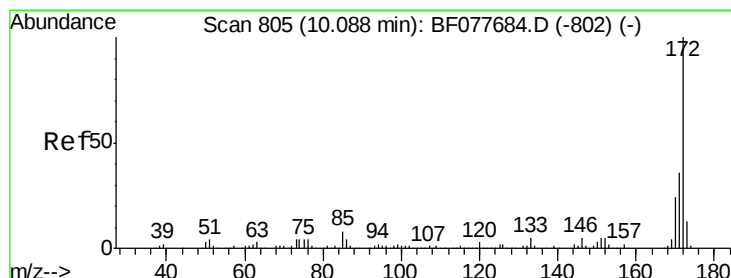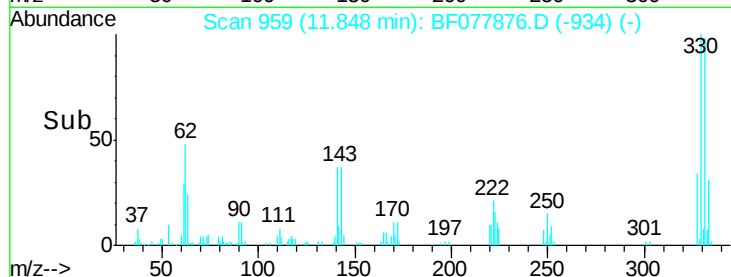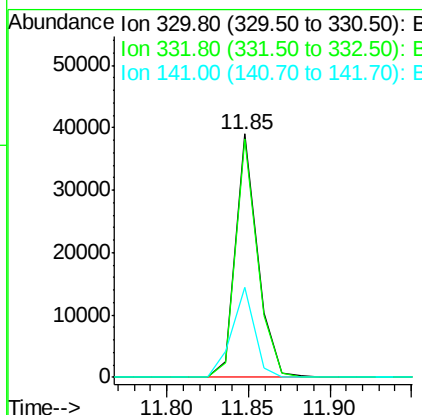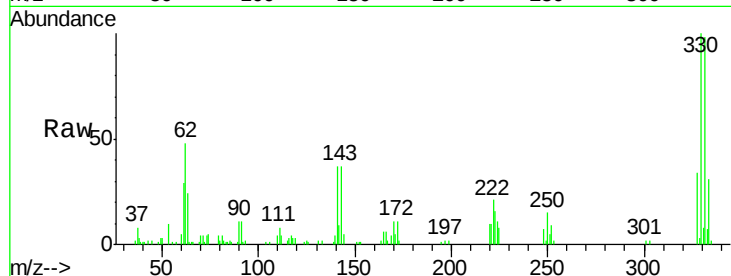

#44
 2-Fluorobiphenyl
 Concen: 29.92 ng
 RT: 10.05 min Scan# 802
 Delta R.T. -0.00 min
 Lab File: BF077876.D
 Acq: 20 Mar 2015 21:22

Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.9	28.5	42.7
170	22.0	18.8	28.2

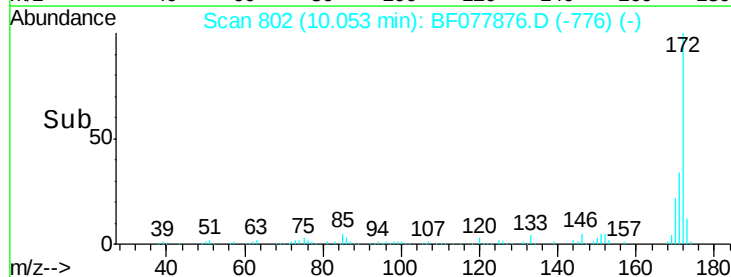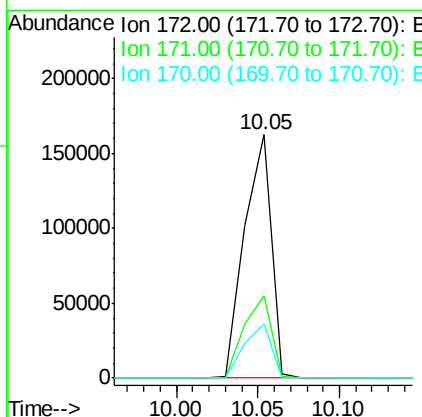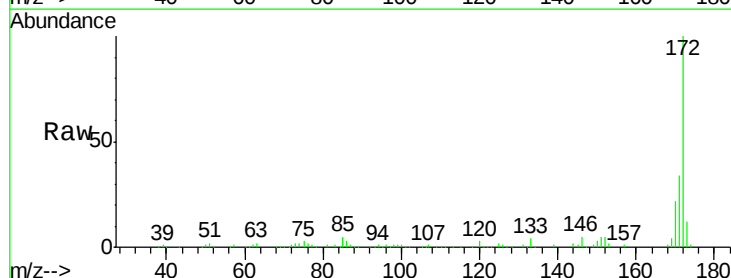

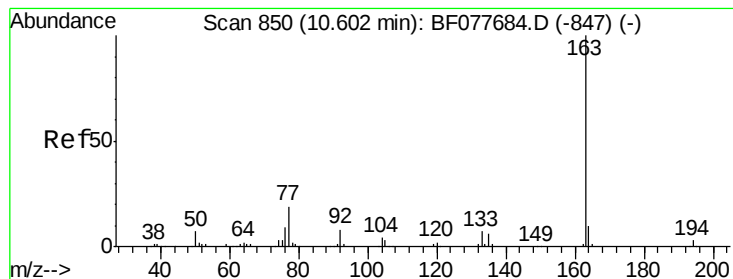

#49

Dimethylphthalate

Concen: 3.39 ng

RT: 10.56 min Scan# 846

Delta R.T. -0.01 min

Lab File: BF077876.D

Acq: 20 Mar 2015 21:22

Instrument :

BNA_F

ClientSampleId :

MW-24V


Tot Ion:163 Resp: 22774

Ion Ratio Lower Upper

163 100

194 3.9 2.7 4.1




164 10.6 8.2 12.2

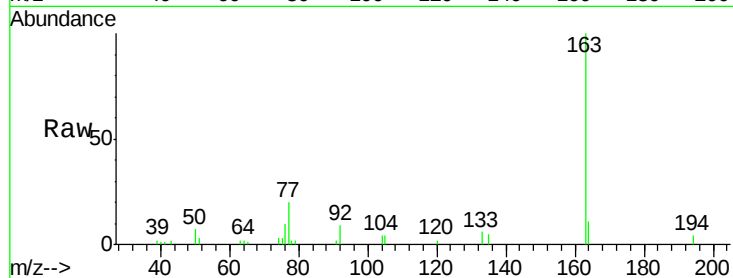

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

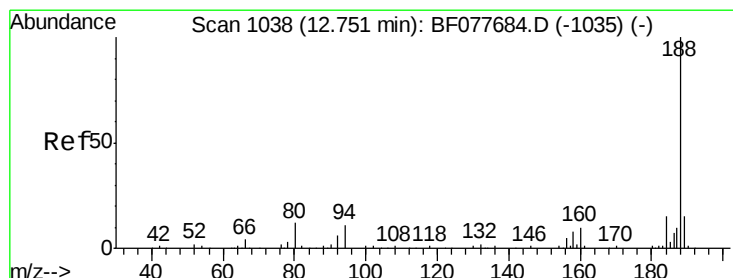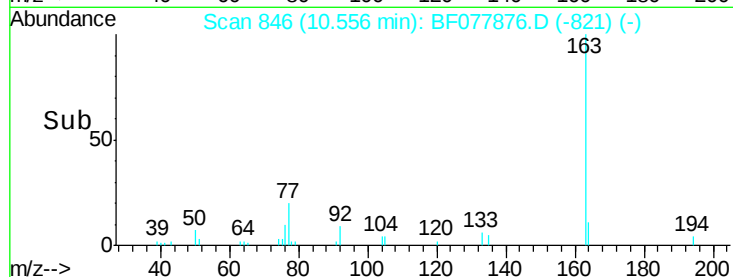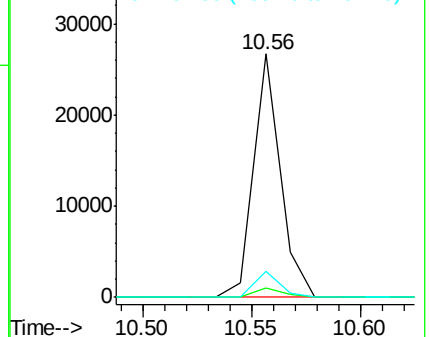

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 12.71 min Scan# 1034

Delta R.T. -0.01 min

Lab File: BF077876.D

Acq: 20 Mar 2015 21:22


Tgt Ion:188 Resp: 180765

Ion Ratio Lower Upper

188 100

94 10.9 8.7 13.1



80 11.4 9.3 13.9

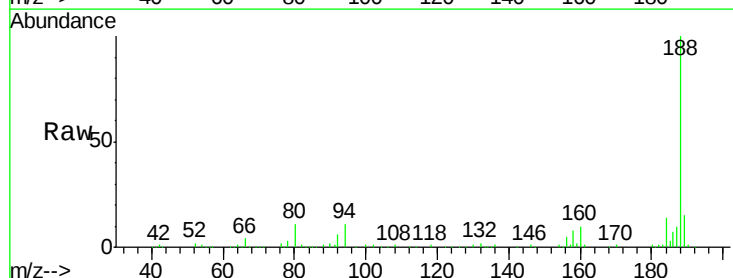


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



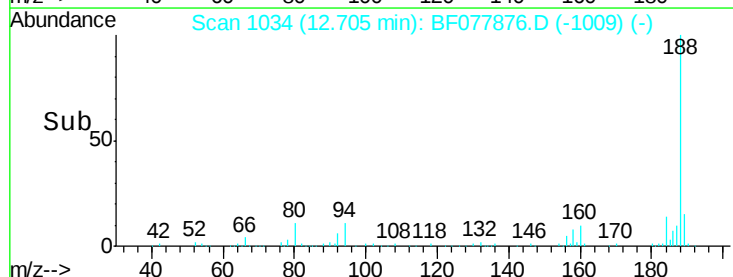
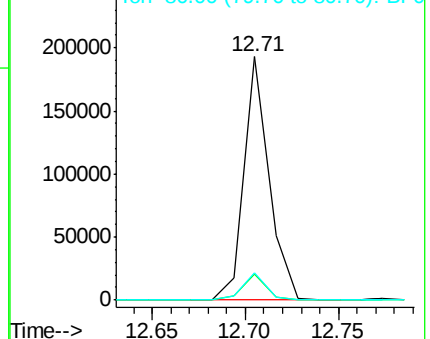


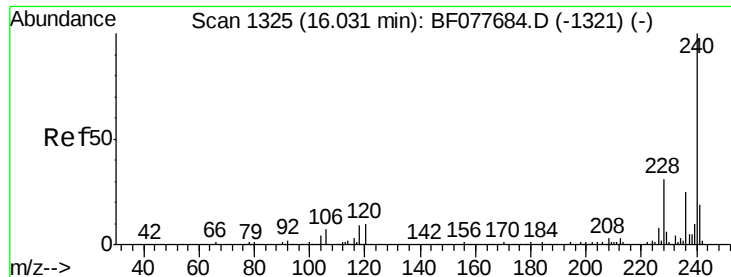

#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.99 min Scan# 1321
Delta R.T. -0.02 min
Lab File: BF077876.D
Acq: 20 Mar 2015 21:22




Instrument :
BNA_F
ClientSampleId :
MW-24V


Tot Ion:240 Resp: 190518
Ion Ratio Lower Upper
240 100
120 9.7 8.2 12.2
236 25.5 20.0 30.0

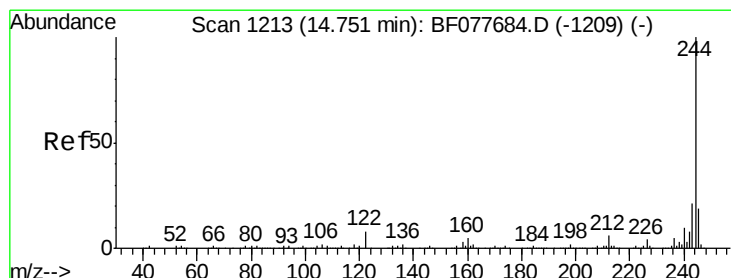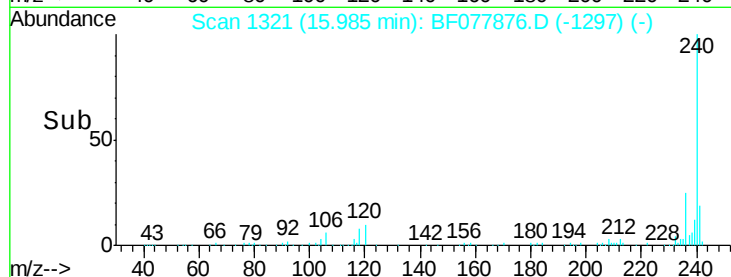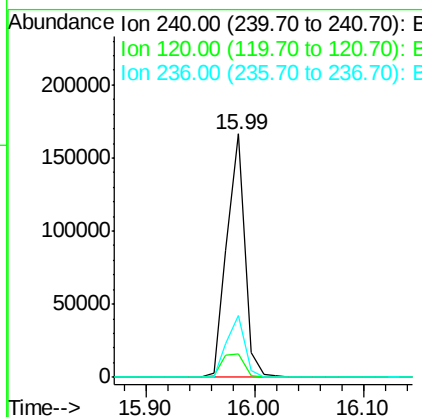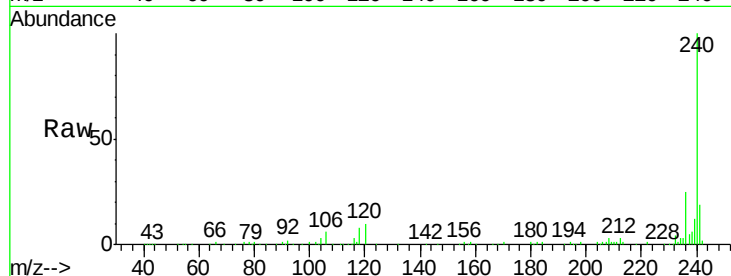

#78
Terphenyl-d14
Concen: 30.34 ng
RT: 14.71 min Scan# 1209
Delta R.T. -0.00 min
Lab File: BF077876.D
Acq: 20 Mar 2015 21:22

Tgt Ion:244 Resp: 236627
Ion Ratio Lower Upper
244 100
212 5.6 4.9 7.3
122 7.7 6.2 9.4

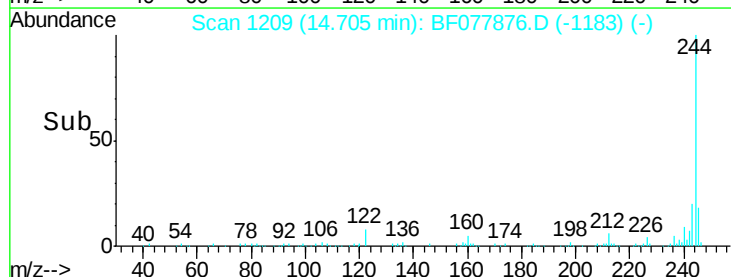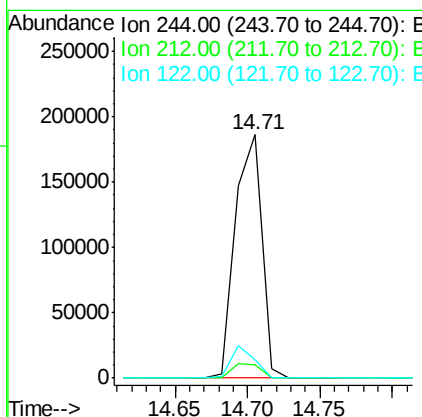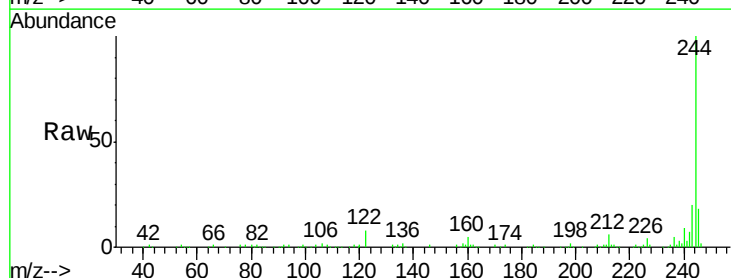


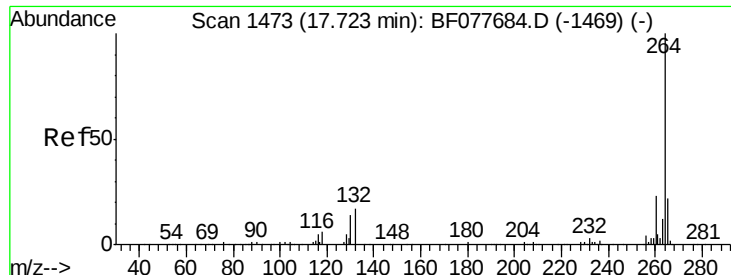

#86
Pervlene-d12
Concen: 20.00 ng
RT: 17.72 min Scan# 1473
Delta R.T. -0.11 min
Lab File: BF077876.D
Acq: 20 Mar 2015 21:22

Instrument :
BNA_F
ClientSampleId :
MW-24V

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.8	18.6	27.8
265	21.3	17.3	25.9

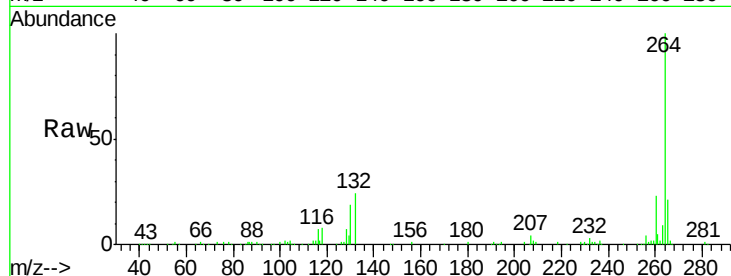

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

