

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032015\
 Data File : BF077876.D
 Acq On : 20 Mar 2015 21:22
 Operator : TP/IZ
 Sample : G1575-11
 Misc : W
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-24V

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.035	11	13	15	rBV	257937	206955	30.69%	2.030%
2	1.298	34	36	39	rVB	124124	179490	26.62%	1.761%
3	1.401	42	45	48	rVB	199686	292739	43.41%	2.872%
4	1.561	57	59	62	rVB	176494	216196	32.06%	2.121%
5	1.652	66	67	74	rVV	22843	43777	6.49%	0.429%
6	1.767	75	77	83	rVV	486378	674346	100.00%	6.616%
7	1.881	85	87	91	rVV2	189679	282471	41.89%	2.771%
8	1.950	91	93	97	rVB2	30253	48745	7.23%	0.478%
9	2.361	124	129	132	rVB	45703	73677	10.93%	0.723%
10	2.898	173	176	180	rBV	152192	295189	43.77%	2.896%
11	3.093	180	193	196	rVV3	9474	50107	7.43%	0.492%
12	3.470	224	226	232	rVB	8807	17654	2.62%	0.173%
13	3.733	246	249	253	rVB	29317	50630	7.51%	0.497%
14	4.156	283	286	287	rBV	48623	77184	11.45%	0.757%
15	4.190	287	289	293	rVB	331462	479521	71.11%	4.704%
16	4.407	305	308	310	rBV	8066	11270	1.67%	0.111%
17	4.876	348	349	352	rBV	20228	33502	4.97%	0.329%
18	5.024	352	362	364	rVV	76650	194200	28.80%	1.905%
19	5.173	366	375	380	rVV2	33109	92393	13.70%	0.906%
20	5.321	386	388	390	rBV	114564	115854	17.18%	1.137%
21	5.413	393	396	399	rBV	178818	192970	28.62%	1.893%
22	5.550	406	408	410	rBV	5324	8046	1.19%	0.079%
23	5.630	414	415	418	rBV2	12390	16710	2.48%	0.164%
24	5.813	428	431	432	rBV	12127	16278	2.41%	0.160%
25	5.847	432	434	437	rVB	147561	162776	24.14%	1.597%
26	6.247	467	469	472	rVB	7263	10779	1.60%	0.106%
27	6.670	504	506	507	rBV	7608	9617	1.43%	0.094%
28	6.704	507	509	513	rVV2	139204	239669	35.54%	2.351%
29	6.762	513	514	518	rVB	5854	7228	1.07%	0.071%
30	6.842	518	521	523	rBV	287153	344731	51.12%	3.382%
31	7.127	543	546	548	rBV	258189	255794	37.93%	2.510%
32	7.310	559	562	564	rBV	332254	291627	43.25%	2.861%
33	7.516	579	580	583	rVB	14233	14104	2.09%	0.138%
34	7.665	591	593	595	rBB	7121	7774	1.15%	0.076%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032015\
 Data File : BF077876.D
 Acq On : 20 Mar 2015 21:22
 Operator : TP/IZ
 Sample : G1575-11
 Misc : W
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-24V

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	7.813	604	606	609 rBV	184495	230827	34.23%	2.265%
36	7.973	618	620	622 rVB	5870	7316	1.08%	0.072%
37	8.110	628	632	634 rBV	8467	9003	1.34%	0.088%
38	8.407	654	658	664 rBV2	64906	128338	19.03%	1.259%
39	8.705	681	684	686 rBV	323892	350238	51.94%	3.436%
40	8.887	697	700	701 rBV	22914	22737	3.37%	0.223%
41	9.070	712	716	724 rBV	141661	215297	31.93%	2.112%
42	9.185	724	726	732 rVB2	4551	6807	1.01%	0.067%
43	9.710	769	772	778 rBV	13328	17167	2.55%	0.168%
44	10.053	799	802	804 rBV	411231	507461	75.25%	4.979%
45	10.179	811	813	816 rBV	11304	9441	1.40%	0.093%
46	10.556	844	846	849 rBV	54084	47620	7.06%	0.467%
47	10.842	869	871	872 rVV	27328	31397	4.66%	0.308%
48	10.865	872	873	876 rVB	299378	411474	61.02%	4.037%
49	11.128	891	896	898 rBV2	3687	9221	1.37%	0.090%
50	11.231	904	905	908 rVB	5193	7052	1.05%	0.069%
51	11.356	912	916	918 rBV	13953	14289	2.12%	0.140%
52	11.413	919	921	923 rVV	7037	9013	1.34%	0.088%
53	11.459	923	925	927 rVB	41226	36229	5.37%	0.355%
54	11.733	946	949	951 rBV	11908	18888	2.80%	0.185%
55	11.768	951	952	956 rVB3	10105	16200	2.40%	0.159%
56	11.848	956	959	961 rBV	313461	302121	44.80%	2.964%
57	11.939	963	967	972 rBV3	2393	8851	1.31%	0.087%
58	12.054	975	977	982 rBV	34910	53151	7.88%	0.521%
59	12.614	1023	1026	1027 rBV	24532	33634	4.99%	0.330%
60	12.648	1027	1029	1032 rVV	10731	14826	2.20%	0.145%
61	12.705	1032	1034	1037 rVV	474533	444419	65.90%	4.360%
62	13.082	1063	1067	1070 rBV2	3009	6914	1.03%	0.068%
63	13.139	1070	1072	1075 rVB	27713	28404	4.21%	0.279%
64	13.437	1095	1098	1099 rBV2	6031	7333	1.09%	0.072%
65	13.471	1099	1101	1103 rVB2	4530	8325	1.23%	0.082%
66	13.654	1114	1117	1118 rBV	10712	11966	1.77%	0.117%
67	13.757	1124	1126	1130 rVB2	9471	10681	1.58%	0.105%
68	14.705	1206	1209	1211 rBV	457426	639762	94.87%	6.277%
69	15.014	1232	1236	1241 rBV2	4182	11679	1.73%	0.115%
70	15.471	1270	1276	1280 rVV3	2835	9097	1.35%	0.089%
71	15.871	1308	1311	1318 rBV2	124854	216785	32.15%	2.127%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	15.985	1318	1321	1323	rVV	410854	496954	73.69%	4.876%
73	16.042	1323	1326	1328	rVB	9236	13375	1.98%	0.131%
74	16.694	1380	1383	1389	rBV4	8798	21271	3.15%	0.209%
75	16.877	1397	1399	1402	rBV4	5581	9122	1.35%	0.089%
76	17.037	1411	1413	1415	rVB2	8734	10515	1.56%	0.103%
77	17.083	1415	1417	1421	rBV5	4827	10568	1.57%	0.104%
78	17.163	1421	1424	1427	rVB	77755	93253	13.83%	0.915%
79	17.483	1449	1452	1455	rBV3	5227	8895	1.32%	0.087%
80	17.723	1471	1473	1476	rBV	344760	476523	70.66%	4.675%
81	17.871	1484	1486	1490	rVB4	5748	10568	1.57%	0.104%
82	18.168	1508	1512	1514	rBV5	4485	12020	1.78%	0.118%
83	18.351	1525	1528	1530	rBV3	10206	23354	3.46%	0.229%
84	18.511	1540	1542	1544	rBV3	3809	7201	1.07%	0.071%
85	18.603	1547	1550	1552	rBV3	6119	11966	1.77%	0.117%
86	18.763	1562	1564	1565	rBV	5266	6873	1.02%	0.067%
87	18.797	1565	1567	1574	rVB2	9940	29872	4.43%	0.293%
88	19.323	1609	1613	1614	rBV3	6180	13911	2.06%	0.136%
89	19.963	1666	1669	1671	rBV4	4147	8648	1.28%	0.085%


Sum of corrected areas: 10192855

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

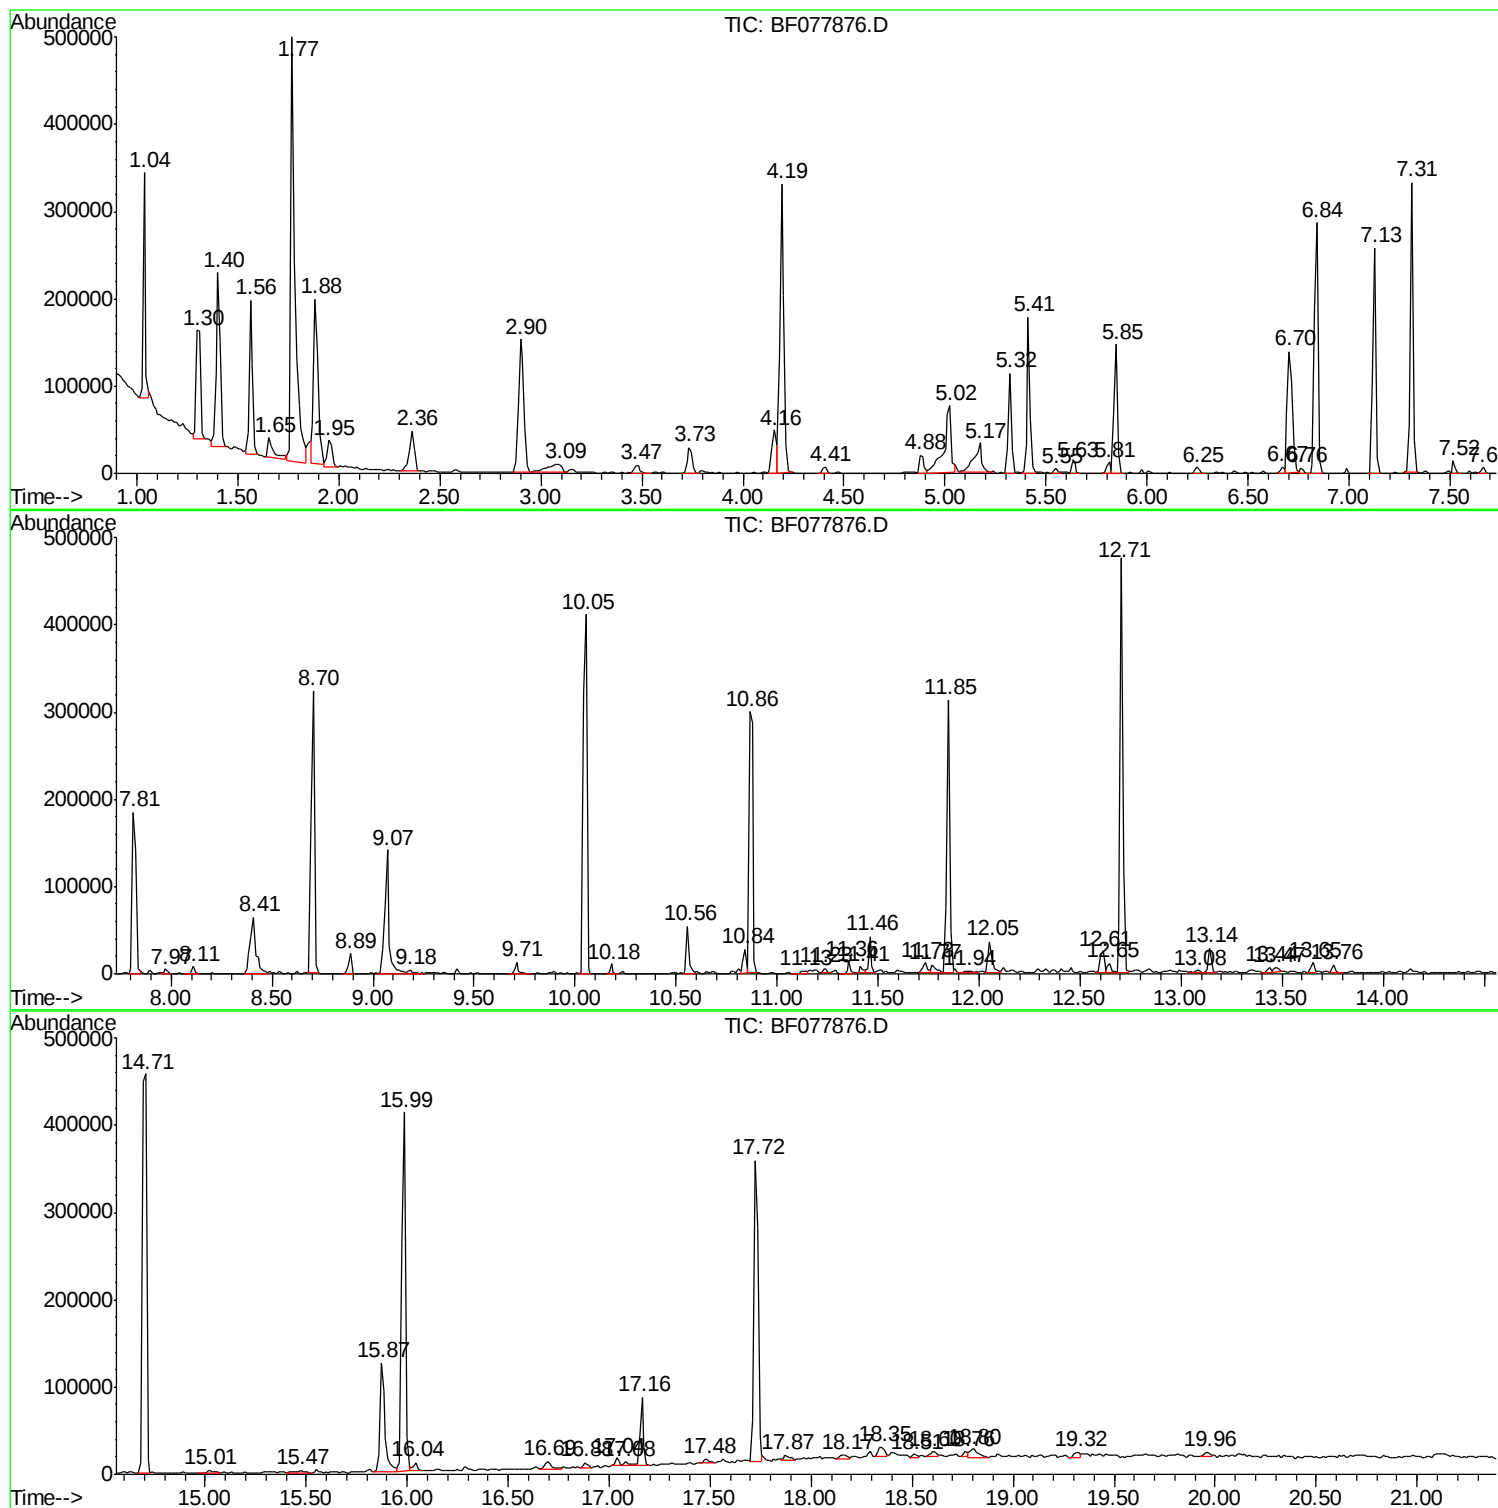

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Roflurane Concentration Rank 11

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.30	14.03 ng	179490	1,4-Dichlorobenzene-d4	7.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Roflurane	192	C3H4BrF3O	000679-90-3	56
2		1H-Pyrrole, 1-methyl-	81	C5H7N	000096-54-8	5
3		2(5H)-Furanone, 5-(2-furanvlmeth...	178	C10H10O3	031969-27-4	4
4		1,1-Dichloro-1-fluoroethane	116	C2H3Cl2F	001717-00-6	4
5		Bis(2-furfuryl)disulfide	226	C10H10O2S2	004437-20-1	4

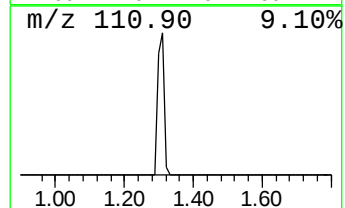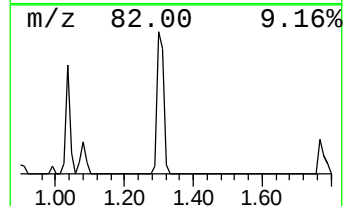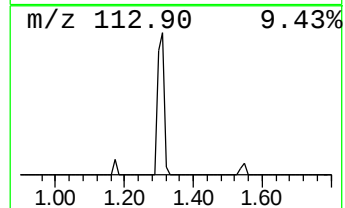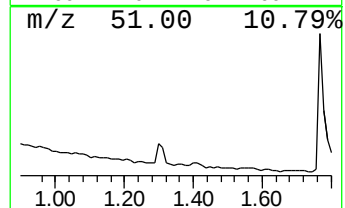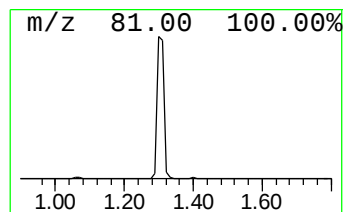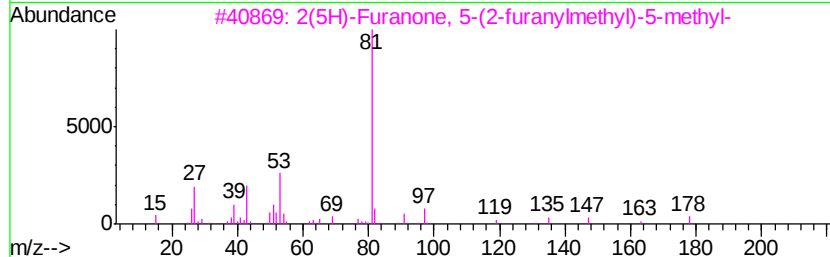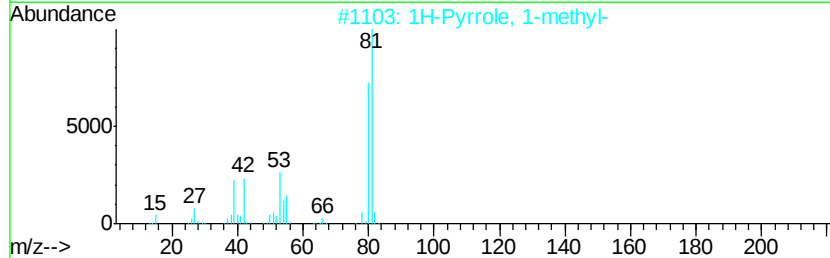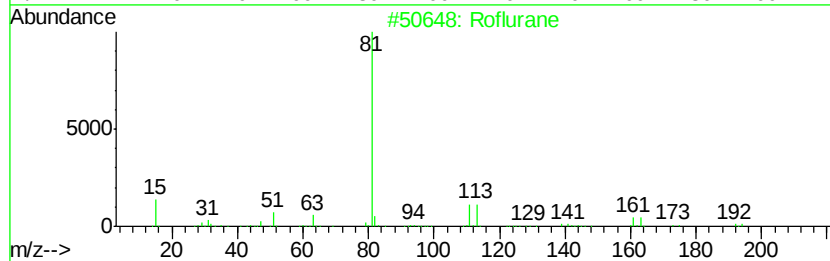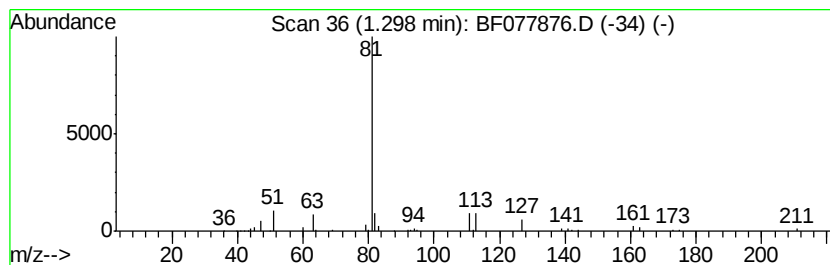

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Butane, 2-methoxy-2-methyl- Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.56	16.90 ng	216196	1,4-Dichlorobenzene-d4	7.13

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	37
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	10
5			Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9

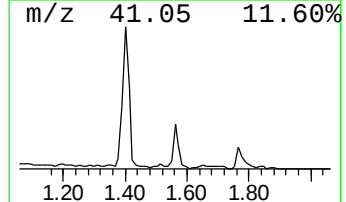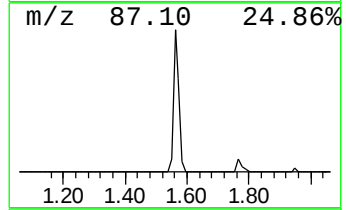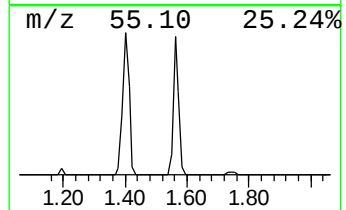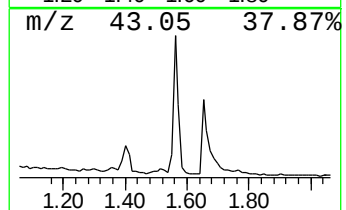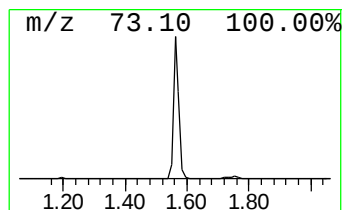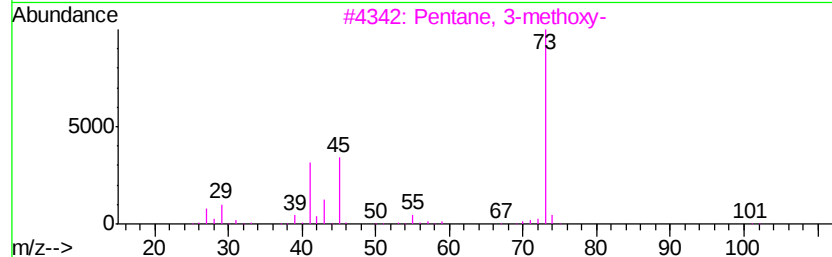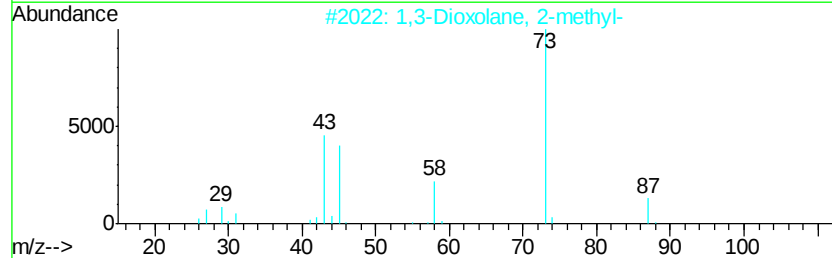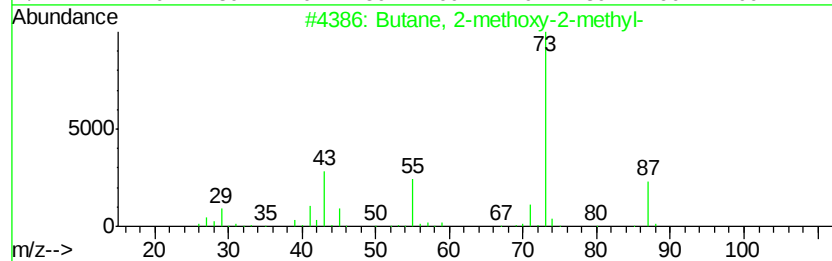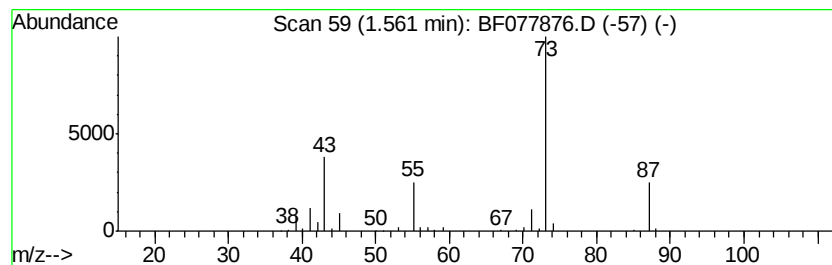

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
MW-24V

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 Methoxyflurane Concentration Rank 18

R.T.	EstConc	Area	Relative to ISTD	R.T.	
2.36	5.76 ng	73677	1,4-Dichlorobenzene-d4	7.13	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Methoxyvflurane	164	C3H4Cl2F2O	000076-38-0	83
2	Ethane, 2-bromo-2-chloro-1,1-dif...	208	C3H4BrClF2O	000679-89-0	9
3	Acetic acid, dichloro-, ethyl ester	156	C4H6Cl2O2	000535-15-9	9
4	Cyclopentene, 4,4-dimethyl-	96	C7H12	019037-72-0	4
5	Cyclopentene, 1,5-dimethyl-	96	C7H12	016491-15-9	4

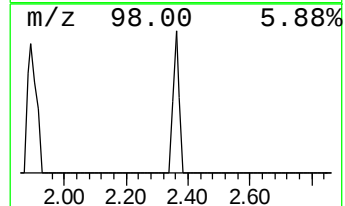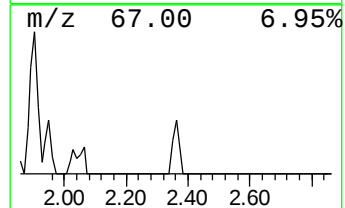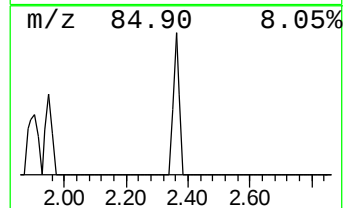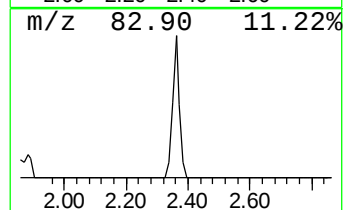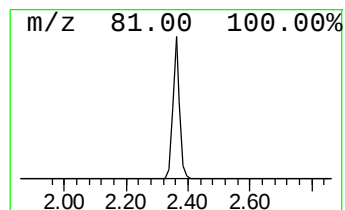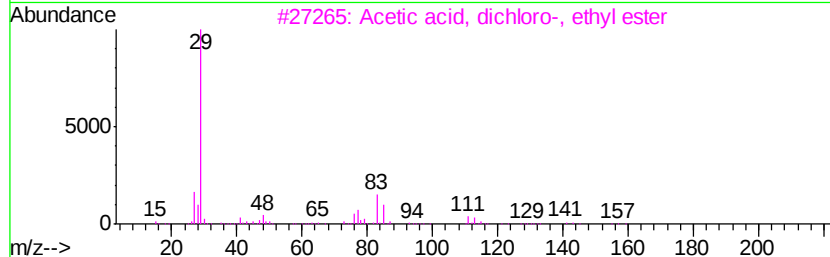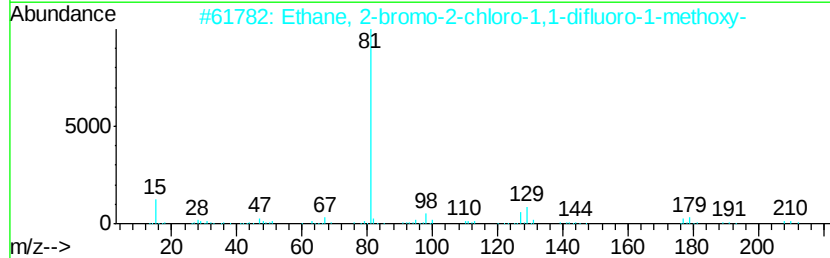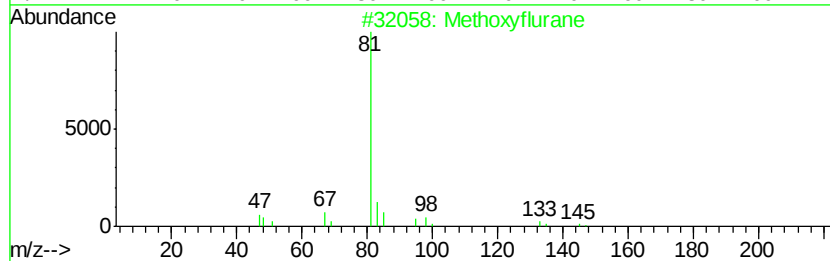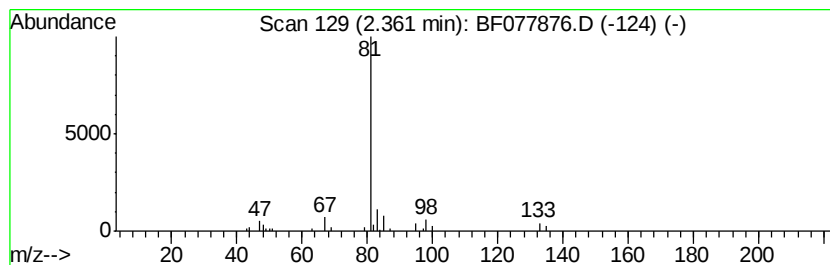

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 10 unknown3.73 Concentration Rank 19

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.73	3.96 ng	50630	1,4-Dichlorobenzene-d4	7.13

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,2,2-trichloro-1,1-difl...	168	C2HCl3F2	000354-21-2	38
2			Ethane, 2,2-dichloro-1,1,1-trifl...	152	C2HCl2F3	000306-83-2	37
3			Methane, bromodichloro-	162	CHBrCl2	000075-27-4	32
4			Trichloromethane	118	CHCl3	000067-66-3	32
5			Ethane, 1,1-dichloro-2,2-difluoro-	134	C2H2Cl2F2	000471-43-2	32

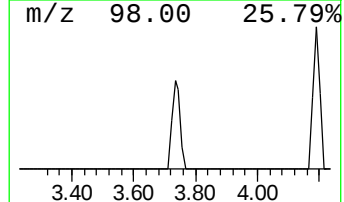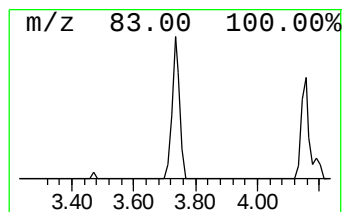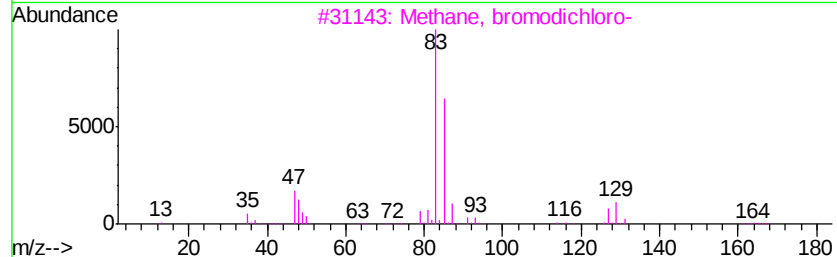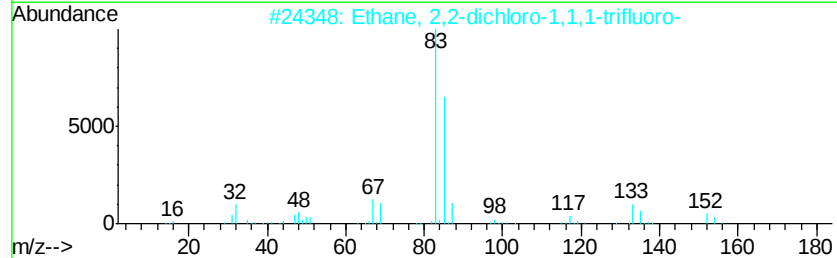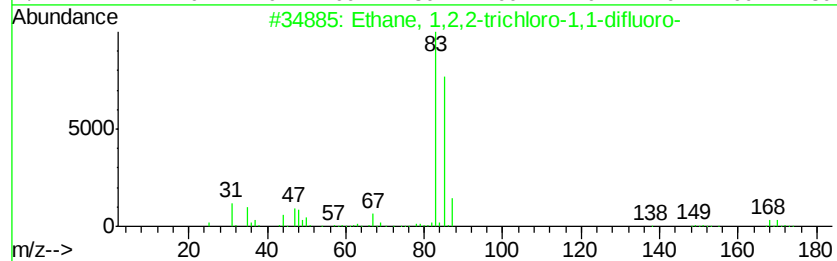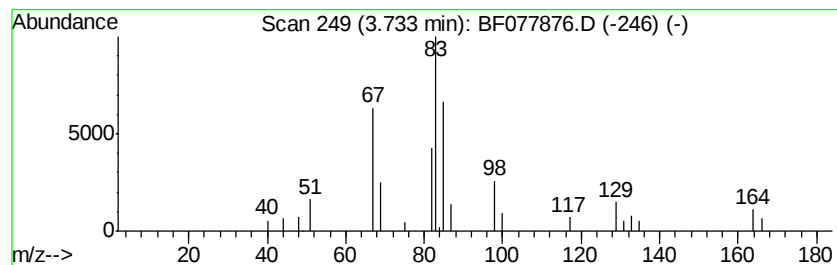

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 13 unknown5.02 Concentration Rank 10

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.02	15.18 ng	194200	1,4-Dichlorobenzene-d4	7.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	27
2		Butanoic acid, 3-methyl-	102	C5H10O2	000503-74-2	22
3		Thiirane	60	C2H4S	000420-12-2	16
4		Formic acid hydrazide	60	CH4N2O	000624-84-0	10
5		Thiazole, 4,5-dihydro-2-methyl-	101	C4H7NS	002346-00-1	10

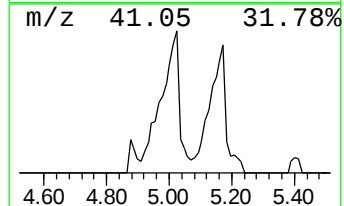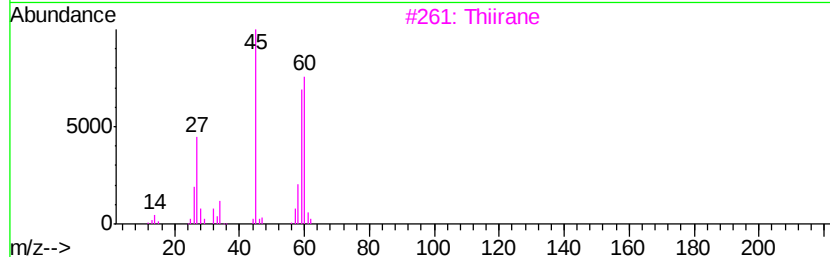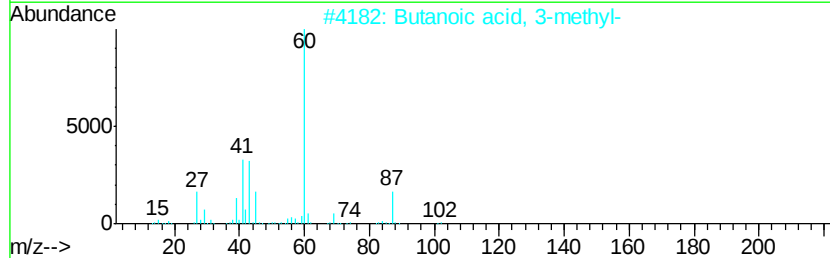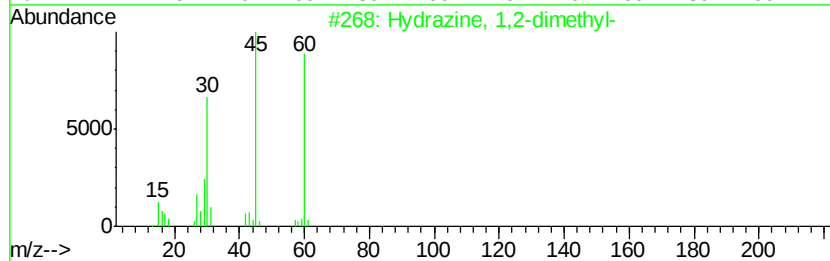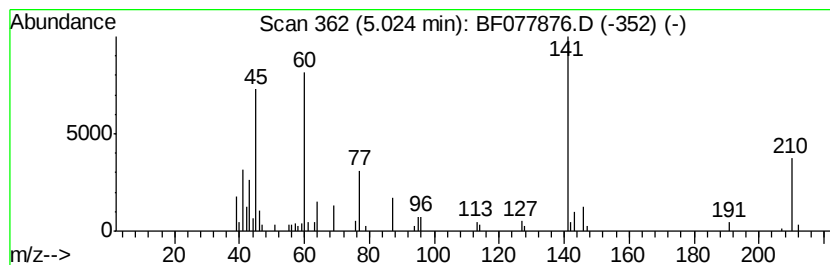

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 14 unknown5.17 Concentration Rank 16

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.17	7.22 ng	92393	1,4-Dichlorobenzene-d4	7.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butanoic acid, 2-methyl-	102	C5H10O2	000116-53-0	38
2		Pentanoic acid, methyl ester	116	C6H12O2	000624-24-8	28
3		Pentanoic acid, 2-methyl-	116	C6H12O2	000097-61-0	25
4		Hexanoic acid, 2-methyl-	130	C7H14O2	004536-23-6	25
5		Succinamic acid	117	C4H7NO3	000638-32-4	17

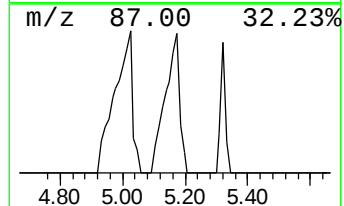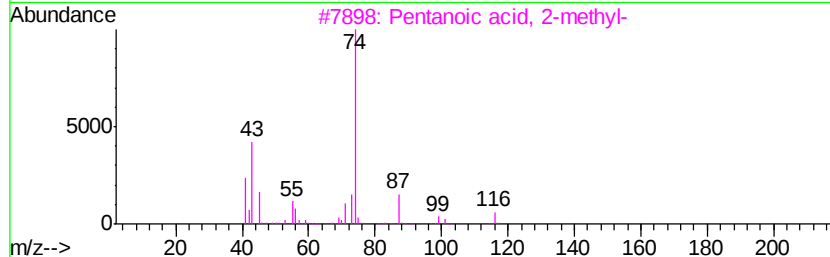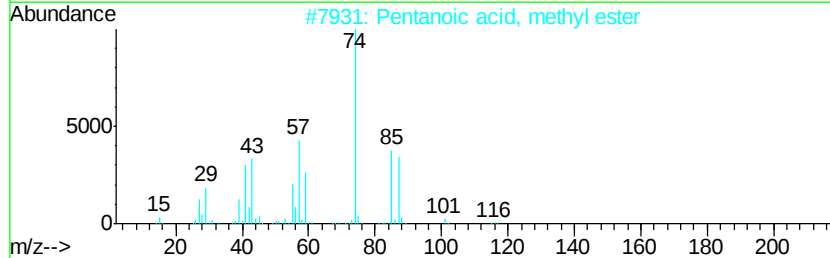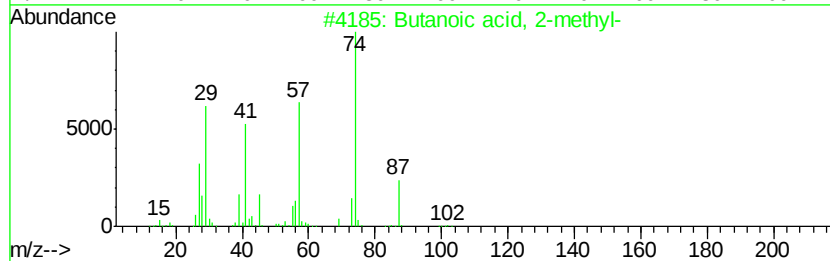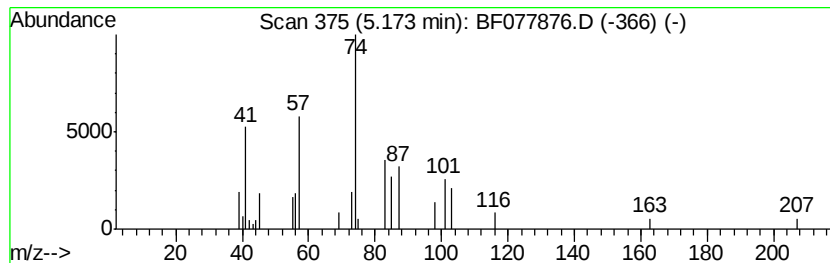

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 15 unknown5.32 Concentration Rank 14

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.32	9.06 ng	115854	1,4-Dichlorobenzene-d4	7.13

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Propanone, 1,1,3,3-tetrachloro-	194	C3H2Cl4O	000632-21-3	35
2			Cyclohexanone, 2,2,5,5-tetrameth...	166	C11H18O	035505-97-6	27
3			Propane, 1,2,2,3,3-pentachloro-1...	250	C3HCl5F2	000422-30-0	22
4			Ethane, 1,2,2-trichloro-1,1-diflu...	168	C2HCl3F2	000354-21-2	22
5			Cyclohexane, (cyclopentylmethyl)-	166	C12H22	004431-89-4	16

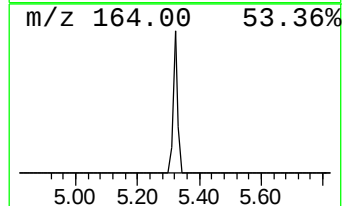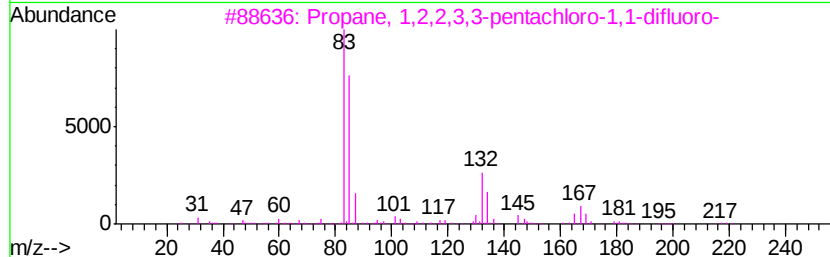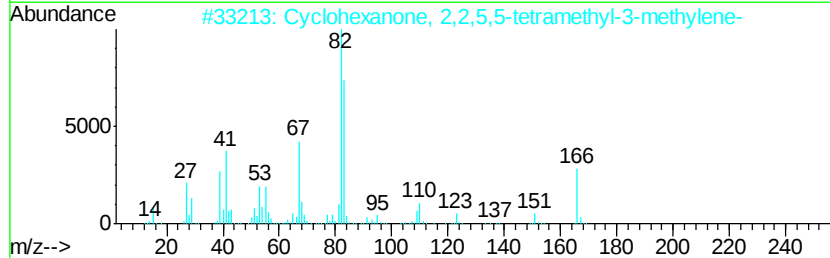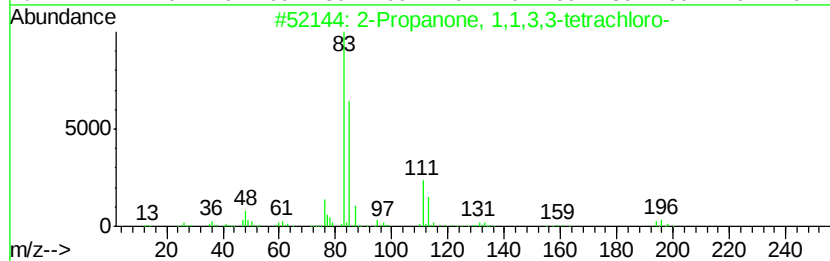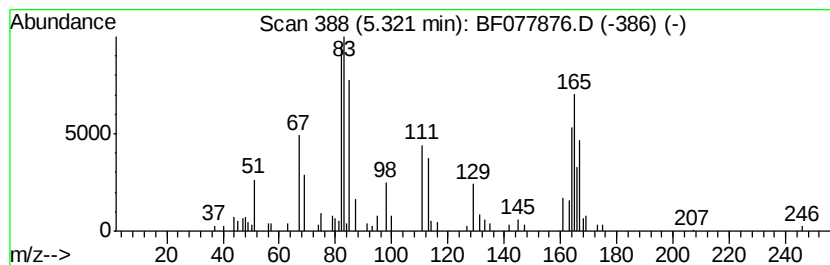

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 16 unknown5.85 Concentration Rank 12

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.85	12.73 ng	162776	1,4-Dichlorobenzene-d4	7.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Methoxyphenyl isothiocyanate	165	C8H7NOS	002284-20-0	40
2		2',4'-Dimethoxyacetophenone	180	C10H12O3	000829-20-9	40
3		Benzene, 1-[(tert-butylidimethylsilyl)oxy]-4-methyl-	222	C13H22OSi	062790-85-6	36
4		Acetamide, 2,2-dichloro-N-(4-nitrophenyl)-	248	C8H6Cl2N2O3	016346-60-4	25
5		2-Amino-6-hydroxy-9-methylpurine	165	C6H7N5O	005502-78-3	9

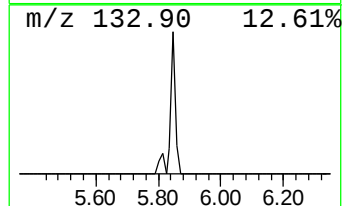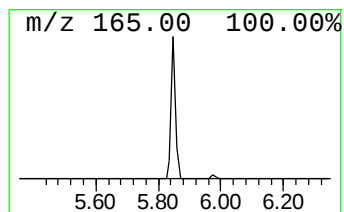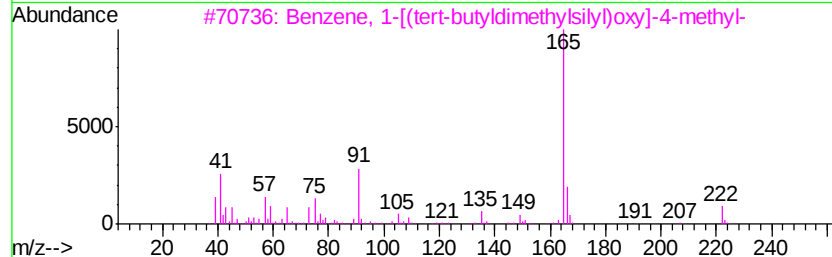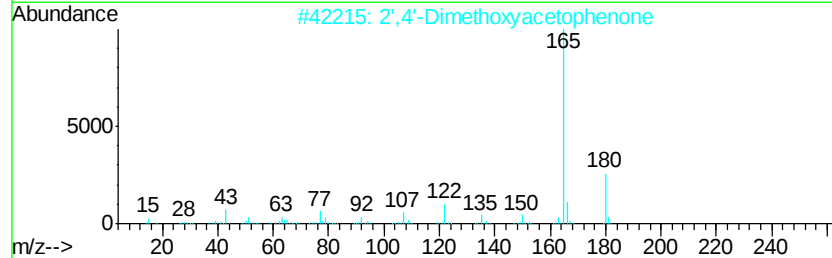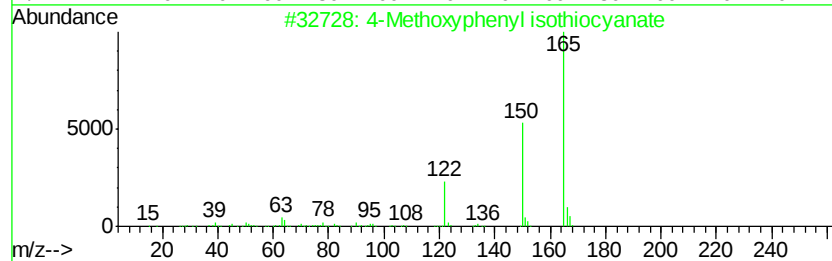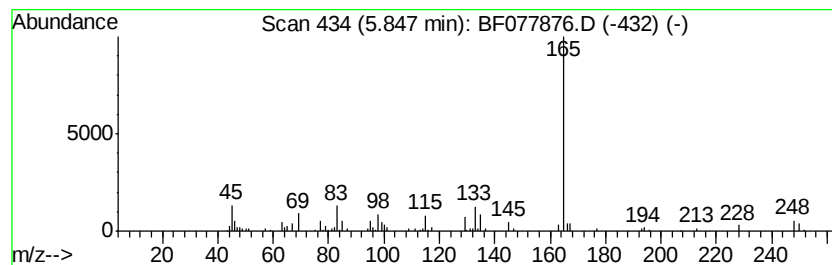

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 17 unknown6.84 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.84	26.95 ng	344731	1,4-Dichlorobenzene-d4	7.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		Amphetaminil	250	C17H18N2	017590-01-1	12
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

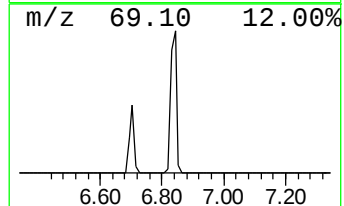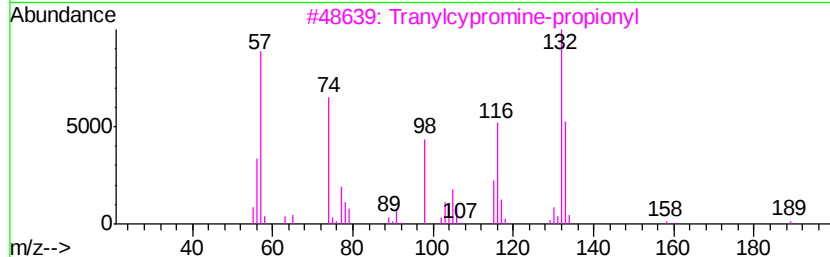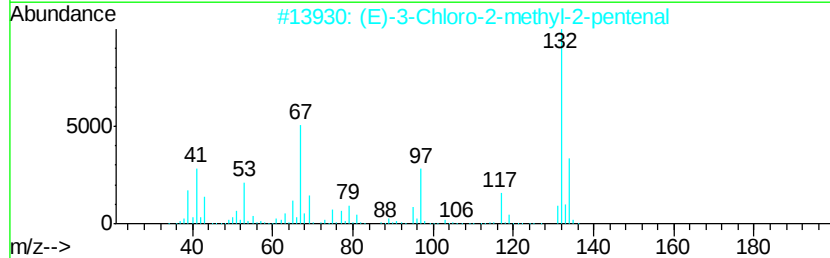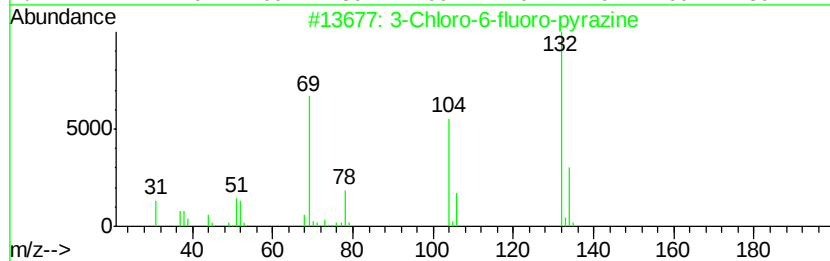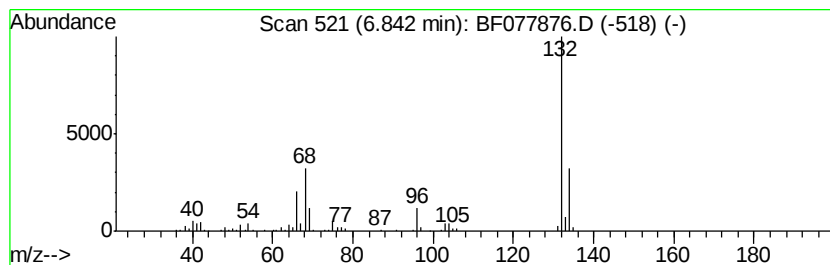

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 19 Benzeneacetic acid Concentration Rank 13

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.07	12.29 ng	215297	Naphthalene-d8	8.70

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Benzeneacetic acid	136	C8H8O2	000103-82-2	90
2		Propanedioic acid, phenyl-	180	C9H8O4	002613-89-0	83
3		Benzene, (2-methoxvethyl)-	136	C9H12O	003558-60-9	72
4		Benzoic acid, 4-methyl-	136	C8H8O2	000099-94-5	64
5		Benzene, (iodomethyl)-	218	C7H7I	000620-05-3	50

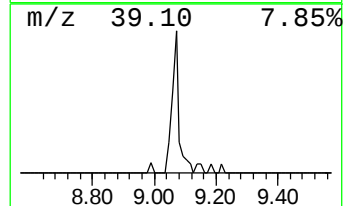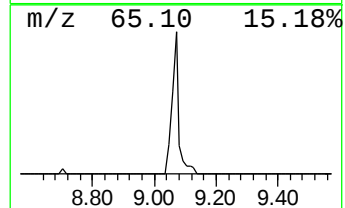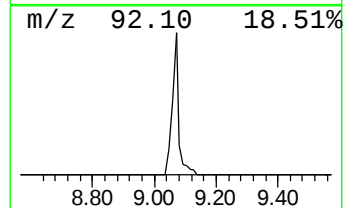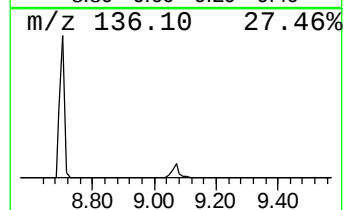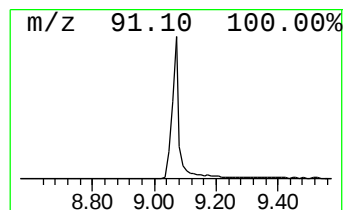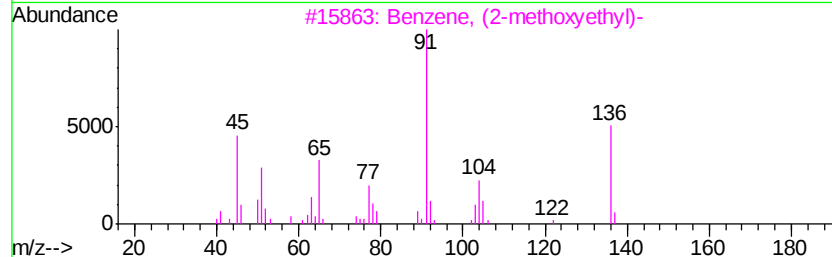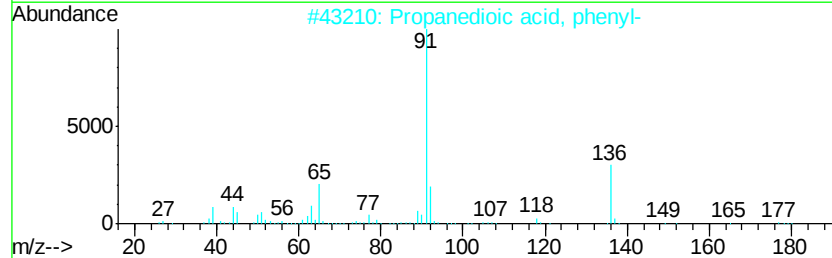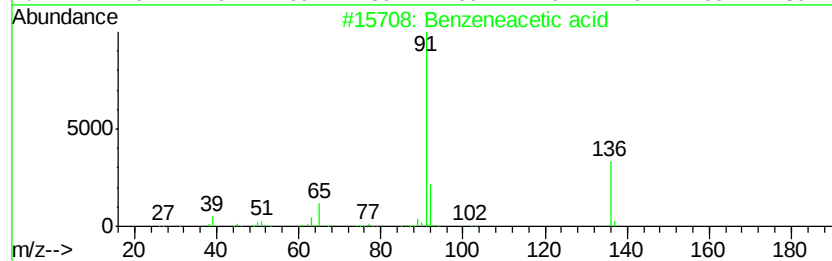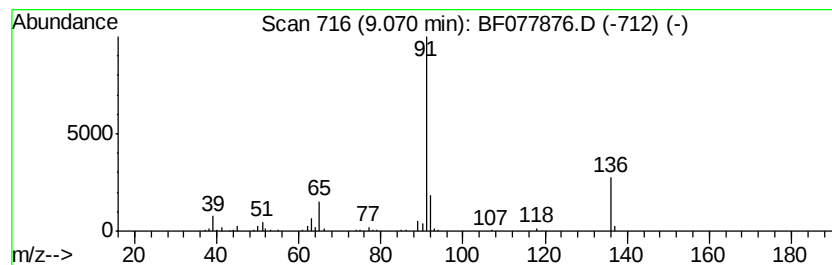

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032015\
Data File : BF077876.D
Acq On : 20 Mar 2015 21:22
Operator : TP/IZ
Sample : G1575-11
Misc : W
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-24V










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 20 Heptafluorobutyric acid, n-... Concentration Rank 15

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.87	8.72 ng	216785	Chrysene-d12	15.99

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptafluorobutyric acid, n-penta...	424	C19H31F7O2	1000216-79-3	91
2			Trichloroacetic acid, tetradecyl...	358	C16H29Cl3O2	074339-52-9	91
3			Bromoacetic acid, octadecyl ester	390	C20H39BrO2	018992-03-5	91
4			9-Eicosene, (E)-	280	C20H40	074685-29-3	91
5			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	90

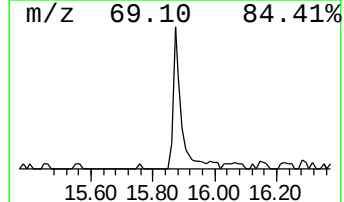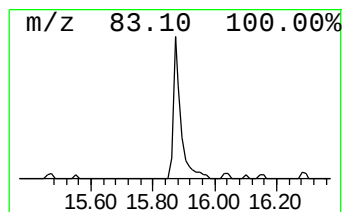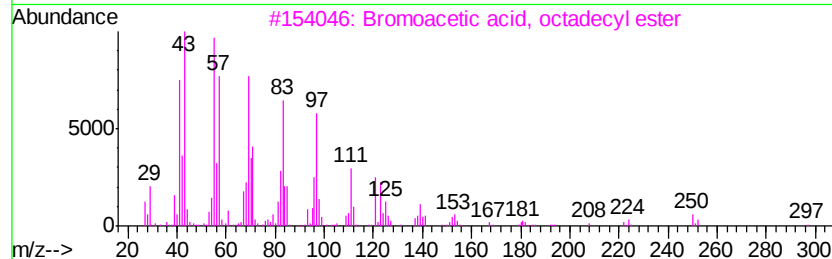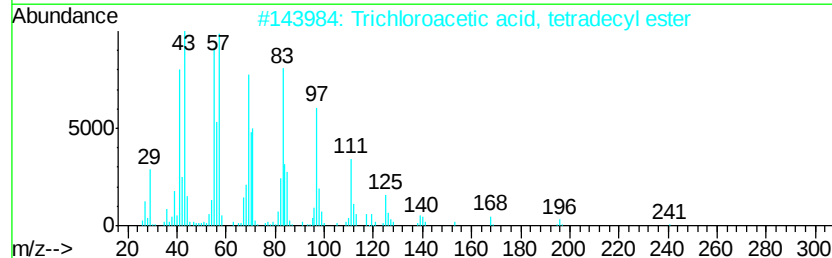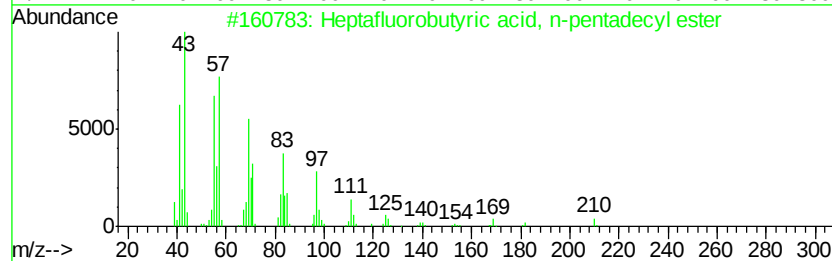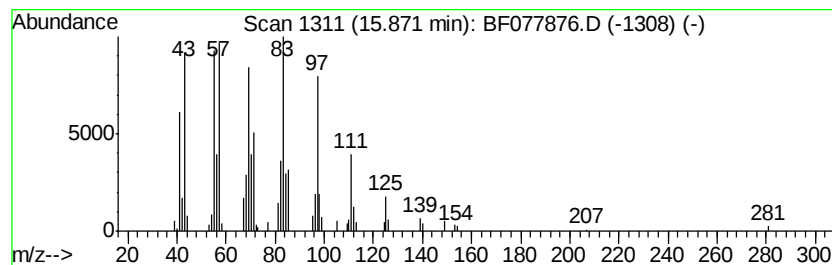

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032015\
 Data File : BF077876.D
 Acq On : 20 Mar 2015 21:22
 Operator : TP/IZ
 Sample : G1575-11
 Misc : W
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-24V

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
 TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Roflurane	1.30	14.0	ng	179490	1	7.13	255794	20.0
Butane, 2-methoxy...	1.56	16.9	ng	216196	1	7.13	255794	20.0
Methoxyflurane	2.36	5.8	ng	73677	1	7.13	255794	20.0
unknown3.73	3.73	4.0	ng	50630	1	7.13	255794	20.0
unknown5.02	5.02	15.2	ng	194200	1	7.13	255794	20.0
unknown5.17	5.17	7.2	ng	92393	1	7.13	255794	20.0
unknown5.32	5.32	9.1	ng	115854	1	7.13	255794	20.0
unknown5.85	5.85	12.7	ng	162776	1	7.13	255794	20.0
unknown6.84	6.84	26.9	ng	344731	1	7.13	255794	20.0
Benzeneacetic acid	9.07	12.3	ng	215297	2	8.70	350238	20.0
Heptafluorobutyri...	15.87	8.7	ng	216785	5	15.99	496954	20.0