

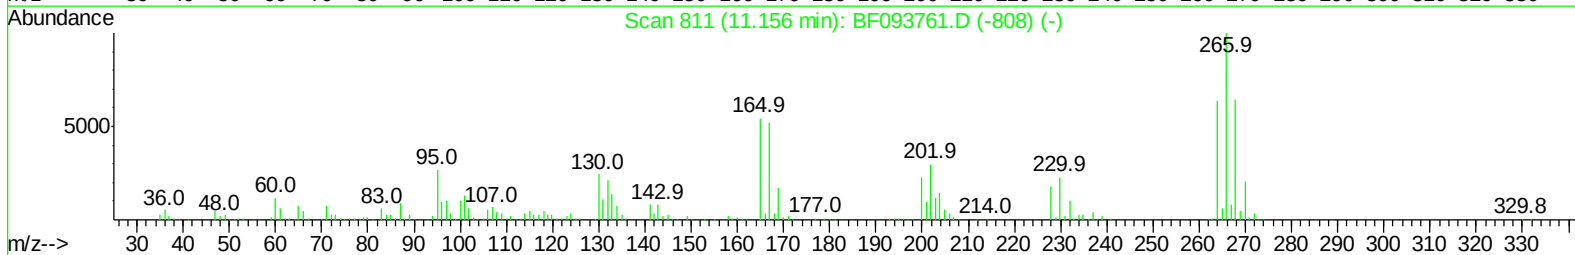


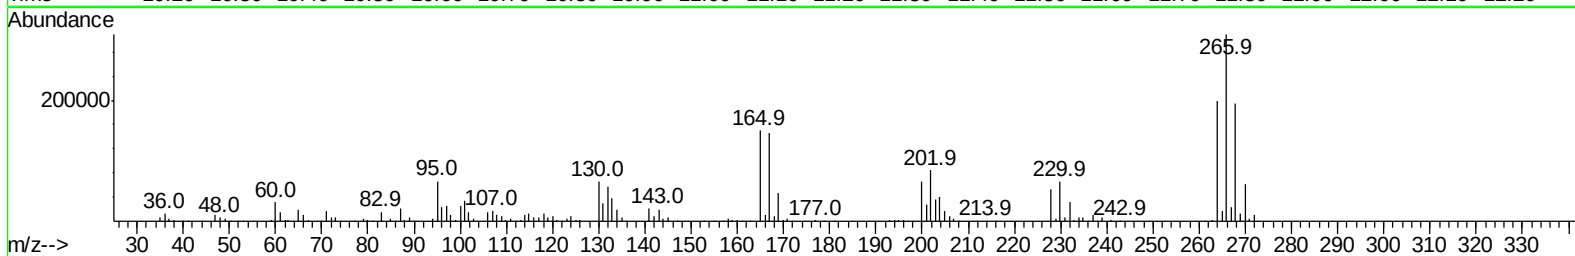

Data Path : Z:\HPCHEM1\BNA F\Data\BF032017\  
Data File : BF093757.D  
Acq On : 20 Mar 2017 10:55  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 07:09:14 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032017.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Mar 20 16:03:59 2017  
Response via : Initial Calibration

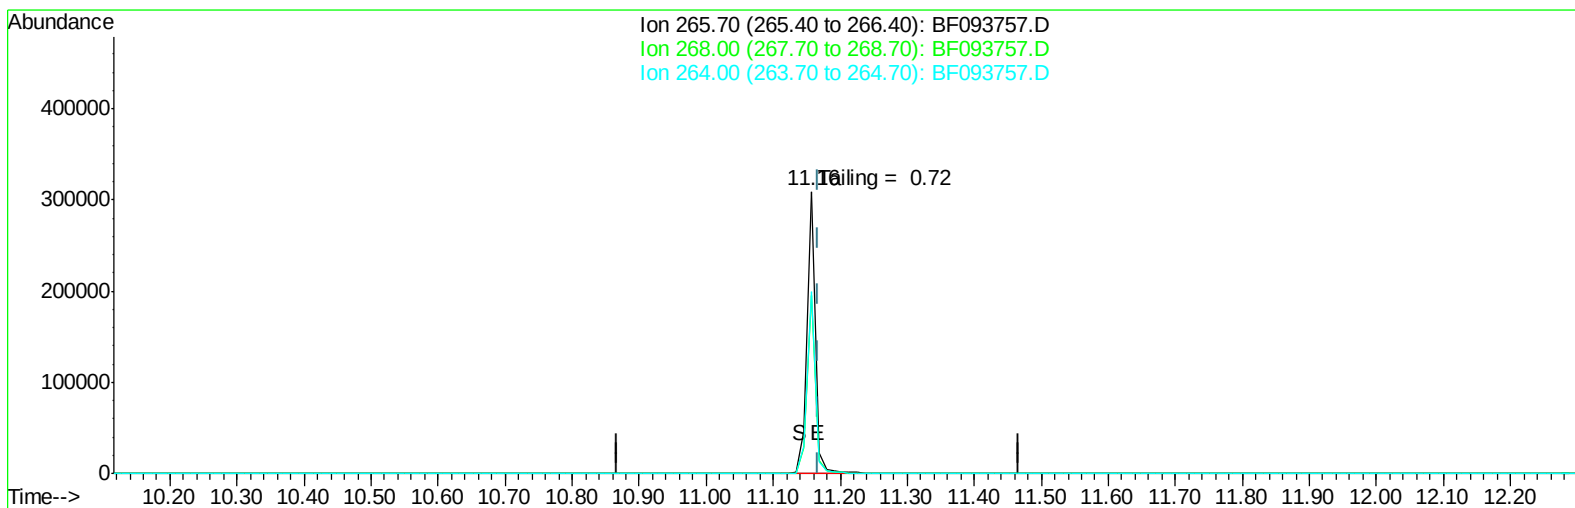

TIC: BF093757.D

(69) Pentachlorophenol (C)

11.156min (-0.011) 0.00ng

response 268525

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 63.17 |
| 264.00 | 64.60 | 64.64 |
| 0.00   | 0.00  | 0.00  |