
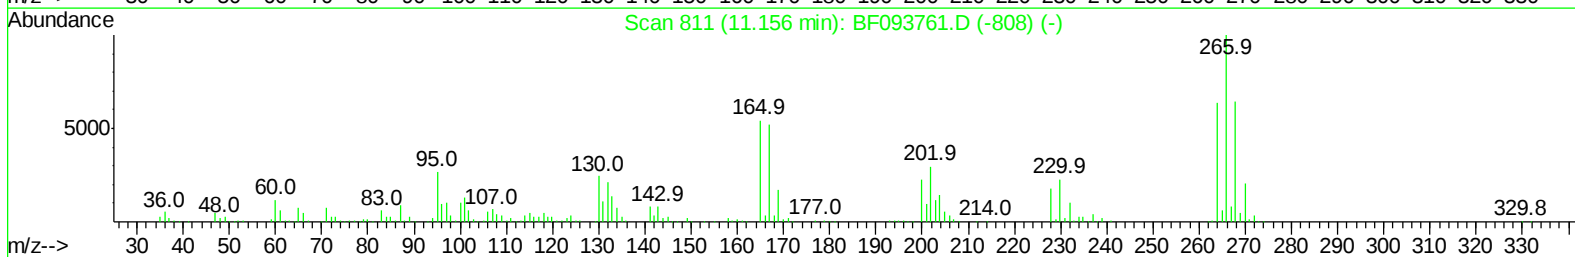
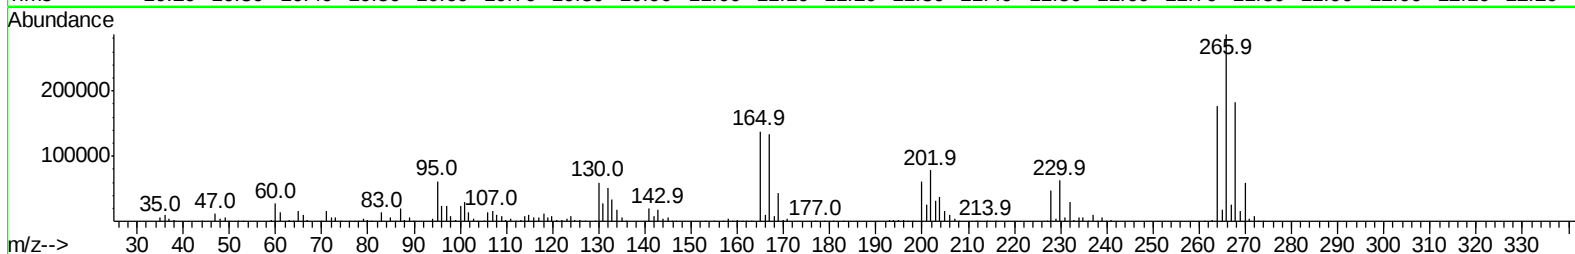


Data Path : Z:\HPCHEM1\BNA F\Data\BF032017\
Data File : BF093766.D
Acq On : 20 Mar 2017 15:53
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 07:09:49 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 20 16:03:59 2017
Response via : Initial Calibration

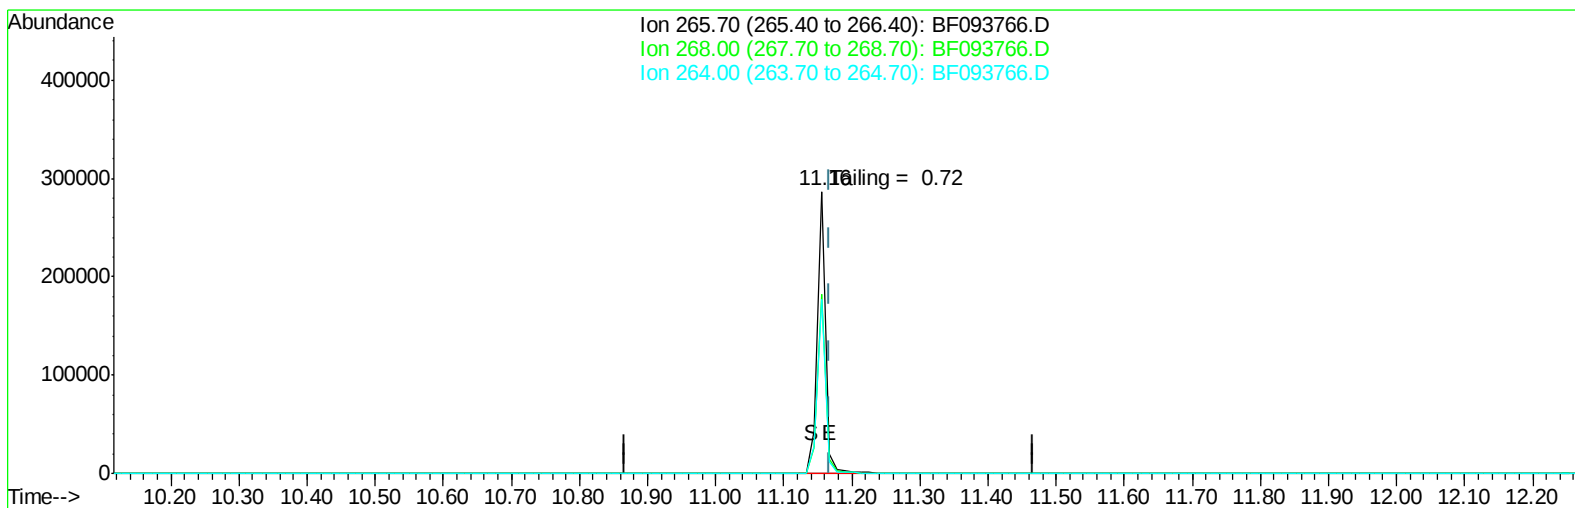

TIC: BF093766.D

(69) Pentachlorophenol (C)




11.156min (-0.011) 0.00ng

response 247836

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.54
264.00	64.60	62.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF032017\
 Data File : BF093766.D
 Acq On : 20 Mar 2017 15:53
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 07:09:49 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 20 16:03:59 2017
 Response via : Initial Calibration

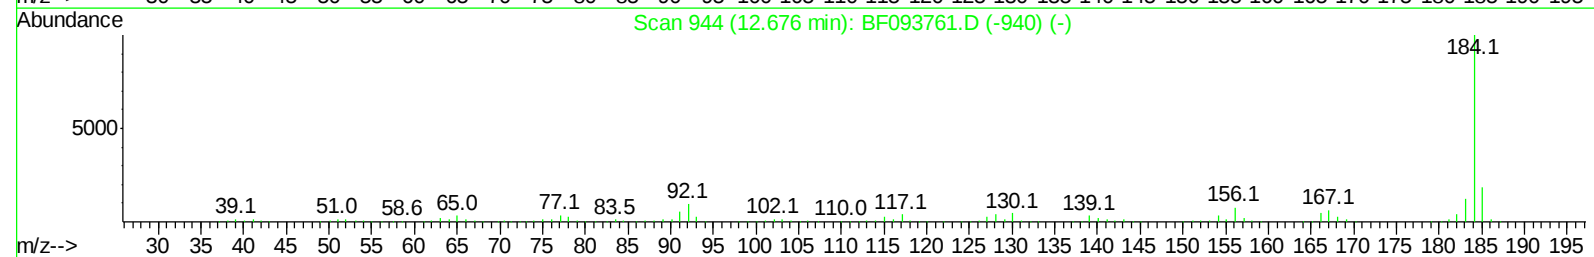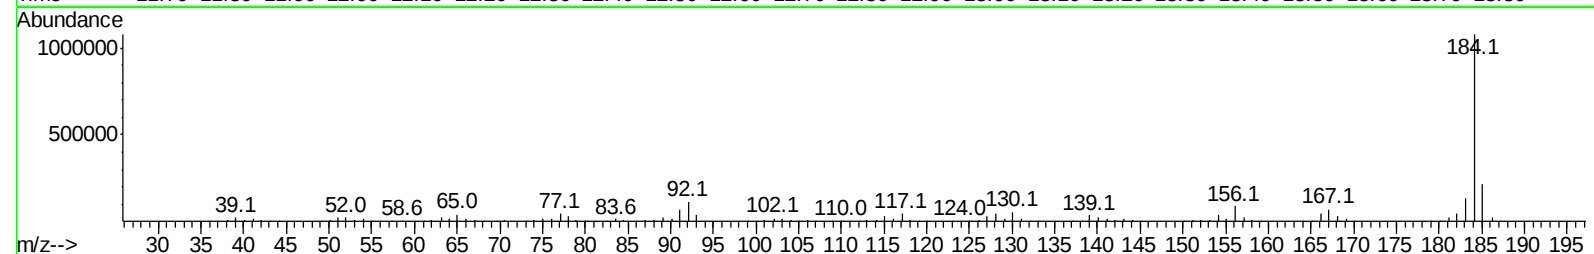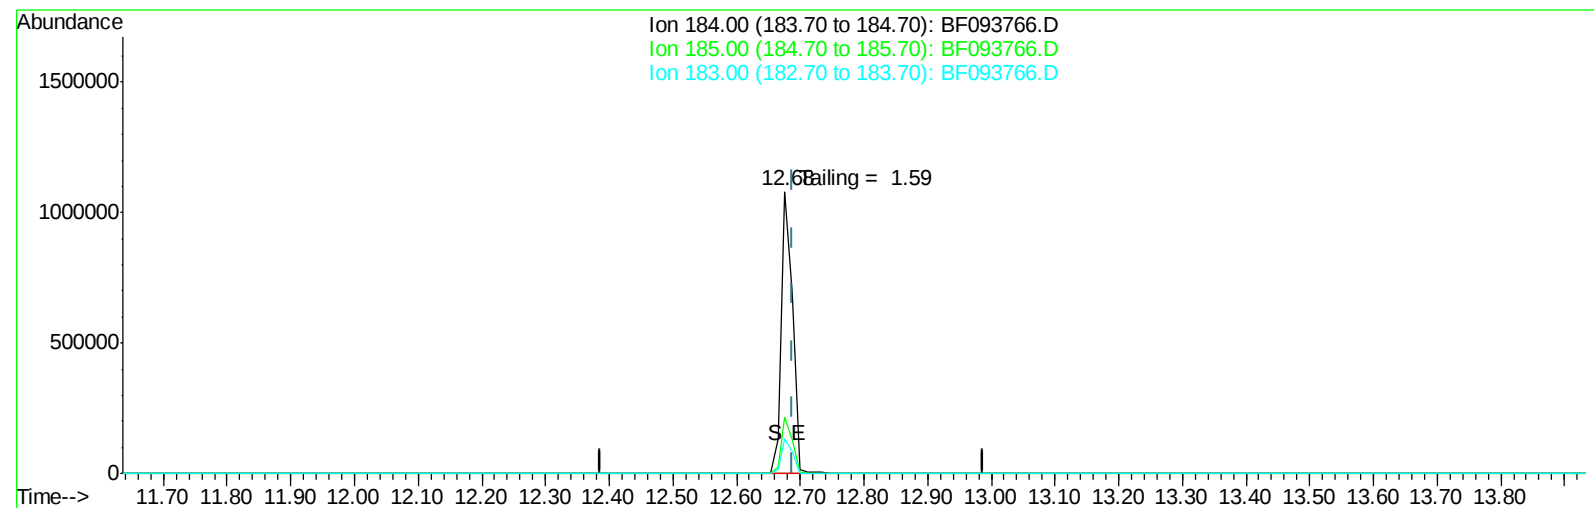

TIC: BF093766.D

(76) Benzidine

12.676min (-0.011) 0.00ng

response 1334933

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	20.19
183.00	12.20	12.30
0.00	0.00	0.00