


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032017\
 Data File : BF093766.D
 Acq On : 20 Mar 2017 15:53
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 21 14:38:20 2017

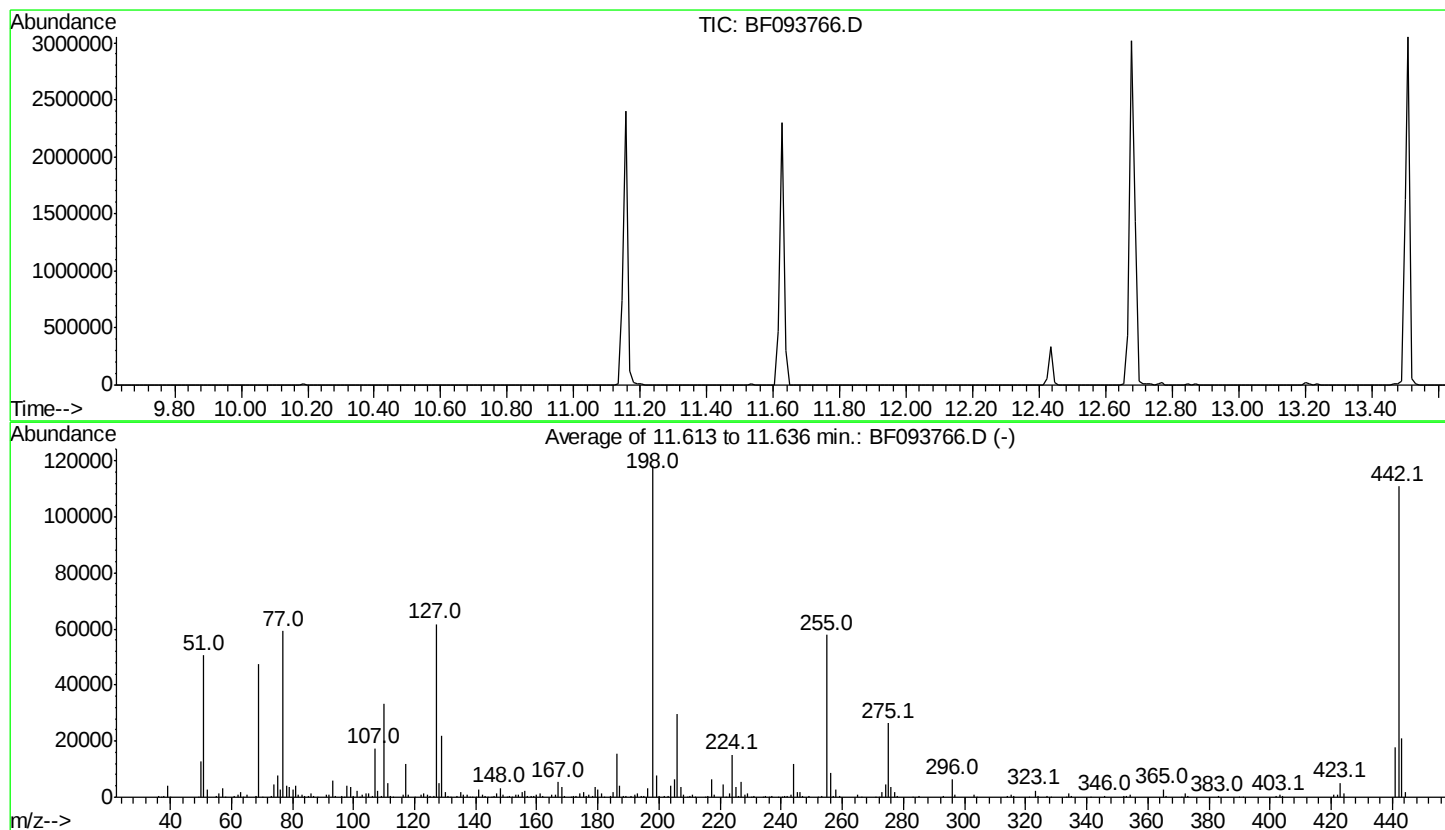

AutoFind: Scans 851, 852, 853; Background Corrected with Scan 847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	50539	PASS
68	69	0.00	2	1.3	598	PASS
69	198	0.00	100	40.1	47342	PASS
70	69	0.00	2	0.5	222	PASS
127	198	10	80	52.3	61773	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118205	PASS
199	198	5	9	6.6	7781	PASS
275	198	10	60	22.2	26253	PASS
365	198	1	100	2.4	2839	PASS
441	442	0.01	24	15.9	17653	PASS
442	198	50	100	93.7	110779	PASS
443	442	15	24	19.0	21013	PASS