
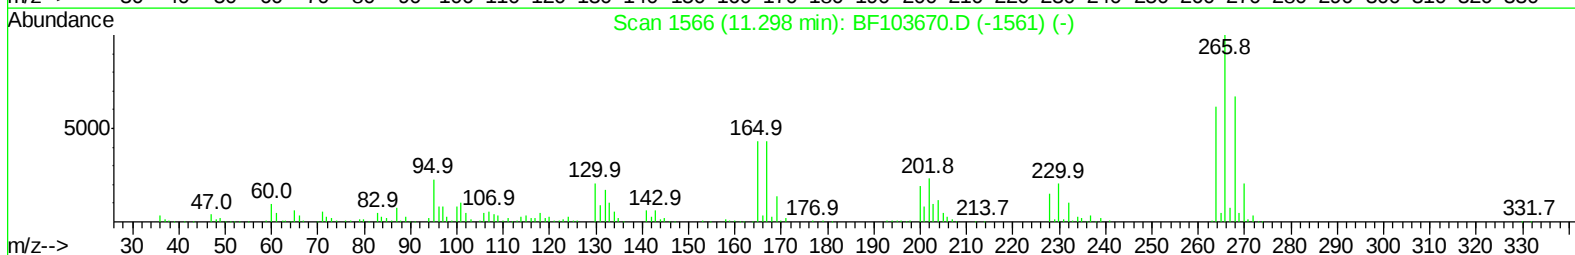
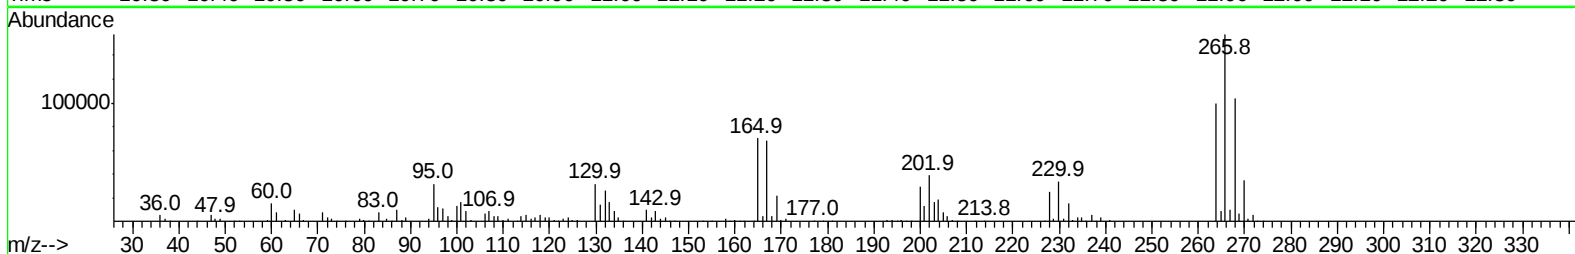


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF032018\
Data File : BF103798.D
Acq On : 20 Mar 2018 13:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 07:21:06 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

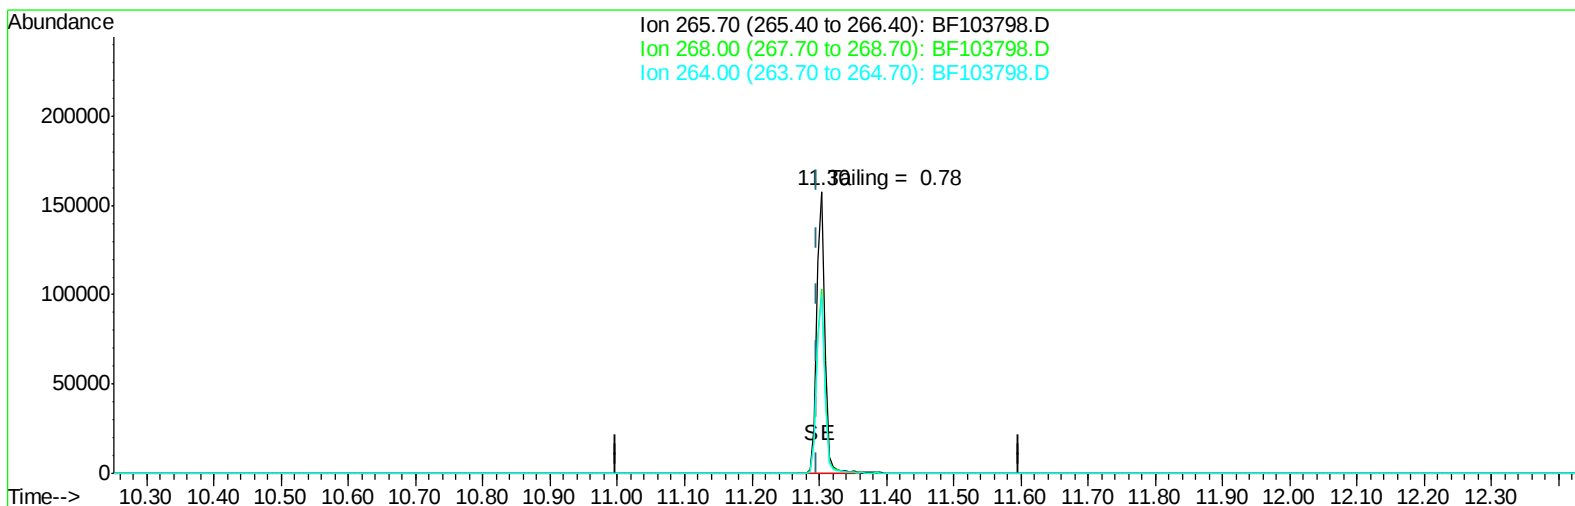

TIC: BF103798.D

(69) Pentachlorophenol (C)

11.304min (+0.006) 55522.13ng

response 139151

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.69
264.00	61.90	63.37
0.00	0.00	0.00