
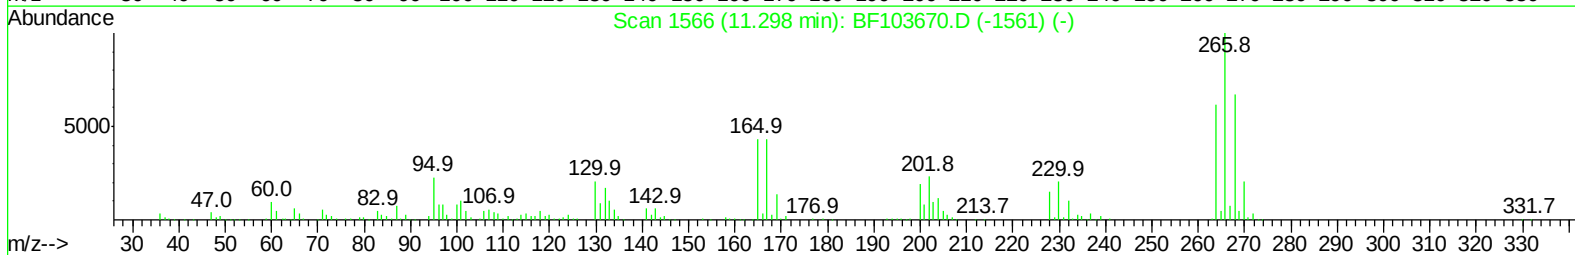
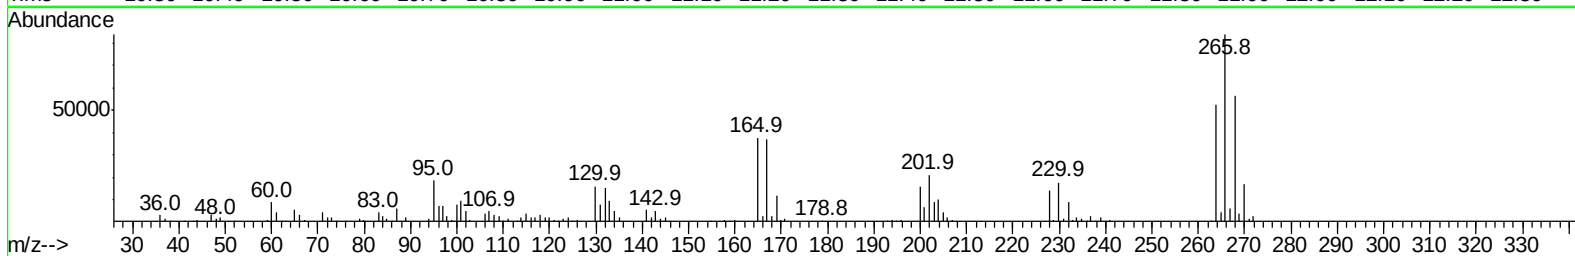


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF032018\
Data File : BF103824.D
Acq On : 21 Mar 2018 1:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 07:22:10 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

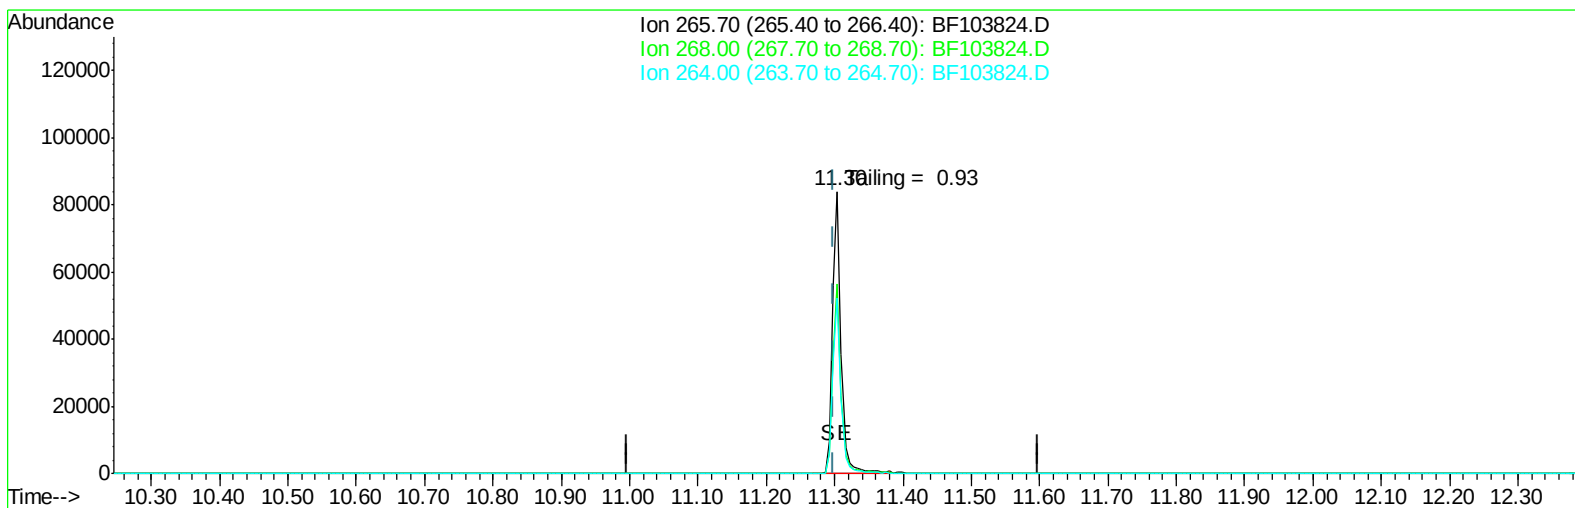

TIC: BF103824.D

(69) Pentachlorophenol (C)

11.304min (+0.006) 49434.83ng

response 72272

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.23
264.00	61.90	62.18
0.00	0.00	0.00