
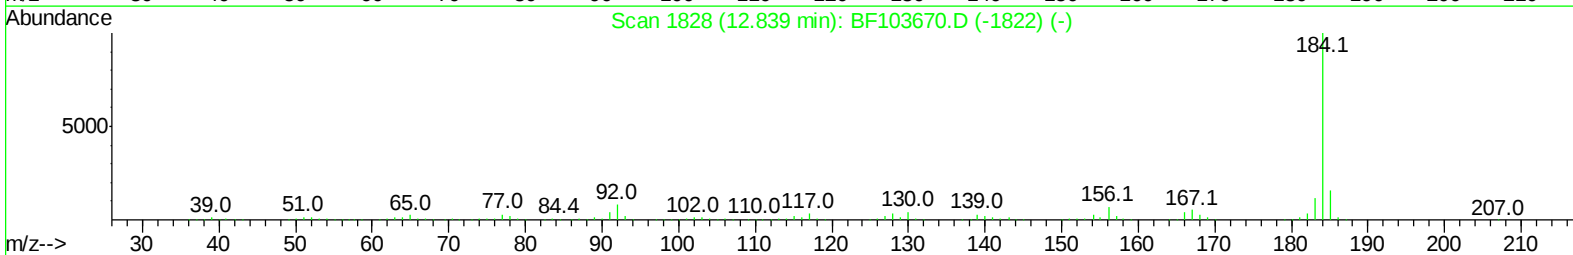
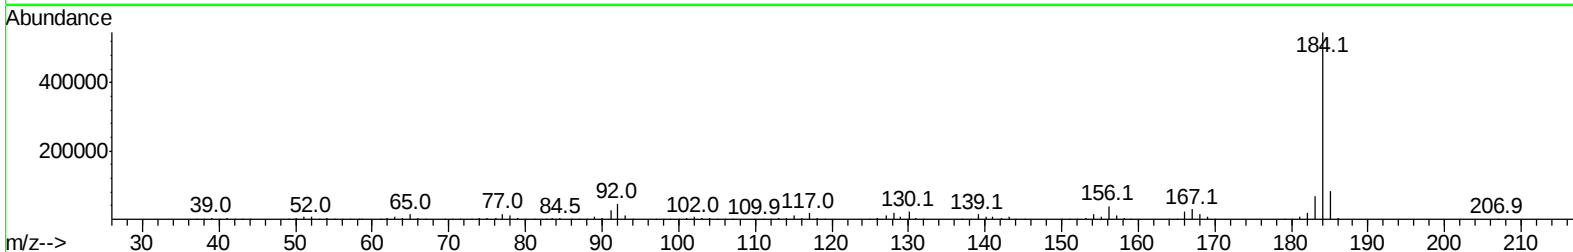


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF032018\
Data File : BF103824.D
Acq On : 21 Mar 2018 1:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 21 07:22:10 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 18:31:53 2018
Response via : Initial Calibration

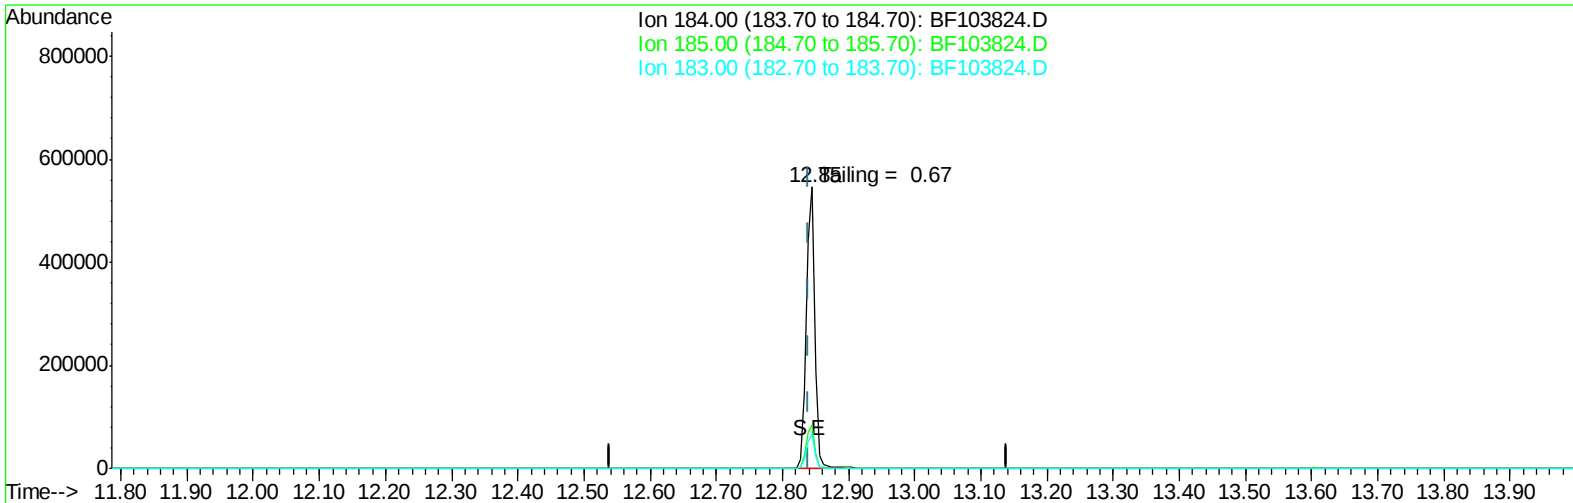

TIC: BF103824.D

(76) Benzidine

12.845min (+0.006) 0.00ng

response 495655

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.40
183.00	11.60	12.43
0.00	0.00	0.00