


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF032018\
 Data File : BF103798.D
 Acq On : 20 Mar 2018 13:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 15 18:31:53 2018

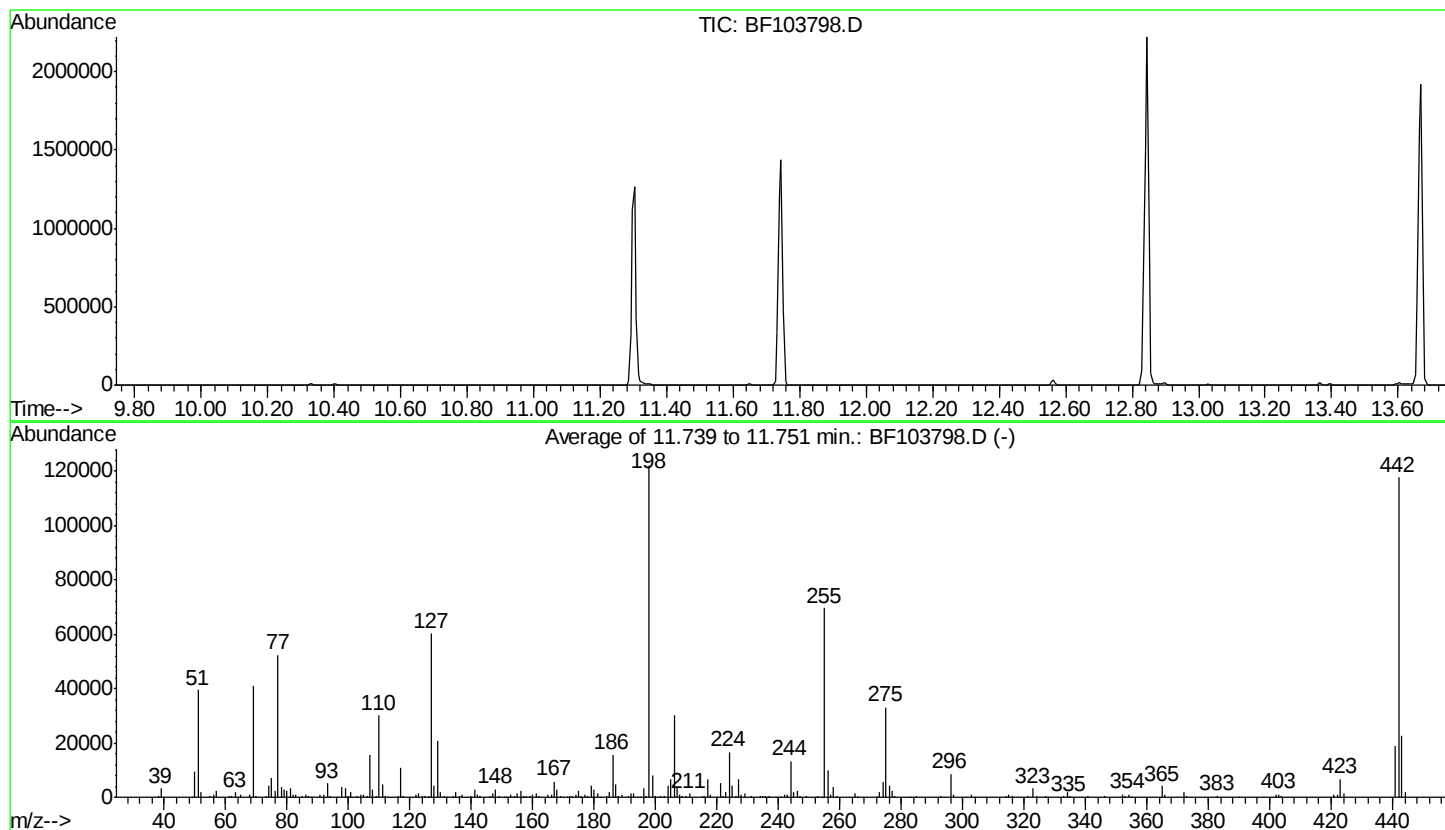

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	39586	PASS
68	69	0.00	2	1.8	731	PASS
69	198	0.00	100	33.4	40793	PASS
70	69	0.00	2	0.6	261	PASS
127	198	10	80	49.3	60184	PASS
197	198	0.00	2	0.5	671	PASS
198	198	100	100	100.0	122120	PASS
199	198	5	9	6.6	8116	PASS
275	198	10	60	27.1	33088	PASS
365	198	1	100	3.4	4151	PASS
441	443	0.01	100	83.0	18683	PASS
442	198	50	100	96.4	117690	PASS
443	442	15	24	19.1	22517	PASS