
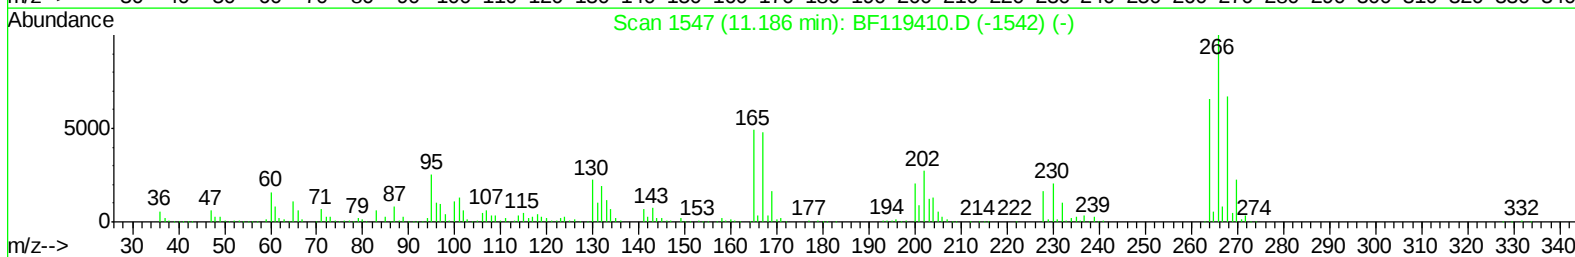
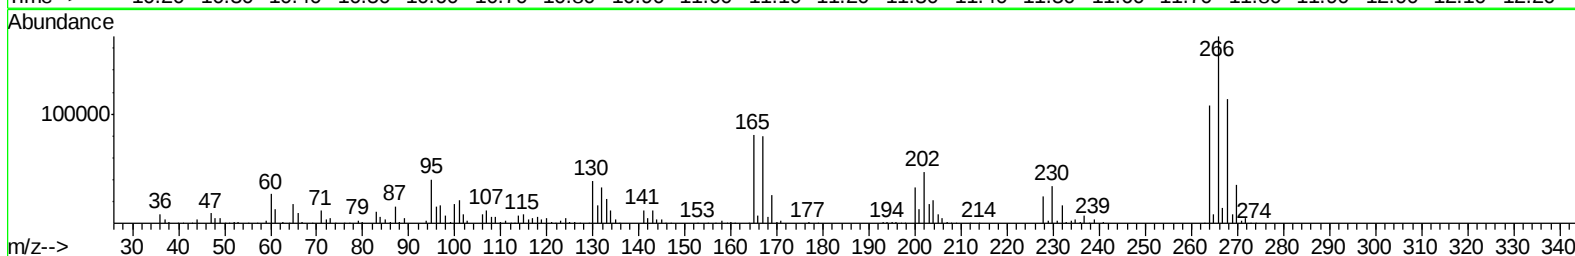


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032020\
Data File : BF119464.D
Acq On : 20 Mar 2020 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 23:16:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 18 15:11:18 2020
Response via : Initial Calibration

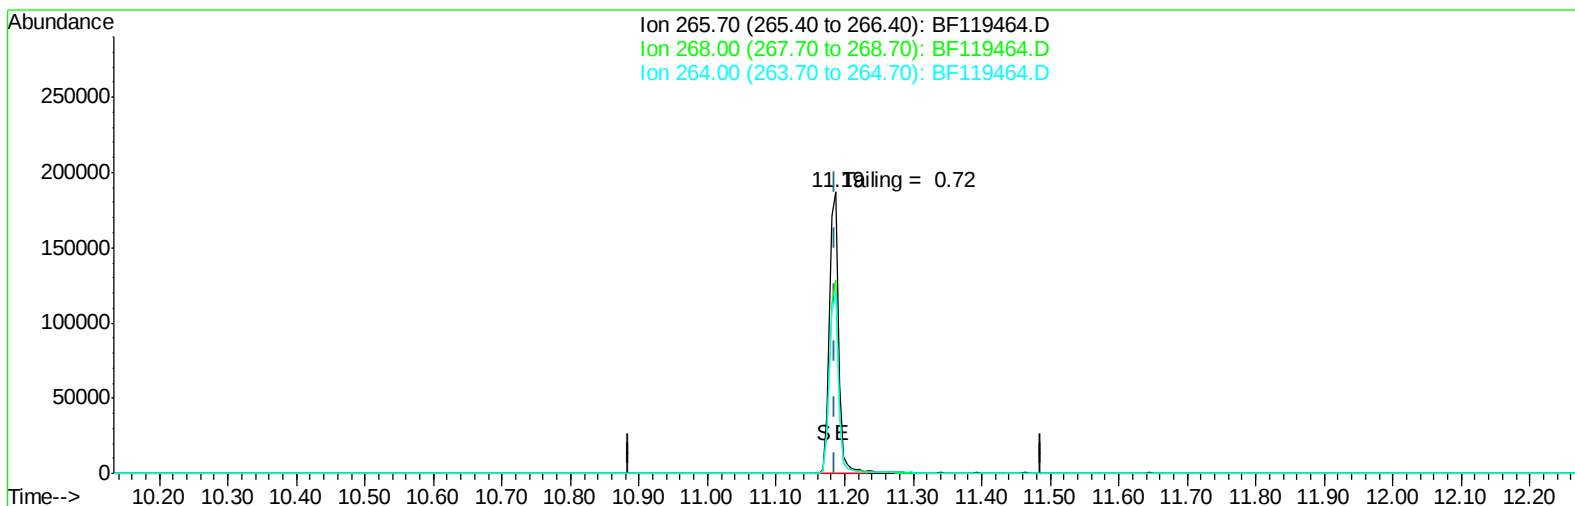

TIC: BF119464.D

(70) Pentachlorophenol (C)




11.186min (+0.000) 46465.97ng

response 174032

Ion	Exp%	Act%
265.70	100	100
268.00	67.10	68.69
264.00	65.60	63.94
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032020\
 Data File : BF119464.D
 Acq On : 20 Mar 2020 9:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 20 23:16:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 18 15:11:18 2020
 Response via : Initial Calibration

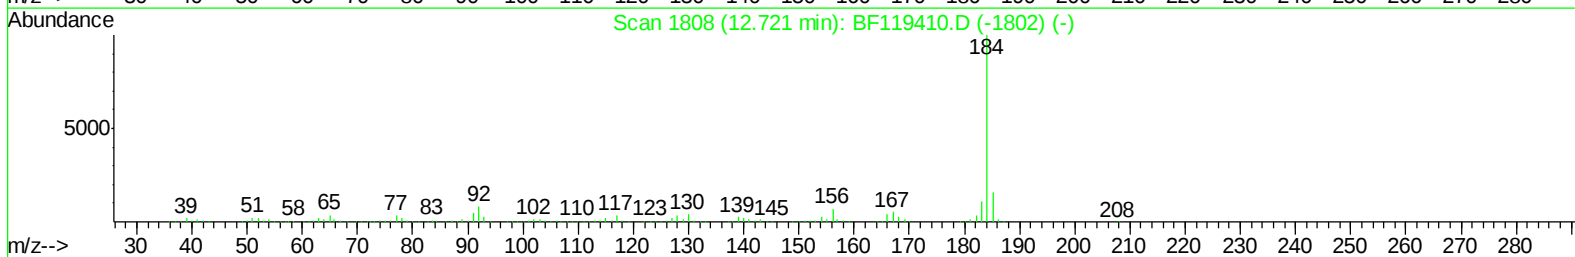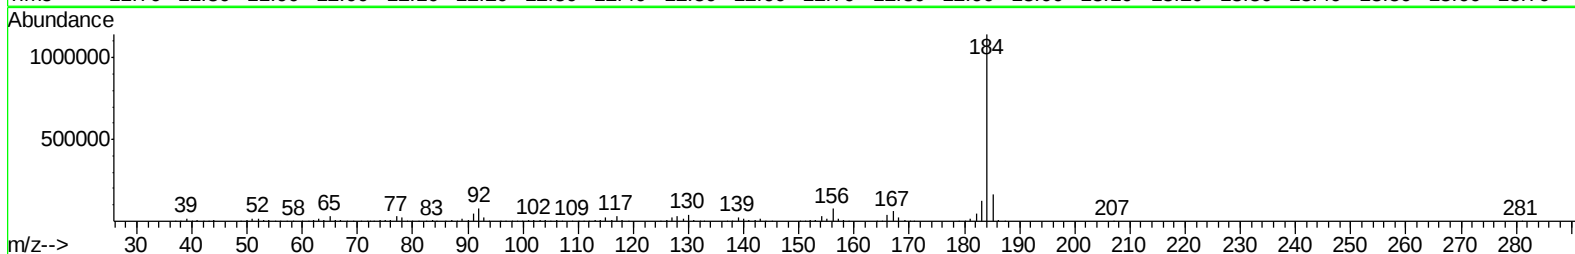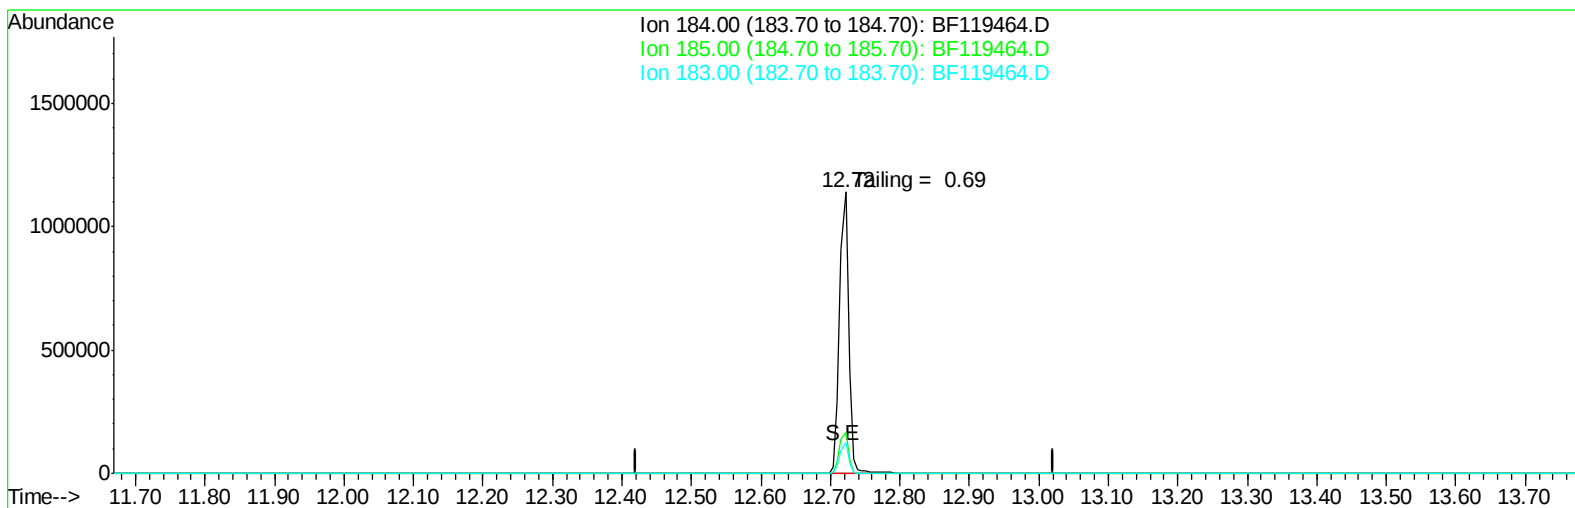

TIC: BF119464.D

(77) Benzidine

12.721min (-12.721) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	16.10	0.00#
183.00	11.20	0.00#
0.00	0.00	0.00