


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032020\
 Data File : BF119464.D
 Acq On : 20 Mar 2020 9:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 18 15:11:18 2020

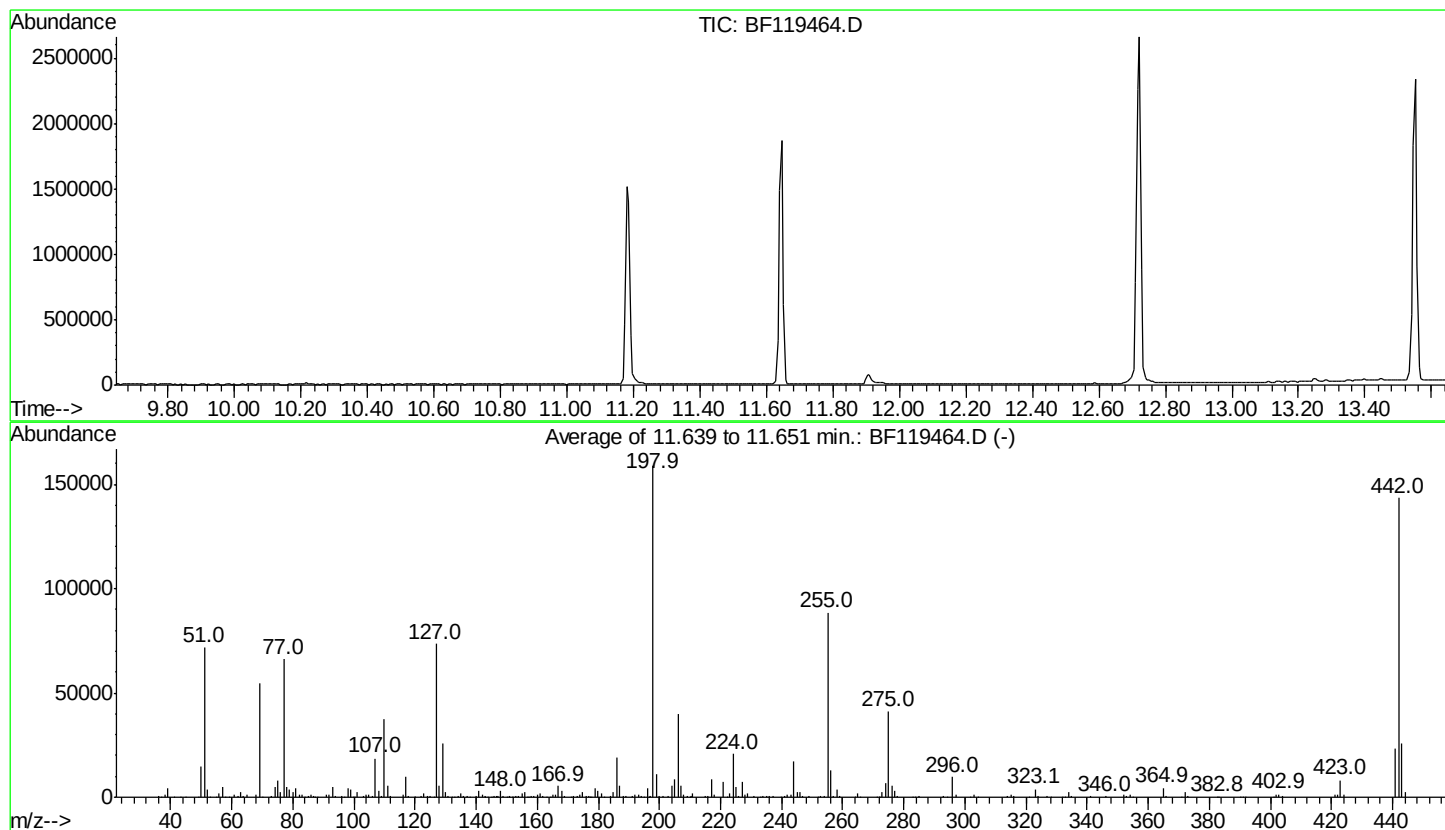

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	71530	PASS
68	69	0.00	2	1.7	945	PASS
69	198	0.00	100	34.2	54383	PASS
70	69	0.00	2	0.3	174	PASS
127	198	10	80	46.3	73568	PASS
197	198	0.00	2	0.5	807	PASS
198	198	100	100	100.0	158925	PASS
199	198	5	9	6.8	10844	PASS
275	198	10	60	25.9	41090	PASS
365	198	1	100	2.8	4451	PASS
441	198	0.01	100	14.8	23468	PASS
442	198	50	100	90.3	143541	PASS
443	442	15	24	18.0	25869	PASS